

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070822\
 Data File : VV026702.D
 Acq On : 08 Jul 2022 17:34
 Operator : SY/MD
 Sample : N3601-18 50X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUB0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV026702.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.323	80	88	102	rBV	79358	92460	17.69%	2.166%
2	1.584	162	169	182	rVB	79800	91614	17.53%	2.146%
3	2.121	327	336	357	rVB	153096	221552	42.39%	5.190%
4	2.523	449	461	480	rBV	18767	33111	6.34%	0.776%
5	3.931	887	899	929	rBV3	38875	151818	29.05%	3.557%
6	4.365	1018	1034	1055	rBV2	105047	257706	49.31%	6.037%
7	5.059	1232	1250	1282	rBV2	209905	522636	100.00%	12.243%
8	5.625	1414	1426	1460	rBV	196274	402666	77.05%	9.433%
9	5.931	1506	1521	1530	rBV8	5728	12469	2.39%	0.292%
10	6.079	1553	1567	1592	rBV	124182	259826	49.71%	6.087%
11	6.995	1841	1852	1869	rBV2	35322	67399	12.90%	1.579%
12	7.320	1942	1953	1972	rBV	206445	367577	70.33%	8.611%
13	7.632	2036	2050	2067	rBV3	17469	34294	6.56%	0.803%
14	7.982	2152	2159	2171	rVB7	4655	8042	1.54%	0.188%
15	8.098	2184	2195	2232	rBV2	155241	390415	74.70%	9.146%
16	8.853	2418	2430	2458	rBV	290578	485664	92.93%	11.377%
17	10.217	2843	2854	2870	rBV	93156	150403	28.78%	3.523%
18	11.249	3164	3175	3195	rBV	248540	385166	73.70%	9.023%
19	11.622	3280	3291	3314	rBV	199634	320605	61.34%	7.511%
20	13.503	3867	3876	3890	rVB2	4014	6979	1.34%	0.163%
21	13.744	3941	3951	3963	rBV5	3900	6286	1.20%	0.147%




Sum of corrected areas: 4268688

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070822\
Data File : VV026702.D
Acq On : 08 Jul 2022 17:34
Operator : SY/MD
Sample : N3601-18 50X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUB0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

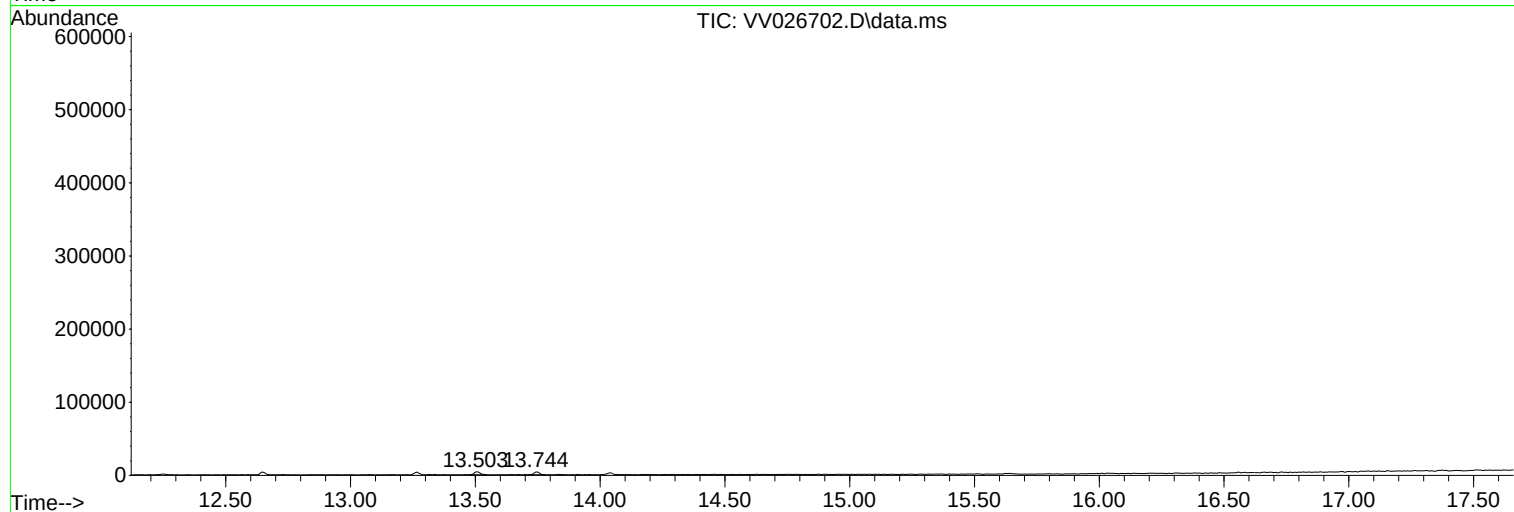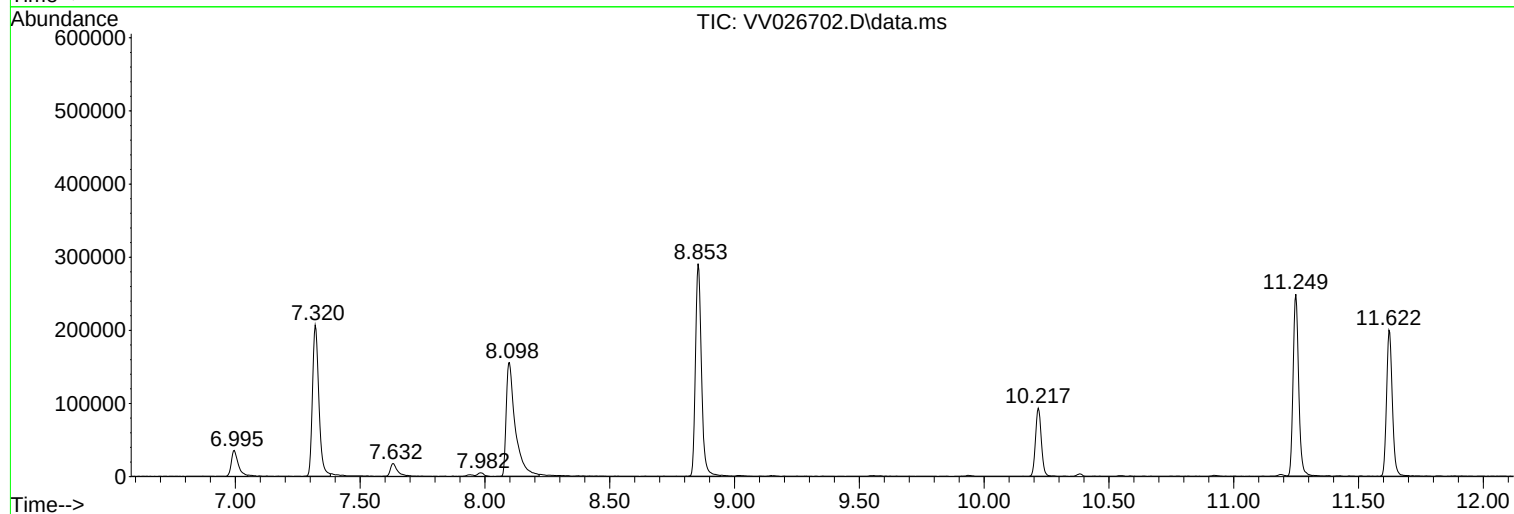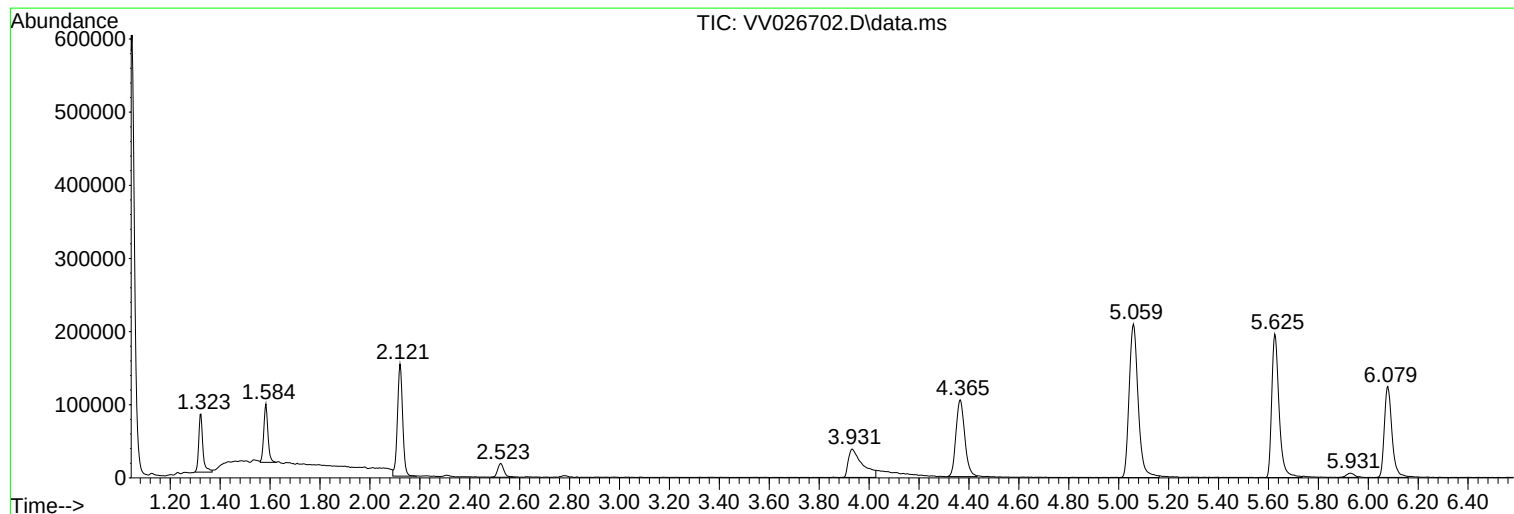

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070822\
Data File : VV026702.D
Acq On : 08 Jul 2022 17:34
Operator : SY/MD
Sample : N3601-18 50X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUB0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070822\
Data File : VV026702.D
Acq On : 08 Jul 2022 17:34
Operator : SY/MD
Sample : N3601-18 50X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUB0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc