

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070822\
 Data File : VV026704.D
 Acq On : 08 Jul 2022 18:24
 Operator : SY/MD
 Sample : N3601-20 50X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUB3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026704.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.317	78	86	101	rBV	84683	97805	3.81%	1.067%
2	1.577	161	167	179	rVB	79313	91173	3.56%	0.995%
3	2.118	325	335	353	rVB	154294	235422	9.18%	2.569%
4	2.519	449	460	476	rVB	18166	30915	1.21%	0.337%
5	3.921	881	896	931	rBV	291513	779732	30.40%	8.508%
6	4.359	1016	1032	1058	rVB2	107358	263949	10.29%	2.880%
7	5.056	1228	1249	1280	rBV2	213765	535059	20.86%	5.839%
8	5.622	1411	1425	1455	rBV	204154	418175	16.31%	4.563%
9	5.918	1503	1517	1550	rBV	822659	1622835	63.28%	17.708%
10	6.076	1553	1566	1586	rVV	127446	262662	10.24%	2.866%
11	6.992	1837	1851	1880	rBV	36570	73601	2.87%	0.803%
12	7.320	1940	1953	1975	rBV	204820	371197	14.47%	4.051%
13	7.632	2040	2050	2068	rBV2	18644	35220	1.37%	0.384%
14	7.976	2138	2157	2184	rBV	1534409	2564589	100.00%	27.985%
15	8.095	2184	2194	2236	rVB2	172507	418980	16.34%	4.572%
16	8.854	2417	2430	2459	rBV	301014	505273	19.70%	5.514%
17	10.217	2843	2854	2869	rBV2	94856	154249	6.01%	1.683%
18	11.249	3163	3175	3192	rBV	251375	389523	15.19%	4.250%
19	11.622	3279	3291	3307	rBV	196850	313860	12.24%	3.425%




Sum of corrected areas: 9164219

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070822\
Data File : VV026704.D
Acq On : 08 Jul 2022 18:24
Operator : SY/MD
Sample : N3601-20 50X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUB3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

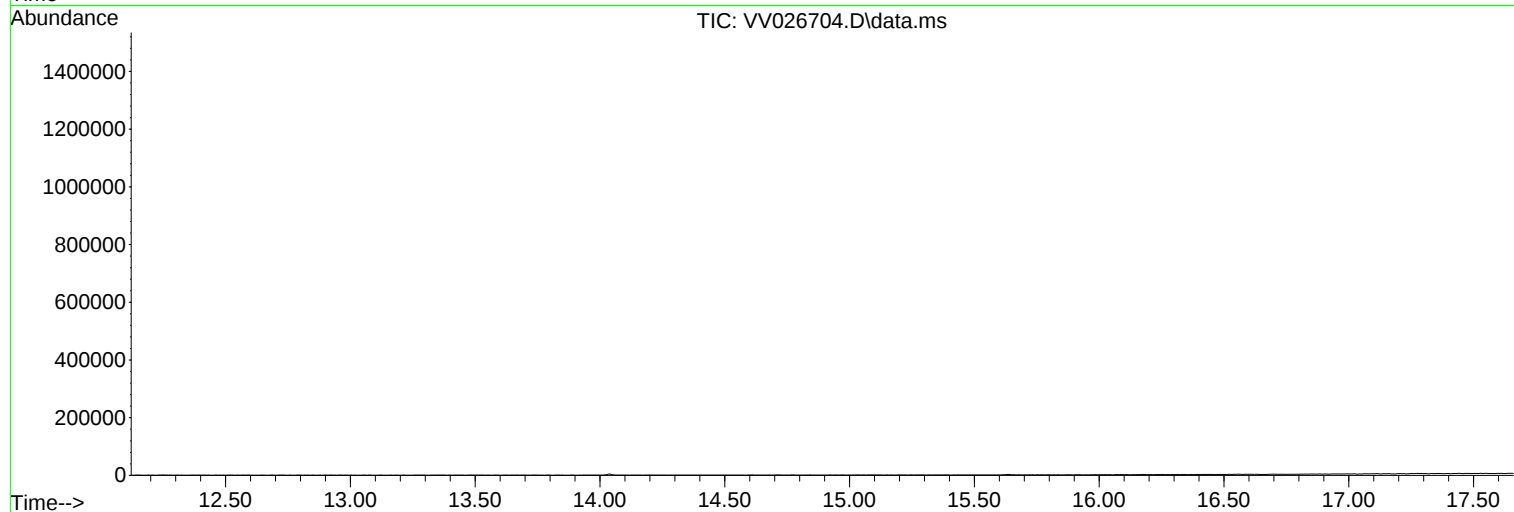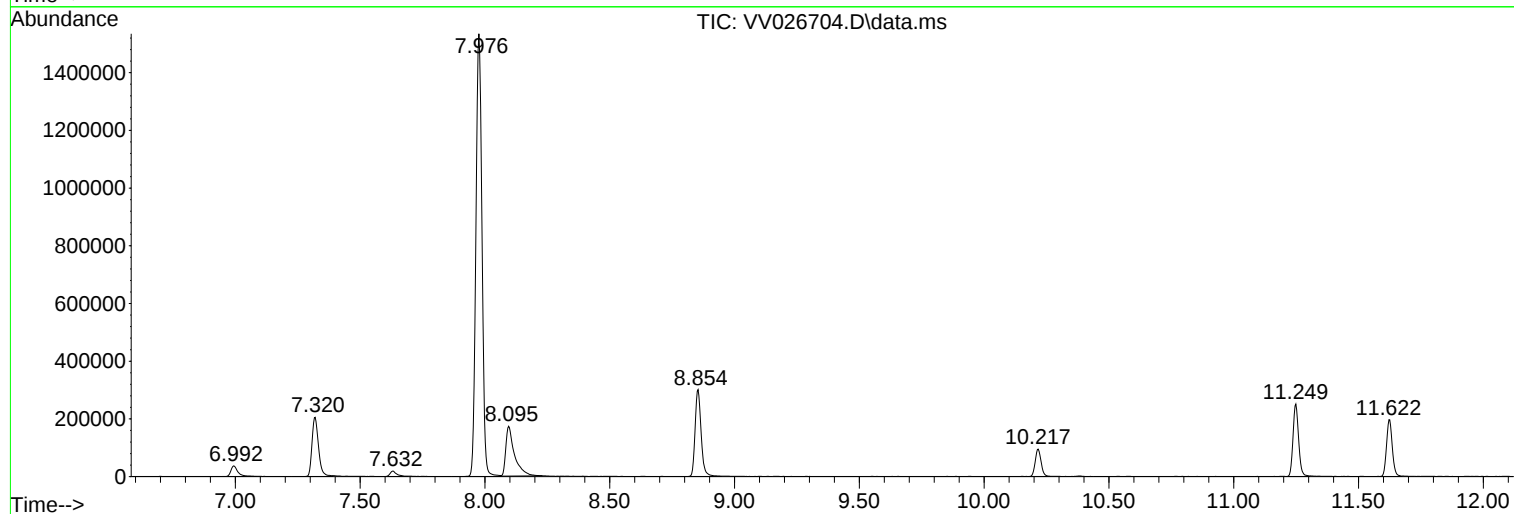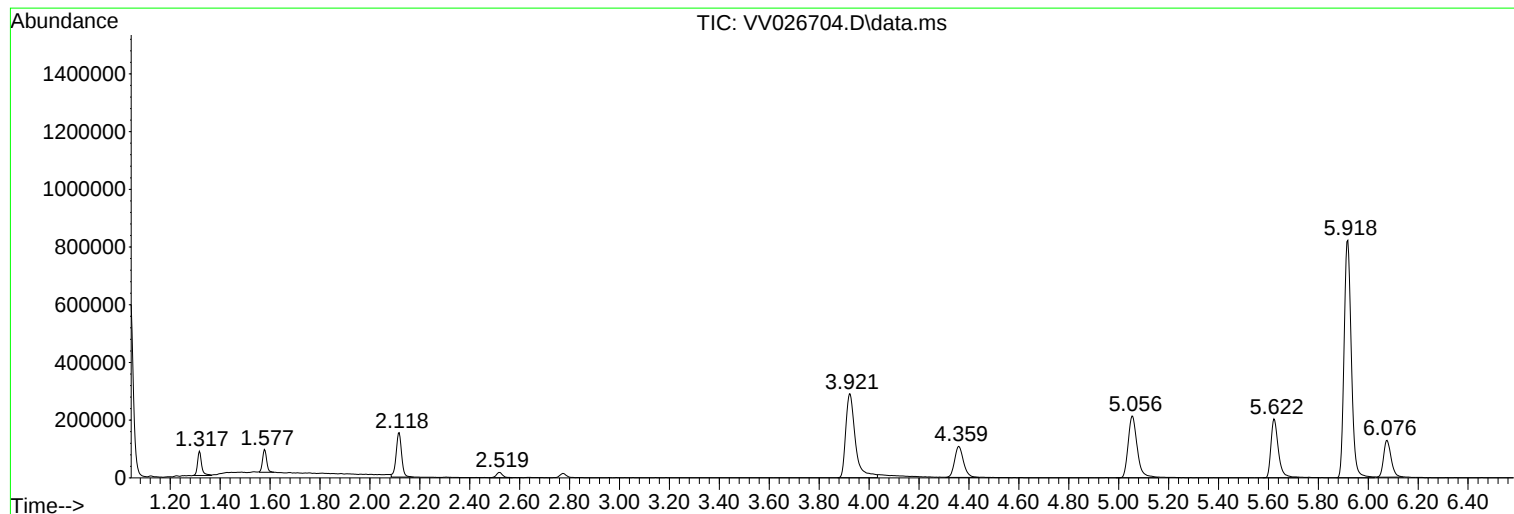

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070822\
Data File : VV026704.D
Acq On : 08 Jul 2022 18:24
Operator : SY/MD
Sample : N3601-20 50X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUB3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070822\
Data File : VV026704.D
Acq On : 08 Jul 2022 18:24
Operator : SY/MD
Sample : N3601-20 50X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUB3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------