

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070822\
 Data File : VV026705.D
 Acq On : 08 Jul 2022 18:48
 Operator : SY/MD
 Sample : N3601-21 50X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUB6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV026705.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.320	79	87	102	rBV	80832	91020	18.08%	2.190%
2	1.413	105	116	117	rBV6	9749	15883	3.16%	0.382%
3	1.580	162	168	185	rVB	77038	93275	18.53%	2.244%
4	2.121	327	336	354	rVB	148987	217479	43.20%	5.232%
5	2.523	451	461	477	rVB	15841	26814	5.33%	0.645%
6	3.931	887	899	934	rBV2	27310	125449	24.92%	3.018%
7	4.362	1017	1033	1059	rVB2	101066	251748	50.01%	6.057%
8	5.056	1234	1249	1277	rBV2	201996	503420	100.00%	12.112%
9	5.625	1414	1426	1451	rBV	193158	396127	78.69%	9.531%
10	5.928	1508	1520	1532	rBV9	5002	11419	2.27%	0.275%
11	6.075	1554	1566	1594	rBV	120716	254772	50.61%	6.130%
12	6.995	1842	1852	1870	rBV2	32697	63680	12.65%	1.532%
13	7.320	1941	1953	1975	rBV	201456	356640	70.84%	8.581%
14	7.632	2041	2050	2073	rBV	17338	33822	6.72%	0.814%
15	7.982	2151	2159	2171	rVB4	7157	11924	2.37%	0.287%
16	8.095	2182	2194	2236	rBV2	147210	379428	75.37%	9.129%
17	8.853	2419	2430	2463	rBV	294324	488306	97.00%	11.749%
18	10.217	2842	2854	2868	rBV	91104	146718	29.14%	3.530%
19	11.249	3163	3175	3196	rBV	247431	380140	75.51%	9.146%
20	11.622	3277	3291	3313	rBV	189161	301836	59.96%	7.262%
21	14.040	4033	4043	4053	rBV2	4063	6425	1.28%	0.155%




Sum of corrected areas: 4156325

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070822\
Data File : VV026705.D
Acq On : 08 Jul 2022 18:48
Operator : SY/MD
Sample : N3601-21 50X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUB6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

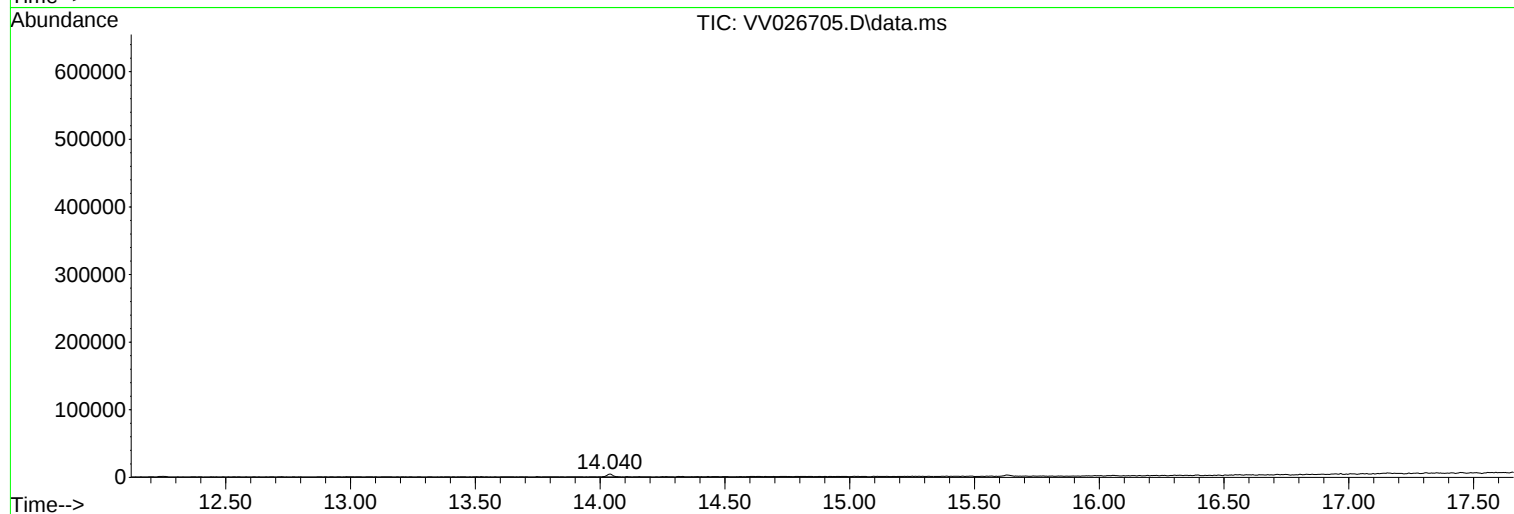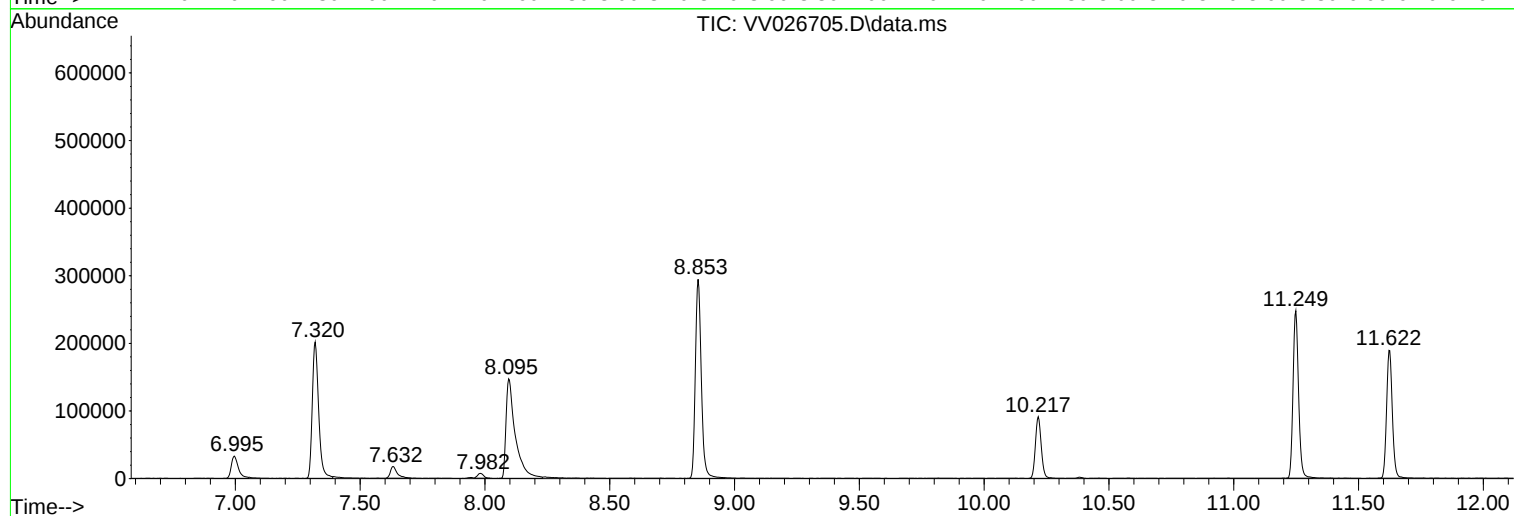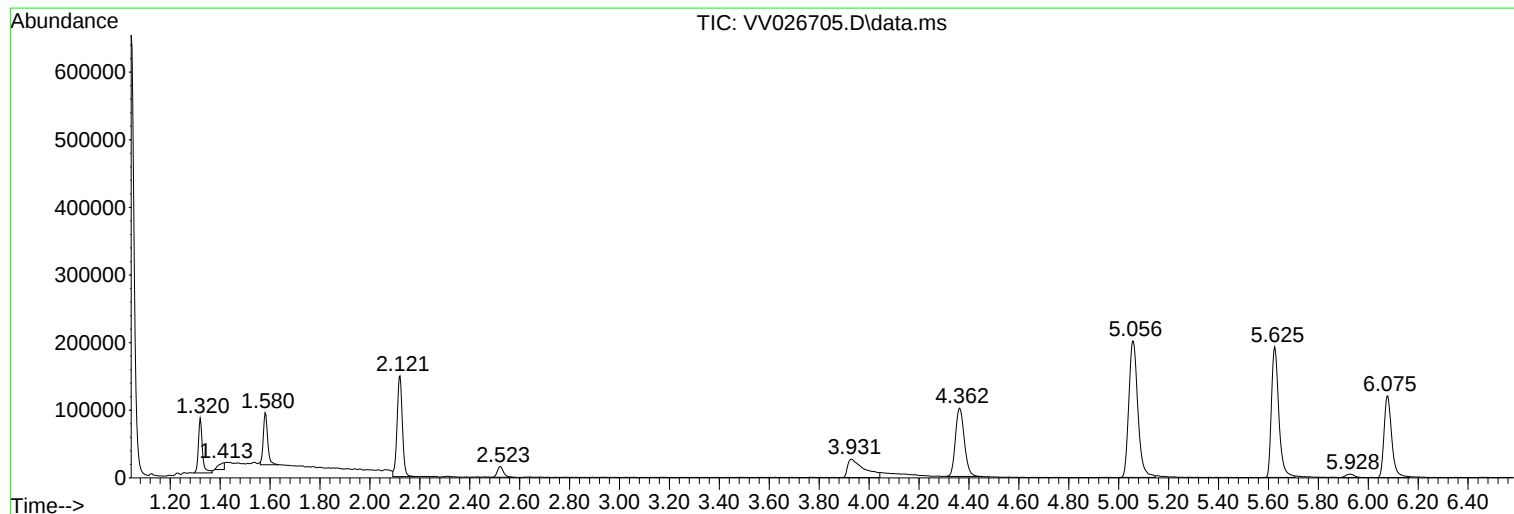

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070822\
Data File : VV026705.D
Acq On : 08 Jul 2022 18:48
Operator : SY/MD
Sample : N3601-21 50X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUB6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070822\
Data File : VV026705.D
Acq On : 08 Jul 2022 18:48
Operator : SY/MD
Sample : N3601-21 50X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUB6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc