

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070822\
 Data File : VV026706.D
 Acq On : 08 Jul 2022 19:13
 Operator : SY/MD
 Sample : N3601-22 50X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUB7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV026706.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.230	44	59	63	rBV7	4226	7817	1.55%	0.189%
2	1.320	80	87	98	rBV	78025	84867	16.84%	2.054%
3	1.420	108	118	120	rBV3	7728	11908	2.36%	0.288%
4	1.584	162	169	180	rVB	76477	88600	17.58%	2.145%
5	2.121	327	336	355	rVB	148833	222329	44.11%	5.382%
6	2.523	451	461	472	rBV2	18411	30699	6.09%	0.743%
7	3.931	887	899	932	rBV3	27461	126859	25.17%	3.071%
8	4.362	1016	1033	1056	rBV	103193	254951	50.58%	6.172%
9	5.060	1234	1250	1280	rBV3	203665	504047	100.00%	12.202%
10	5.625	1414	1426	1448	rBV	192197	395140	78.39%	9.565%
11	5.928	1510	1520	1529	rBV8	3949	7907	1.57%	0.191%
12	6.076	1553	1566	1591	rBV	122344	256528	50.89%	6.210%
13	6.995	1841	1852	1876	rBV	33059	64628	12.82%	1.565%
14	7.320	1941	1953	1971	rBV	198542	349867	69.41%	8.470%
15	7.632	2041	2050	2066	rBV3	17235	33203	6.59%	0.804%
16	8.095	2184	2194	2224	rBV2	149050	374234	74.25%	9.059%
17	8.854	2419	2430	2456	rBV	292976	482377	95.70%	11.677%
18	10.217	2842	2854	2870	rBV	91620	147390	29.24%	3.568%
19	11.249	3164	3175	3197	rBV	242489	377765	74.95%	9.145%
20	11.622	3280	3291	3310	rBV	190377	303669	60.25%	7.351%
21	14.037	4032	4042	4053	rBV	3774	6106	1.21%	0.148%




Sum of corrected areas: 4130891

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070822\
Data File : VV026706.D
Acq On : 08 Jul 2022 19:13
Operator : SY/MD
Sample : N3601-22 50X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUB7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

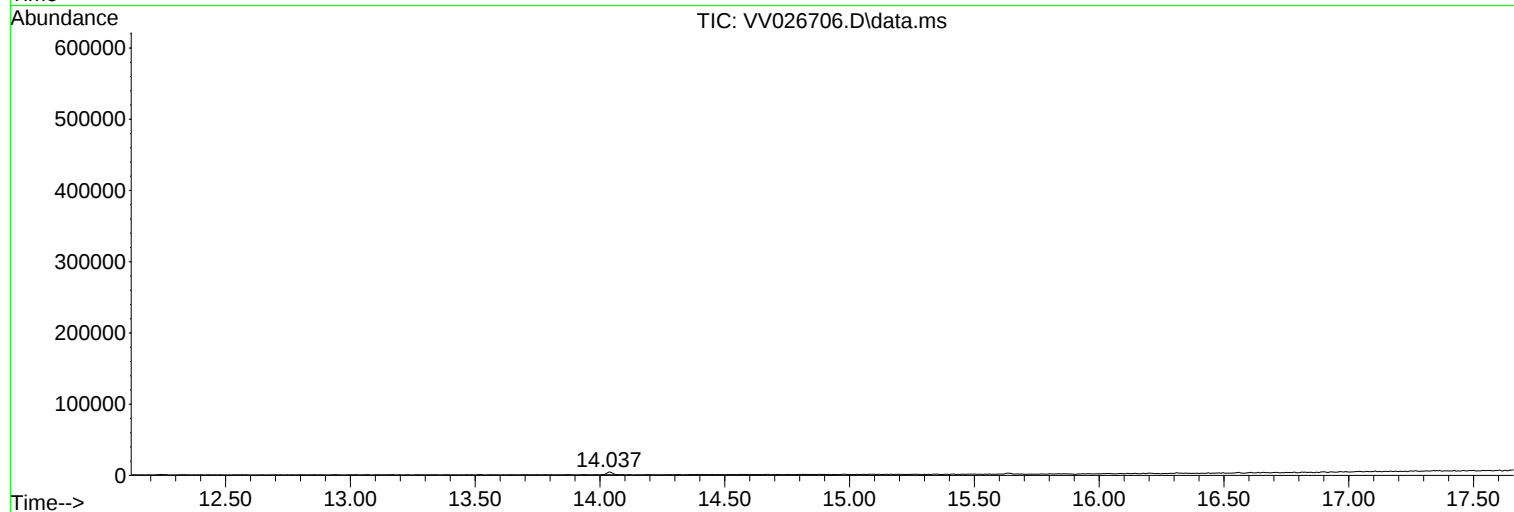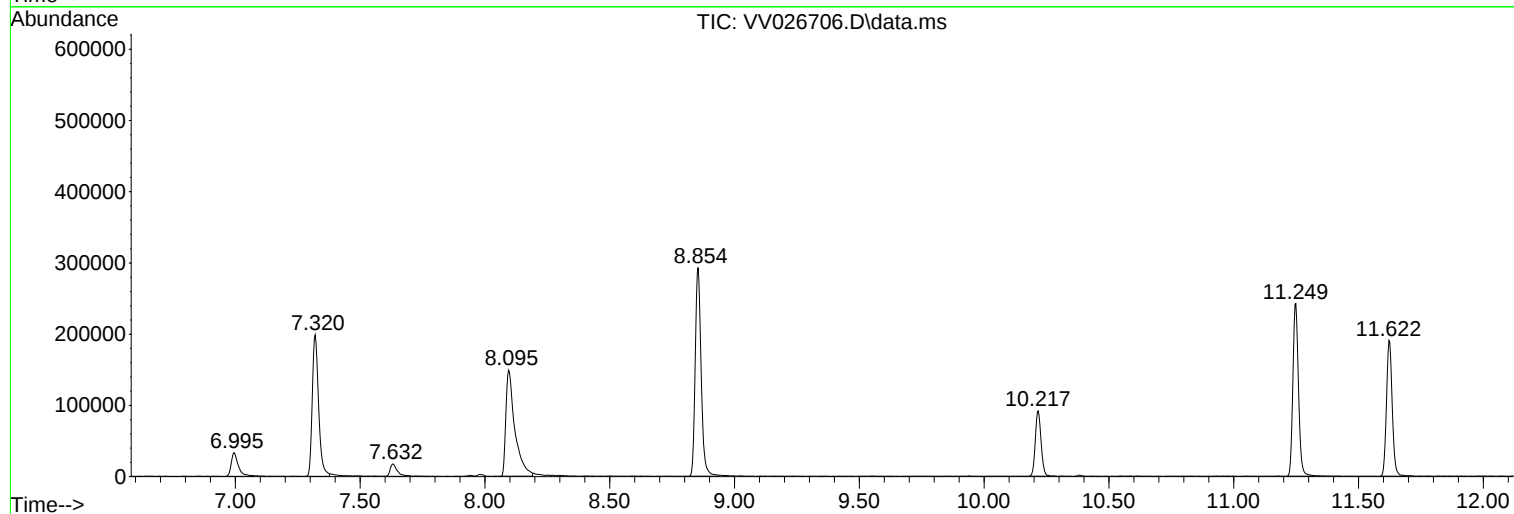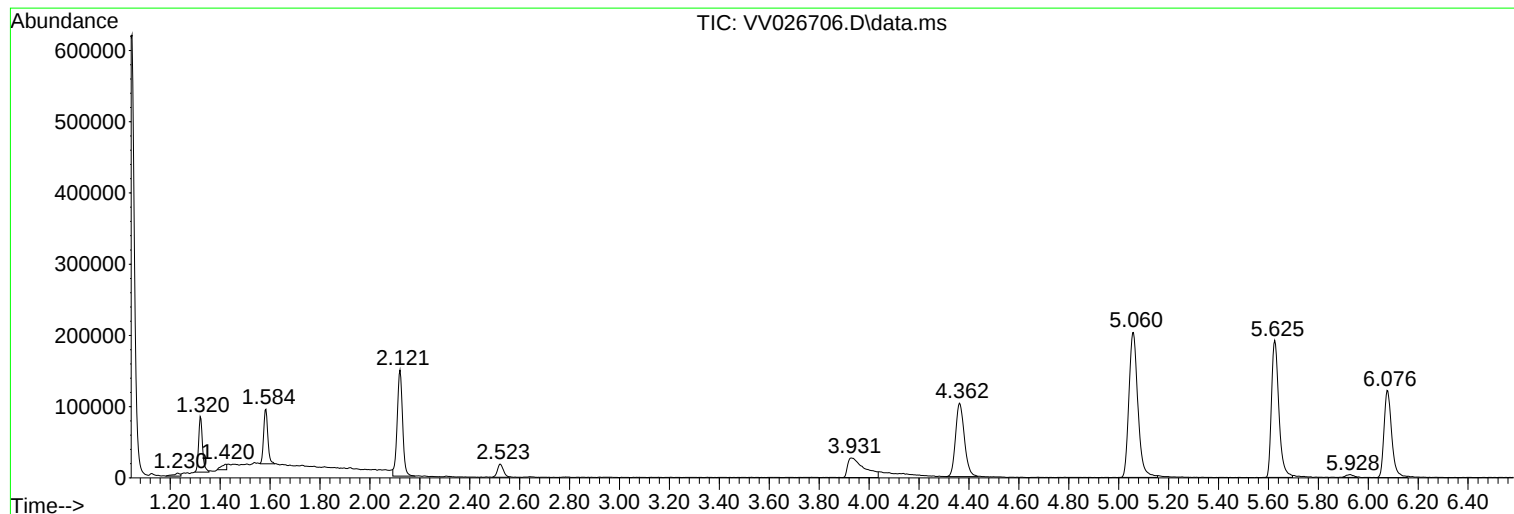

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070822\
Data File : VV026706.D
Acq On : 08 Jul 2022 19:13
Operator : SY/MD
Sample : N3601-22 50X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUB7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070822\
Data File : VV026706.D
Acq On : 08 Jul 2022 19:13
Operator : SY/MD
Sample : N3601-22 50X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUB7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc