


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070822\
 Data File : VV026687.D
 Acq On : 08 Jul 2022 09:31
 Operator : SY/MD
 Sample : BFB341
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB341

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Fri Jul 08 23:50:05 2022

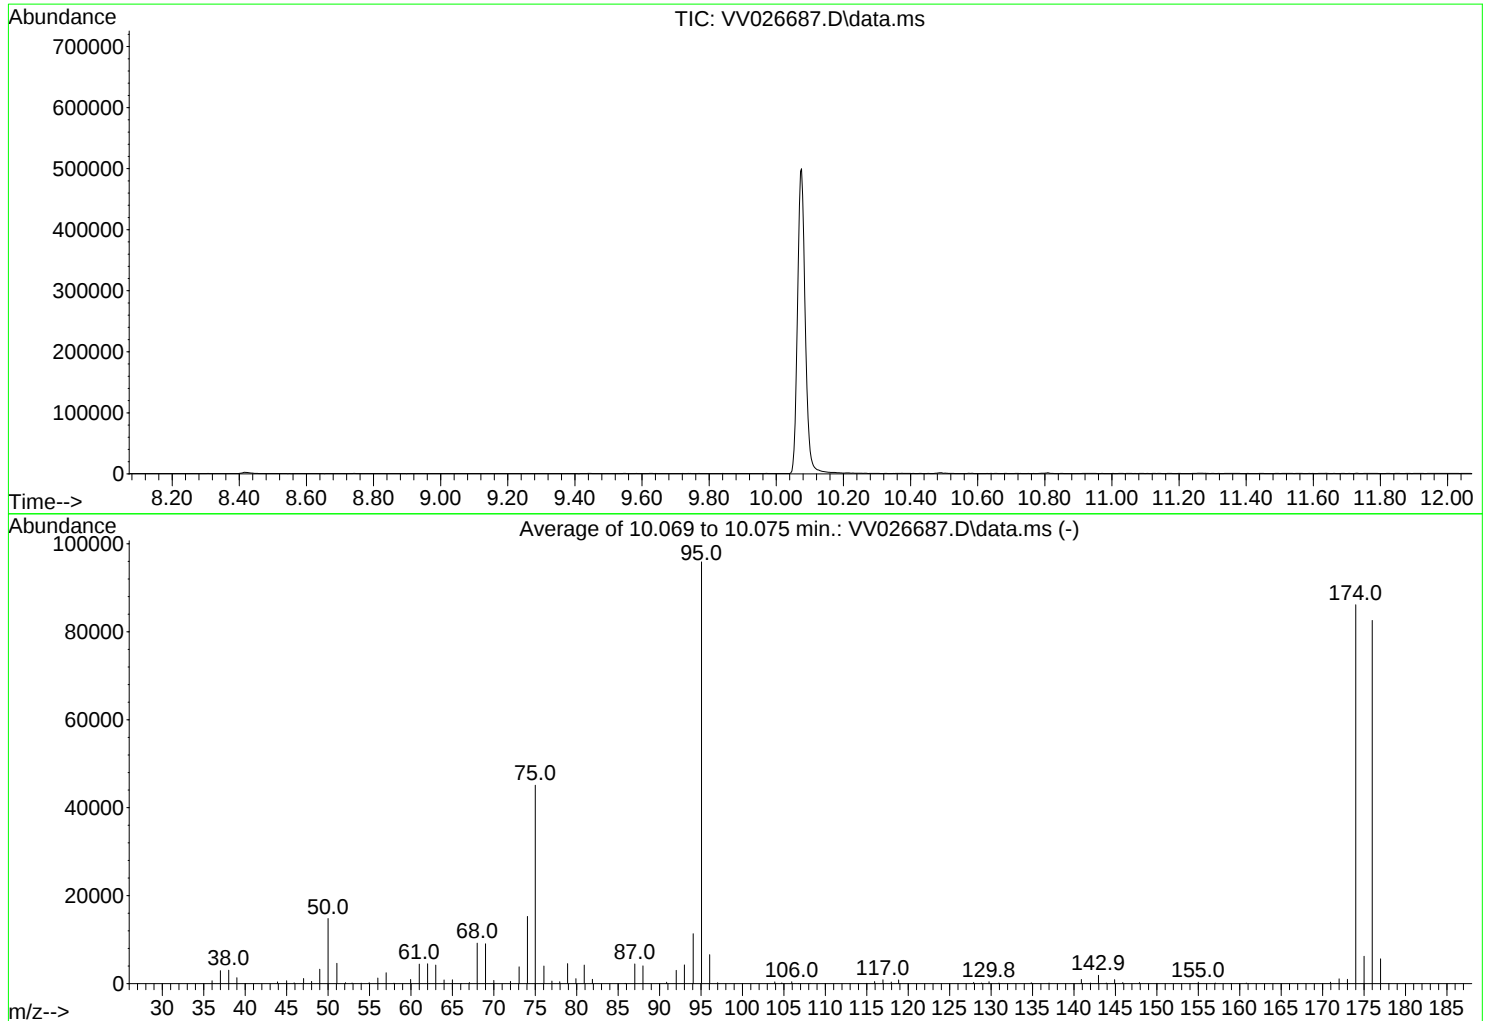

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.4	14805	PASS
75	95	30	80	47.0	45120	PASS
95	95	100	100	100.0	95899	PASS
96	95	5	9	6.9	6570	PASS
173	174	0.00	2	1.2	997	PASS
174	95	50	120	89.8	86131	PASS
175	174	5	9	7.2	6237	PASS
176	174	95	105	95.9	82568	PASS
177	176	5	10	6.8	5641	PASS

m/z	Abundance
40.10	236.0
43.90	358.0

Instrument :
MSVOA_V
ClientSampleId :
BFB341

m/z	Abundance
36.00	615.0
37.00	2871.0
38.00	2909.0
39.00	1225.0
40.10	215.0
44.00	821.0
45.00	629.0
45.90	198.0
47.10	1014.0
48.00	484.0
49.00	3092.0
50.00	14004.0
51.00	4373.0
52.10	228.0
52.90	102.0
54.00	104.0
55.00	195.0
56.00	1229.0
57.00	2179.0
57.90	114.0
60.00	911.0
61.00	4180.0
62.00	4182.0
63.00	4018.0
64.00	792.0
65.00	841.0
67.10	227.0
68.00	8605.0
69.00	8355.0
70.00	744.0
72.00	469.0
73.10	3631.0
74.10	14072.0
75.00	41728.0
76.00	3767.0
77.00	515.0
78.00	434.0
78.90	4152.0
79.90	994.0
80.90	3906.0
81.90	891.0
87.00	4117.0
88.00	3814.0
90.80	292.0
92.00	2862.0
93.00	3872.0
94.00	10471.0
95.00	89072.0
96.10	6366.0
97.00	193.0
103.90	401.0
104.80	194.0
105.90	410.0
116.00	430.0
116.90	866.0
118.00	311.0
118.90	752.0
127.90	299.0
128.80	125.0
129.80	427.0
131.00	113.0
134.90	224.0
136.90	138.0
140.90	829.0
142.00	105.0
143.00	1746.0
143.90	144.0
144.90	890.0
145.90	189.0
147.90	242.0
155.00	255.0
157.00	136.0
160.80	176.0
171.00	318.0
171.90	981.0
173.00	934.0
174.00	77680.0
175.00	5670.0
176.00	74344.0
177.00	5246.0

Instrument :
MSVOA_V
ClientSampleId :
BFB341

m/z	Abundance
36.00	710.0
37.00	3024.0
38.00	3164.0
39.00	1357.0
40.10	290.0
44.00	771.0
45.00	672.0
45.90	198.0
47.10	1200.0
48.00	525.0
49.00	3404.0
50.00	15164.0
51.10	4770.0
52.10	213.0
52.90	134.0
54.00	130.0
55.00	219.0
56.00	1290.0
57.00	2557.0
58.00	103.0
60.00	986.0
61.00	4585.0
62.00	4755.0
63.00	4401.0
64.00	840.0
65.00	894.0
67.00	264.0
68.00	9590.0
69.00	9425.0
70.00	762.0
72.00	535.0
73.00	3894.0
74.00	15788.0
75.00	46736.0
76.10	4173.0
77.00	593.0
77.90	437.0
78.90	4743.0
79.90	1165.0
80.90	4368.0
81.90	993.0
85.90	114.0
87.00	4636.0
88.00	4174.0
90.90	323.0
92.00	3177.0
93.00	4430.0
94.10	11798.0
95.00	99456.0
96.10	6826.0
97.00	248.0
103.90	406.0
104.80	182.0
106.00	450.0
108.10	108.0
115.00	115.0
115.90	483.0
117.00	895.0
117.90	405.0
118.80	870.0
127.90	274.0
128.90	149.0
129.70	490.0
131.00	142.0
134.90	221.0
137.00	155.0
140.90	971.0
142.00	155.0
142.90	1986.0
143.90	179.0
144.90	920.0
145.90	270.0
147.90	268.0
150.00	102.0
155.00	353.0
157.10	161.0
159.00	105.0
160.80	154.0
171.00	338.0
172.00	1178.0
173.00	1015.0
174.00	89288.0
175.00	6412.0
176.00	85520.0
177.00	5898.0

Instrument :
MSVOA_V
ClientSampleId :
BFB341

m/z	Abundance
36.00	691.0
37.00	2987.0
38.00	3125.0
39.00	1472.0
40.00	358.0
43.90	716.0
45.00	630.0
45.90	146.0
47.00	1237.0
48.00	489.0
49.00	3315.0
50.00	15247.0
51.10	4670.0
52.10	207.0
52.90	160.0
54.00	155.0
54.90	218.0
56.00	1271.0
57.00	2688.0
58.00	131.0
59.90	946.0
61.00	4567.0
62.00	4631.0
63.00	4263.0
64.00	871.0
65.00	937.0
66.10	100.0
67.00	275.0
68.00	9368.0
69.00	9414.0
70.00	673.0
72.00	564.0
73.00	3956.0
74.00	15952.0
75.00	46896.0
76.10	4080.0
77.00	595.0
77.90	413.0
78.90	4725.0
79.90	1257.0
80.90	4361.0
81.90	1039.0
85.80	172.0
87.00	4701.0
88.00	4090.0
90.90	365.0
92.00	3019.0
93.00	4512.0
94.10	11817.0
95.10	99168.0
96.00	6518.0
97.00	271.0
103.90	378.0
104.70	169.0
106.00	469.0
106.80	105.0
108.20	122.0
113.00	103.0
115.00	111.0
115.90	475.0
117.00	898.0
117.90	414.0
118.90	902.0
127.90	271.0
128.90	178.0
129.80	444.0
130.90	171.0
134.80	168.0
137.10	159.0
140.90	1055.0
142.00	160.0
143.00	1970.0
143.90	173.0
144.90	928.0
145.90	291.0
147.90	226.0
150.00	116.0
155.00	376.0
157.10	175.0
158.90	126.0
160.80	115.0
170.90	305.0
172.10	1154.0
173.00	1043.0
174.00	91424.0
175.00	6628.0
176.00	87840.0
177.00	5780.0
178.00	108.0

Instrument :
MSVOA_V
ClientSampleId :
BFB341