


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV070918\
Data File : VV006558.D
Acq On : 09 Jul 2018 13:30
Operator : SY/MD
Sample : BFB62
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB62

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR070718WMA.M
Title : TRACE VOA SOM01.0
Last Update : Mon Jul 09 22:52:57 2018

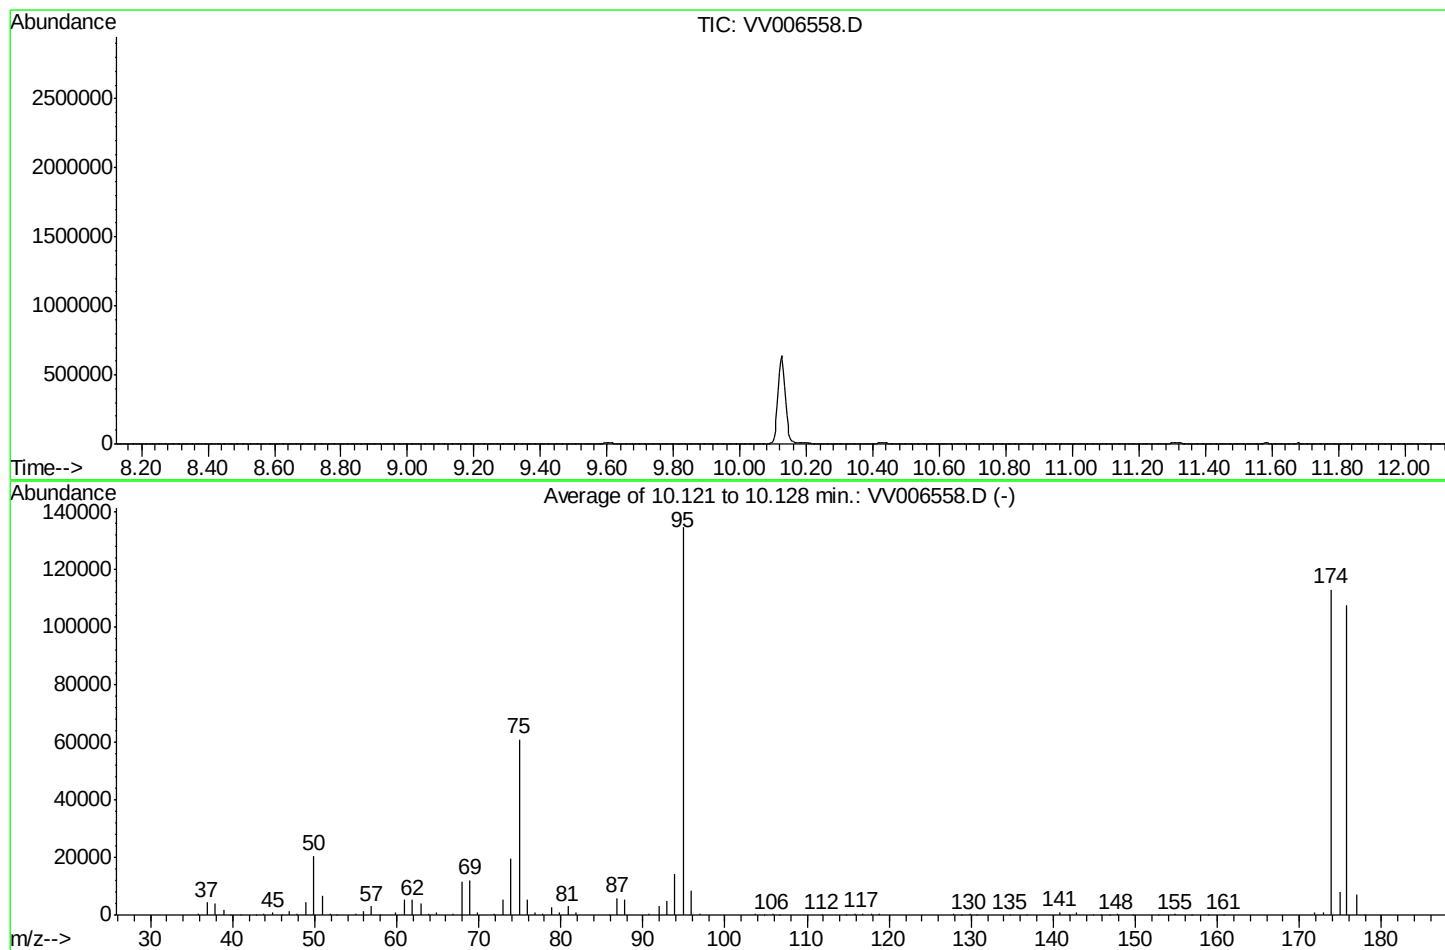

AutoFind: Scans 2871, 2872, 2873; Background Corrected with Scan 2858

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.3	20605	PASS
75	95	30	80	45.3	60925	PASS
95	95	100	100	100.0	134506	PASS
96	95	5	9	6.3	8449	PASS
173	174	0.00	2	0.8	902	PASS
174	95	50	120	83.9	112869	PASS
175	174	5	9	7.1	8067	PASS
176	174	95	101	95.2	107501	PASS
177	176	5	9	6.4	6918	PASS

Scan 2858 (10.080 min): VV006558.D
BFB62

m/z	Abundance
35.90	1316.0
36.90	104.0
37.80	557.0
39.70	219.0
43.90	675.0

Instrument :
MSVOA_V
ClientSampleId :
BFB62

m/z	Abundance
35.80	1912.0
36.90	4537.0
37.90	4344.0
38.90	1908.0
39.90	287.0
41.00	125.0
42.80	151.0
43.80	1254.0
44.90	835.0
46.90	1407.0
47.80	581.0
48.90	4233.0
49.90	20616.0
50.90	6443.0
52.00	357.0
55.00	296.0
55.90	1486.0
56.90	2957.0
57.90	105.0
59.90	1102.0
60.90	5109.0
61.90	5219.0
62.90	4098.0
63.90	510.0
64.90	784.0
66.90	311.0
67.90	11328.0
68.90	11856.0
69.90	922.0
71.80	612.0
72.90	5306.0
73.90	19544.0
74.90	60440.0
75.90	5167.0
76.90	848.0
77.70	704.0
78.80	2584.0
79.80	962.0
80.90	3093.0
81.80	717.0
86.00	172.0
86.90	5922.0
87.80	5305.0
90.80	395.0
91.90	3162.0
92.90	4979.0
93.90	13722.0
94.90	132928.0
95.90	8475.0
96.90	328.0
103.80	395.0
104.80	177.0
105.80	444.0
106.70	146.0
111.80	114.0
114.80	130.0
115.80	318.0
116.70	673.0
117.80	323.0
118.90	589.0
127.80	392.0
128.70	255.0
129.80	395.0
130.70	208.0
134.70	219.0
136.70	183.0
140.80	979.0
141.90	129.0
142.80	952.0
144.80	177.0
145.80	204.0
147.80	252.0
149.70	137.0
154.90	256.0
156.80	217.0
158.90	133.0
160.80	113.0
171.90	1017.0
172.90	852.0
173.90	108056.0
174.90	7890.0
175.80	102320.0
176.90	6769.0
177.90	166.0

Instrument :
MSVOA_V
ClientSampleId :
BFB62

m/z	Abundance
35.90	1946.0
36.90	4713.0
37.90	4553.0
38.90	1889.0
39.90	297.0
41.00	128.0
42.80	138.0
43.80	1220.0
44.90	878.0
45.90	105.0
46.90	1495.0
47.80	602.0
48.90	4430.0
49.90	21344.0
50.90	6754.0
51.90	335.0
52.70	105.0
54.90	328.0
55.90	1595.0
56.90	3047.0
57.90	113.0
59.90	1094.0
60.90	5348.0
61.90	5451.0
62.90	4226.0
63.90	551.0
64.90	884.0
66.90	279.0
67.90	11926.0
68.90	12428.0
69.90	888.0
71.80	644.0
72.90	5492.0
73.90	19936.0
74.90	63008.0
75.90	5293.0
76.90	882.0
77.80	704.0
78.80	2819.0
79.80	1056.0
80.80	3186.0
81.80	733.0
86.00	215.0
86.90	6065.0
87.80	5531.0
90.80	380.0
91.90	3307.0
92.90	5260.0
93.90	14860.0
94.90	139072.0
95.90	8733.0
96.90	312.0
103.70	424.0
104.80	179.0
105.80	441.0
106.70	169.0
111.90	109.0
114.80	138.0
115.80	336.0
116.80	699.0
117.80	351.0
118.90	591.0
127.80	392.0
128.80	234.0
129.80	448.0
130.70	237.0
134.70	219.0
136.70	184.0
140.80	1078.0
141.90	133.0
142.80	1052.0
144.90	193.0
145.80	215.0
146.80	103.0
147.80	266.0
149.70	135.0
152.80	107.0
154.90	295.0
156.80	219.0
158.90	140.0
160.80	120.0
171.90	1013.0
172.80	933.0
173.90	116560.0
174.90	8346.0
175.80	111200.0
176.90	7145.0
177.90	176.0

Instrument :
MSVOA_V
ClientSampleId :
BFB62

m/z	Abundance
35.90	1945.0
36.90	4378.0
37.90	4329.0
38.90	1686.0
39.90	300.0
41.00	110.0
42.80	129.0
43.80	1092.0
44.90	847.0
46.00	127.0
46.90	1485.0
47.80	649.0
48.90	4184.0
49.90	19856.0
50.90	6420.0
51.90	281.0
52.70	107.0
54.90	333.0
55.90	1536.0
56.90	2834.0
57.90	117.0
59.90	1005.0
60.90	5073.0
61.90	5100.0
62.90	3933.0
63.90	551.0
64.90	854.0
66.90	250.0
67.90	11320.0
68.90	11932.0
69.90	768.0
71.90	585.0
72.90	5101.0
73.90	18672.0
74.90	59328.0
75.90	4948.0
76.90	848.0
77.80	600.0
78.80	2716.0
79.80	1010.0
80.80	2880.0
81.80	716.0
85.90	207.0
86.90	5512.0
87.80	5279.0
90.80	356.0
91.90	3203.0
92.90	5063.0
93.90	14501.0
94.90	131520.0
96.00	8139.0
96.90	252.0
103.70	390.0
104.80	148.0
105.80	401.0
106.70	152.0
111.80	118.0
114.80	124.0
115.80	344.0
116.80	673.0
117.80	353.0
118.80	520.0
127.80	360.0
128.80	166.0
129.80	461.0
130.70	213.0
134.80	180.0
136.70	179.0
140.80	1019.0
141.90	114.0
142.80	1064.0
144.80	214.0
145.80	182.0
147.70	252.0
149.70	117.0
152.90	110.0
154.80	281.0
156.80	206.0
158.80	143.0
160.80	103.0
171.80	985.0
172.90	921.0
173.90	113992.0
174.90	7965.0
175.80	108984.0
176.90	6842.0
177.90	154.0

Instrument :
MSVOA_V
ClientSampleId :
BFB62