


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV070919\
Data File : VV011842.D
Acq On : 09 Jul 2019 10:06
Operator : SY/MD
Sample : BFB10
Misc : 25ML/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB10

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR070819SIM.M
Title : TRACE VOA SOM01.0
Last Update : Wed Jul 10 01:45:06 2019

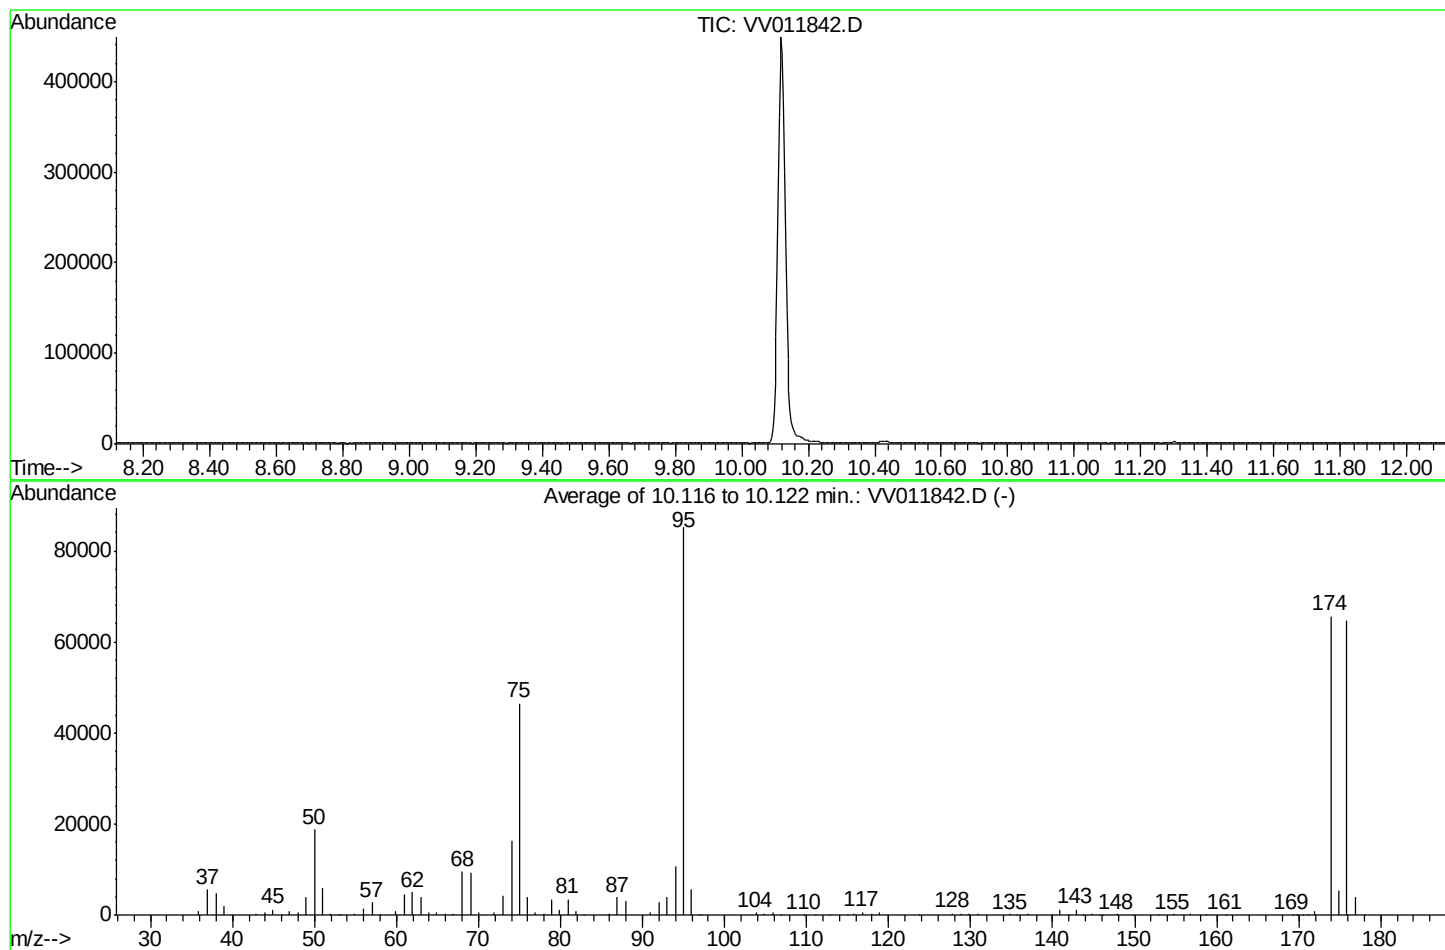

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.1	18816	PASS
75	95	30	80	54.6	46469	PASS
95	95	100	100	100.0	85157	PASS
96	95	5	9	6.6	5662	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	77.0	65552	PASS
175	174	5	9	8.3	5457	PASS
176	174	95	101	98.8	64776	PASS
177	176	5	9	6.2	4036	PASS

Scan 2794 (10.074 min): VV011842.D
BFB10

m/z	Abundance
35.60	115.0
39.80	333.0
41.30	102.0
43.10	108.0
44.00	366.0

Instrument :
MSVOA_V
ClientSampleId :
BFB10

m/z	Abundance
35.90	949.0
37.00	5383.0
37.90	4783.0
38.90	1812.0
39.90	227.0
42.80	173.0
43.90	1020.0
44.90	1164.0
45.90	134.0
46.90	956.0
47.90	563.0
49.00	4058.0
50.00	18696.0
51.00	5671.0
51.90	364.0
53.10	102.0
54.90	348.0
56.00	1541.0
57.00	2518.0
58.00	108.0
59.90	857.0
61.00	4549.0
62.00	4787.0
63.00	3877.0
63.90	576.0
64.90	682.0
66.00	218.0
66.80	248.0
68.00	9187.0
69.00	9200.0
70.00	707.0
71.90	556.0
73.00	4102.0
74.00	15958.0
75.00	45696.0
76.00	3994.0
76.90	567.0
77.90	412.0
78.80	3466.0
79.90	1072.0
80.90	3545.0
81.80	741.0
82.80	112.0
86.00	196.0
86.90	3926.0
88.00	3239.0
90.90	477.0
92.00	2816.0
93.00	3984.0
94.00	10565.0
95.00	83112.0
96.00	5529.0
96.90	154.0
103.80	454.0
104.70	184.0
105.80	415.0
109.70	112.0
112.80	123.0
114.80	136.0
115.70	299.0
116.80	583.0
117.80	324.0
118.80	608.0
123.70	146.0
127.80	390.0
128.90	193.0
129.80	280.0
130.80	210.0
134.90	195.0
136.90	209.0
139.90	103.0
140.80	1066.0
141.90	109.0
142.90	1105.0
143.70	104.0
144.80	318.0
145.70	143.0
147.90	230.0
149.80	101.0
154.80	232.0
156.80	176.0
158.70	145.0
169.20	126.0
171.10	200.0
171.90	1013.0
173.90	62320.0
174.90	5286.0
175.90	61608.0
176.90	3856.0
178.00	154.0

Instrument :
MSVOA_V
ClientSampleId :
BFB10

m/z	Abundance
35.90	904.0
37.00	5802.0
38.00	4844.0
39.00	1869.0
39.90	236.0
42.80	164.0
43.90	971.0
44.90	1172.0
46.90	951.0
47.90	637.0
49.00	4085.0
50.00	19608.0
51.00	6059.0
51.90	331.0
54.90	328.0
56.00	1610.0
57.00	2775.0
57.90	105.0
59.90	956.0
61.00	4791.0
61.90	5141.0
63.00	4041.0
63.90	580.0
64.90	679.0
66.00	235.0
66.80	240.0
68.00	9829.0
69.00	9687.0
69.90	679.0
71.80	668.0
73.00	4249.0
74.00	16944.0
75.00	48016.0
75.90	4156.0
76.90	607.0
77.90	449.0
78.80	3654.0
79.90	1036.0
80.90	3635.0
81.80	776.0
82.80	108.0
86.00	268.0
86.90	3983.0
88.00	3180.0
90.90	515.0
92.00	2968.0
93.00	4064.0
94.00	11173.0
95.00	88144.0
96.00	5823.0
97.10	190.0
103.80	480.0
104.80	204.0
105.80	451.0
106.90	114.0
109.70	138.0
111.00	126.0
112.70	155.0
114.90	133.0
115.80	351.0
116.80	710.0
117.90	362.0
118.80	617.0
123.80	116.0
127.80	431.0
128.90	184.0
129.80	302.0
130.90	193.0
134.80	216.0
136.90	226.0
139.80	102.0
140.80	1162.0
141.90	106.0
142.90	1231.0
144.80	317.0
145.80	153.0
146.10	146.0
147.90	249.0
149.70	115.0
154.80	253.0
156.90	201.0
158.70	105.0
169.20	104.0
170.50	115.0
171.90	961.0
173.90	67464.0
174.90	5639.0
175.90	66856.0
176.90	4226.0
178.00	145.0

Instrument :
MSVOA_V
ClientSampleId :
BFB10

m/z	Abundance
35.90	841.0
37.00	5461.0
38.00	4500.0
39.00	1919.0
39.90	252.0
42.90	130.0
44.00	886.0
44.90	1050.0
46.90	970.0
48.00	665.0
49.00	3757.0
50.00	18144.0
51.00	5818.0
51.90	295.0
52.80	109.0
54.80	325.0
56.00	1477.0
57.00	2773.0
57.90	142.0
59.90	1021.0
61.00	4555.0
61.90	5037.0
63.00	3858.0
63.90	575.0
64.90	655.0
66.00	176.0
66.90	234.0
68.00	9599.0
69.00	9344.0
69.90	647.0
71.80	676.0
73.00	4140.0
74.00	16070.0
75.00	45696.0
75.90	4075.0
76.90	545.0
77.90	409.0
78.90	3373.0
79.90	958.0
80.90	3391.0
81.90	782.0
86.00	299.0
86.90	3673.0
88.00	3036.0
90.90	493.0
91.90	2848.0
93.00	3823.0
94.00	10660.0
95.00	84216.0
95.90	5634.0
97.10	223.0
103.80	445.0
104.80	211.0
105.90	462.0
106.90	131.0
109.70	126.0
111.00	131.0
112.70	150.0
115.00	114.0
115.80	389.0
116.80	759.0
117.80	341.0
118.80	542.0
127.80	427.0
128.80	152.0
129.80	254.0
130.90	181.0
134.90	237.0
135.60	104.0
136.90	195.0
140.80	1126.0
142.80	1247.0
144.80	287.0
146.10	150.0
147.80	212.0
149.70	139.0
152.90	105.0
154.70	255.0
156.90	207.0
161.10	103.0
169.80	119.0
170.50	132.0
171.90	854.0
173.90	66872.0
174.90	5448.0
175.90	65864.0
176.90	4027.0
178.00	118.0

Instrument :
MSVOA_V
ClientSampleId :
BFB10