

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV070920\
 Data File : VV017424.D
 Acq On : 10 Jul 2020 01:43
 Operator : SY/MD
 Sample : L3253-17
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A37

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM070820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	64	71	81	rVB	95987	98402	12.06%	1.335%
2	1.579	146	152	162	rVB	75355	82554	10.12%	1.120%
3	2.122	311	321	337	rBV	184026	284947	34.93%	3.867%
4	2.280	367	370	372	rBV3	588	456	0.06%	0.006%
5	2.782	524	526	528	rBV2	833	472	0.06%	0.006%
6	3.177	646	649	650	rBV2	1020	487	0.06%	0.007%
7	3.219	650	662	673	rBV2	6503	13675	1.68%	0.186%
8	3.293	683	685	690	rVB2	1003	634	0.08%	0.009%
9	3.396	714	717	718	rBV	817	451	0.06%	0.006%
10	3.560	765	768	774	rVB3	564	586	0.07%	0.008%
11	3.602	777	781	783	rBV2	1302	796	0.10%	0.011%
12	3.672	798	803	808	rVB3	620	676	0.08%	0.009%
13	3.769	830	833	837	rVV3	648	476	0.06%	0.006%
14	3.830	848	852	854	rBV3	515	427	0.05%	0.006%
15	3.936	866	885	912	rBV3	133737	442049	54.19%	5.999%
16	4.376	1007	1022	1051	rVB2	145928	359837	44.12%	4.883%
17	4.524	1065	1068	1071	rBV3	1134	762	0.09%	0.010%
18	4.585	1084	1087	1091	rVB3	861	637	0.08%	0.009%
19	4.711	1113	1126	1134	rVV7	4969	11789	1.45%	0.160%
20	4.859	1169	1172	1174	rBV3	1147	511	0.06%	0.007%
21	4.942	1193	1198	1201	rBV5	726	525	0.06%	0.007%
22	4.974	1205	1208	1210	rBV2	753	550	0.07%	0.007%
23	5.071	1216	1238	1259	rBV4	312205	809812	99.28%	10.990%
24	5.331	1317	1319	1323	rBV4	1144	736	0.09%	0.010%
25	5.376	1331	1333	1334	rBV2	990	459	0.06%	0.006%
26	5.421	1339	1347	1349	rBV6	792	900	0.11%	0.012%
27	5.473	1360	1363	1364	rBV	880	461	0.06%	0.006%
28	5.640	1403	1415	1439	rBV	342672	681822	83.59%	9.253%
29	5.807	1464	1467	1468	rBV3	882	506	0.06%	0.007%
30	5.936	1497	1507	1524	rVB6	24493	57031	6.99%	0.774%
31	6.026	1533	1535	1537	rBV2	831	483	0.06%	0.007%
32	6.093	1540	1556	1579	rBV2	178076	369953	45.36%	5.021%
33	6.193	1582	1587	1589	rBV4	691	693	0.08%	0.009%
34	6.402	1649	1652	1655	rBV3	1073	729	0.09%	0.010%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV070920\
 Data File : VV017424.D
 Acq On : 10 Jul 2020 01:43
 Operator : SY/MD
 Sample : L3253-17
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A37

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM070820WMA.M
 Title : VOC Analysis

35	6.470	1666	1673	1675	rBV5	942	1025	0.13%	0.014%
36	6.553	1695	1699	1701	rBV2	938	743	0.09%	0.010%
37	6.653	1727	1730	1732	rBV2	1186	755	0.09%	0.010%
38	6.730	1751	1754	1759	rBV4	985	903	0.11%	0.012%
39	6.836	1781	1787	1788	rBV4	946	881	0.11%	0.012%
40	6.962	1824	1826	1829	rBV2	766	430	0.05%	0.006%
41	7.007	1829	1840	1857	rBV	102983	185972	22.80%	2.524%
42	7.183	1892	1895	1899	rVB4	1227	918	0.11%	0.012%
43	7.212	1899	1904	1906	rBV3	764	510	0.06%	0.007%
44	7.338	1932	1943	1965	rBV	372955	633660	77.69%	8.600%
45	7.643	2027	2038	2059	rBV	74939	132303	16.22%	1.796%
46	7.945	2128	2132	2134	rVV2	1091	899	0.11%	0.012%
47	7.997	2138	2148	2162	rVB	107356	178428	21.88%	2.422%
48	8.109	2173	2183	2214	rBV	188703	363872	44.61%	4.938%
49	8.392	2268	2271	2272	rBV2	813	456	0.06%	0.006%
50	8.482	2297	2299	2304	rVB3	1148	620	0.08%	0.008%
51	8.524	2308	2312	2316	rBV3	762	821	0.10%	0.011%
52	8.582	2327	2330	2333	rBV3	779	571	0.07%	0.008%
53	8.704	2365	2368	2370	rBV2	1358	803	0.10%	0.011%
54	8.871	2408	2420	2437	rBV	496878	815670	100.00%	11.070%
55	9.199	2518	2522	2525	rBV3	671	431	0.05%	0.006%
56	9.457	2598	2602	2605	rBV4	736	551	0.07%	0.007%
57	9.521	2619	2622	2625	rVB4	893	569	0.07%	0.008%
58	9.537	2625	2627	2629	rBV3	963	499	0.06%	0.007%
59	9.723	2680	2685	2689	rVB4	906	820	0.10%	0.011%
60	9.807	2708	2711	2716	rVB3	966	652	0.08%	0.009%
61	9.833	2716	2719	2721	rBV2	929	564	0.07%	0.008%
62	9.897	2736	2739	2741	rBV2	876	461	0.06%	0.006%
63	9.984	2764	2766	2772	rVB3	926	525	0.06%	0.007%
64	10.032	2776	2781	2786	rBV5	881	1226	0.15%	0.017%
65	10.055	2786	2788	2793	rVB3	1286	785	0.10%	0.011%
66	10.154	2814	2819	2820	rBV3	862	626	0.08%	0.008%
67	10.177	2824	2826	2832	rVB3	800	686	0.08%	0.009%
68	10.238	2832	2845	2863	rBV	235660	375490	46.03%	5.096%
69	10.395	2889	2894	2895	rBV3	1752	1201	0.15%	0.016%
70	10.527	2930	2935	2936	rBV	540	480	0.06%	0.007%
71	10.807	3017	3022	3023	rBV2	825	513	0.06%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV070920\
 Data File : VV017424.D
 Acq On : 10 Jul 2020 01:43
 Operator : SY/MD
 Sample : L3253-17
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A37

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM070820WMA.M
 Title : VOC Analysis

72	10.958	3067	3069	3077	rVB5	830	641	0.08%	0.009%
73	11.071	3100	3104	3108	rVB3	835	813	0.10%	0.011%
74	11.177	3134	3137	3144	rVB5	1076	1035	0.13%	0.014%
75	11.270	3155	3166	3188	rBV	508707	784155	96.14%	10.642%
76	11.402	3205	3207	3209	rBV3	839	506	0.06%	0.007%
77	11.550	3248	3253	3255	rBV3	3853	3199	0.39%	0.043%
78	11.646	3272	3283	3306	rVB	403711	630850	77.34%	8.561%
79	11.829	3337	3340	3342	rBV3	1029	611	0.07%	0.008%
80	12.048	3406	3408	3413	rBV2	643	574	0.07%	0.008%
81	12.177	3443	3448	3452	rBV5	643	593	0.07%	0.008%
82	12.219	3456	3461	3465	rBV5	694	554	0.07%	0.008%
83	12.254	3468	3472	3476	rBV3	1507	1482	0.18%	0.020%
84	12.334	3491	3497	3500	rBV4	915	1023	0.13%	0.014%
85	12.466	3534	3538	3540	rBV4	689	594	0.07%	0.008%
86	12.604	3579	3581	3586	rVB3	644	522	0.06%	0.007%
87	12.897	3667	3672	3675	rBV4	1129	1049	0.13%	0.014%
88	12.964	3689	3693	3695	rBV2	668	481	0.06%	0.007%
89	13.180	3758	3760	3765	rVB3	974	866	0.11%	0.012%
90	13.209	3765	3769	3770	rBV2	938	582	0.07%	0.008%
91	13.305	3795	3799	3803	rBV2	860	584	0.07%	0.008%
92	13.360	3812	3816	3820	rBV2	752	828	0.10%	0.011%
93	13.730	3927	3931	3934	rBV3	898	773	0.09%	0.010%
94	14.135	4055	4057	4062	rBV3	855	627	0.08%	0.009%
95	14.534	4178	4181	4182	rBV2	819	529	0.06%	0.007%
96	14.672	4221	4224	4225	rBV3	686	455	0.06%	0.006%
97	14.797	4260	4263	4267	rBV3	709	636	0.08%	0.009%
98	15.215	4389	4393	4394	rBV2	685	486	0.06%	0.007%
99	15.315	4420	4424	4429	rBV5	1114	1271	0.16%	0.017%
100	15.730	4551	4553	4555	rBV2	965	545	0.07%	0.007%


Sum of corrected areas: 7368467

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV070920\
Data File : VV017424.D
Acq On : 10 Jul 2020 01:43
Operator : SY/MD
Sample : L3253-17
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
F4A37

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM070820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

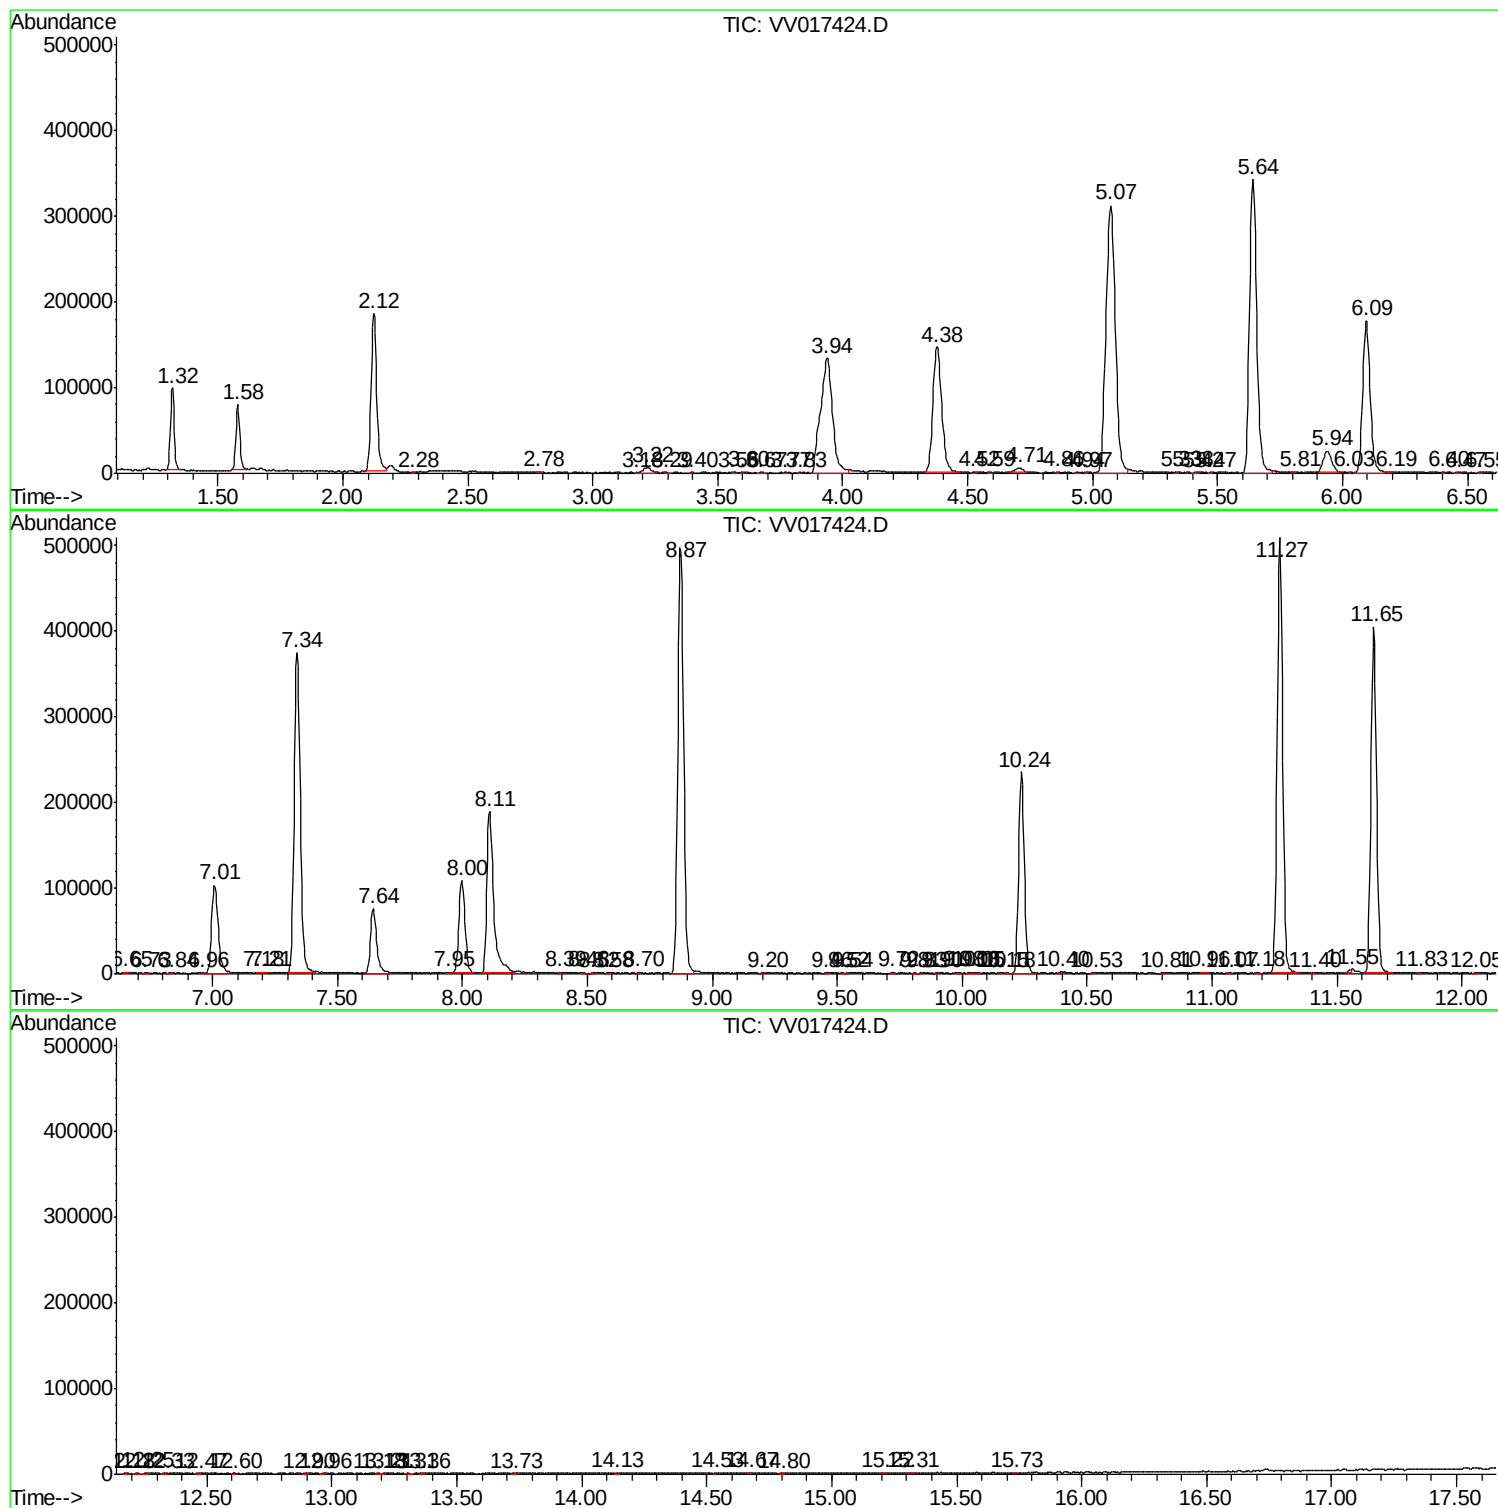

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV070920\
Data File : VV017424.D
Acq On : 10 Jul 2020 01:43
Operator : SY/MD
Sample : L3253-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A37

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM070820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV070920\
Data File : VV017424.D
Acq On : 10 Jul 2020 01:43
Operator : SY/MD
Sample : L3253-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A37

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM070820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc