

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV070920\
 Data File : VV017427.D
 Acq On : 10 Jul 2020 02:52
 Operator : SY/MD
 Sample : L3253-20
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A40

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM070820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	83	rVB	92563	99297	6.99%	1.196%
2	1.579	145	152	161	rBV	78128	86696	6.10%	1.044%
3	2.123	311	321	336	rBV	180332	278661	19.62%	3.355%
4	2.785	520	527	535	rVV5	1907	3164	0.22%	0.038%
5	2.840	540	544	546	rBV3	1029	639	0.04%	0.008%
6	2.952	576	579	585	rVB2	736	622	0.04%	0.007%
7	2.981	585	588	591	rBV3	959	661	0.05%	0.008%
8	3.074	614	617	620	rBV3	676	476	0.03%	0.006%
9	3.216	650	661	675	rVB3	19069	40870	2.88%	0.492%
10	3.331	695	697	701	rVB	793	404	0.03%	0.005%
11	3.672	800	803	807	rBV2	458	420	0.03%	0.005%
12	3.746	822	826	829	rVB3	864	628	0.04%	0.008%
13	3.782	833	837	840	rBV3	1078	672	0.05%	0.008%
14	3.942	866	887	912	rBV2	533448	1420104	100.00%	17.099%
15	4.380	1007	1023	1048	rBV	142349	360345	25.37%	4.339%
16	4.544	1070	1074	1077	rBV4	1070	828	0.06%	0.010%
17	4.634	1099	1102	1104	rBV2	902	585	0.04%	0.007%
18	4.704	1110	1124	1134	rBV9	3572	9910	0.70%	0.119%
19	4.823	1159	1161	1165	rVB3	954	415	0.03%	0.005%
20	4.955	1199	1202	1205	rVB3	961	638	0.04%	0.008%
21	4.978	1205	1209	1211	rBV2	701	536	0.04%	0.006%
22	4.994	1211	1214	1218	rBV3	1016	783	0.06%	0.009%
23	5.074	1222	1239	1259	rBV2	312784	804535	56.65%	9.687%
24	5.229	1284	1287	1289	rBV3	1173	900	0.06%	0.011%
25	5.434	1347	1351	1352	rBV2	666	452	0.03%	0.005%
26	5.486	1364	1367	1371	rBB3	532	412	0.03%	0.005%
27	5.511	1371	1375	1377	rBV2	1076	799	0.06%	0.010%
28	5.640	1401	1415	1439	rBV	339078	677368	47.70%	8.156%
29	5.939	1494	1508	1530	rBV8	26691	64737	4.56%	0.779%
30	6.093	1543	1556	1574	rBV2	178477	362941	25.56%	4.370%
31	6.331	1628	1630	1633	rBV2	750	508	0.04%	0.006%
32	6.457	1664	1669	1672	rBV5	798	726	0.05%	0.009%
33	6.482	1675	1677	1684	rVB5	1134	1016	0.07%	0.012%
34	6.518	1684	1688	1691	rBV3	914	799	0.06%	0.010%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV070920\
 Data File : VV017427.D
 Acq On : 10 Jul 2020 02:52
 Operator : SY/MD
 Sample : L3253-20
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A40

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM070820WMA.M
 Title : VOC Analysis

35	7.007	1827	1840	1859	rBV	102833	184315	12.98%	2.219%
36	7.338	1930	1943	1963	rBV	372085	640873	45.13%	7.717%
37	7.643	2028	2038	2056	rVV	72551	126859	8.93%	1.527%
38	7.830	2093	2096	2098	rBV2	750	470	0.03%	0.006%
39	7.859	2102	2105	2107	rBV4	641	418	0.03%	0.005%
40	7.949	2130	2133	2135	rVV2	1614	1047	0.07%	0.013%
41	7.997	2138	2148	2165	rVB	91144	156119	10.99%	1.880%
42	8.109	2173	2183	2213	rBV	188828	363062	25.57%	4.372%
43	8.370	2260	2264	2269	rBV4	855	783	0.06%	0.009%
44	8.412	2271	2277	2280	rVV6	1453	1274	0.09%	0.015%
45	8.479	2294	2298	2300	rBV2	1069	821	0.06%	0.010%
46	8.531	2311	2314	2318	rBV3	582	442	0.03%	0.005%
47	8.679	2358	2360	2364	rBV2	889	527	0.04%	0.006%
48	8.810	2397	2401	2404	rBV4	819	665	0.05%	0.008%
49	8.875	2409	2421	2436	rBV	502697	806667	56.80%	9.713%
50	9.293	2547	2551	2553	rBV2	649	471	0.03%	0.006%
51	9.408	2583	2587	2588	rBV2	570	410	0.03%	0.005%
52	9.640	2653	2659	2660	rBV3	862	682	0.05%	0.008%
53	9.759	2693	2696	2698	rBV2	872	666	0.05%	0.008%
54	9.891	2735	2737	2739	rBV2	882	461	0.03%	0.006%
55	9.958	2755	2758	2764	rBV4	718	632	0.04%	0.008%
56	10.003	2769	2772	2773	rBV2	832	483	0.03%	0.006%
57	10.238	2833	2845	2860	rBV	229515	363911	25.63%	4.382%
58	10.376	2884	2888	2889	rBV3	787	452	0.03%	0.005%
59	10.399	2889	2895	2904	rVV6	2219	2973	0.21%	0.036%
60	10.569	2946	2948	2954	rBV4	550	529	0.04%	0.006%
61	10.662	2974	2977	2979	rVB2	931	567	0.04%	0.007%
62	10.736	2996	3000	3001	rBV2	612	425	0.03%	0.005%
63	10.813	3020	3024	3026	rBV2	874	555	0.04%	0.007%
64	10.871	3039	3042	3045	rVB3	1035	599	0.04%	0.007%
65	10.910	3050	3054	3060	rBV3	775	714	0.05%	0.009%
66	10.939	3060	3063	3067	rVB2	790	534	0.04%	0.006%
67	10.987	3075	3078	3081	rBV2	713	433	0.03%	0.005%
68	11.270	3154	3166	3186	rBV	510105	776765	54.70%	9.353%
69	11.431	3214	3216	3218	rBV3	797	516	0.04%	0.006%
70	11.646	3272	3283	3299	rVB	402591	626735	44.13%	7.546%
71	11.788	3324	3327	3329	rBV3	831	520	0.04%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV070920\
 Data File : VV017427.D
 Acq On : 10 Jul 2020 02:52
 Operator : SY/MD
 Sample : L3253-20
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A40

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM070820WMA.M
 Title : VOC Analysis

72	11.804	3329	3332	3336	rVB3	1246	1016	0.07%	0.012%
73	11.836	3336	3342	3346	rBV4	1022	855	0.06%	0.010%
74	12.141	3433	3437	3440	rVB2	726	499	0.04%	0.006%
75	12.170	3443	3446	3448	rBV	802	519	0.04%	0.006%
76	12.212	3456	3459	3462	rBV3	580	484	0.03%	0.006%
77	12.395	3513	3516	3520	rBV3	831	650	0.05%	0.008%
78	12.553	3560	3565	3569	rBV2	653	722	0.05%	0.009%
79	12.572	3569	3571	3575	rVB2	770	500	0.04%	0.006%
80	12.646	3590	3594	3596	rBV3	755	525	0.04%	0.006%
81	12.707	3610	3613	3616	rBV3	1046	646	0.05%	0.008%
82	12.762	3626	3630	3631	rBV3	951	697	0.05%	0.008%
83	12.794	3637	3640	3643	rVB3	940	605	0.04%	0.007%
84	13.087	3729	3731	3734	rVB3	859	485	0.03%	0.006%
85	13.196	3762	3765	3766	rBV	808	443	0.03%	0.005%
86	13.720	3926	3928	3931	rBV2	862	574	0.04%	0.007%
87	13.736	3931	3933	3936	rVV	731	459	0.03%	0.006%
88	13.762	3939	3941	3946	rVB3	743	432	0.03%	0.005%
89	13.813	3952	3957	3958	rBV2	509	446	0.03%	0.005%
90	13.871	3973	3975	3980	rVB2	1034	719	0.05%	0.009%
91	13.923	3988	3991	3993	rBV	1040	519	0.04%	0.006%
92	14.055	4029	4032	4033	rBV2	727	445	0.03%	0.005%
93	14.106	4045	4048	4052	rBV3	1045	720	0.05%	0.009%
94	14.354	4120	4125	4127	rBV3	986	1013	0.07%	0.012%
95	14.424	4144	4147	4151	rBV3	724	659	0.05%	0.008%
96	14.588	4196	4198	4203	rVB3	814	480	0.03%	0.006%
97	14.691	4227	4230	4233	rBV2	865	677	0.05%	0.008%
98	15.080	4349	4351	4353	rBV2	851	497	0.03%	0.006%
99	15.508	4482	4484	4488	rBV	997	734	0.05%	0.009%
100	16.228	4704	4708	4709	rBV3	1527	1155	0.08%	0.014%


Sum of corrected areas: 8305097

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV070920\
Data File : VV017427.D
Acq On : 10 Jul 2020 02:52
Operator : SY/MD
Sample : L3253-20
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
F4A40

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM070820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

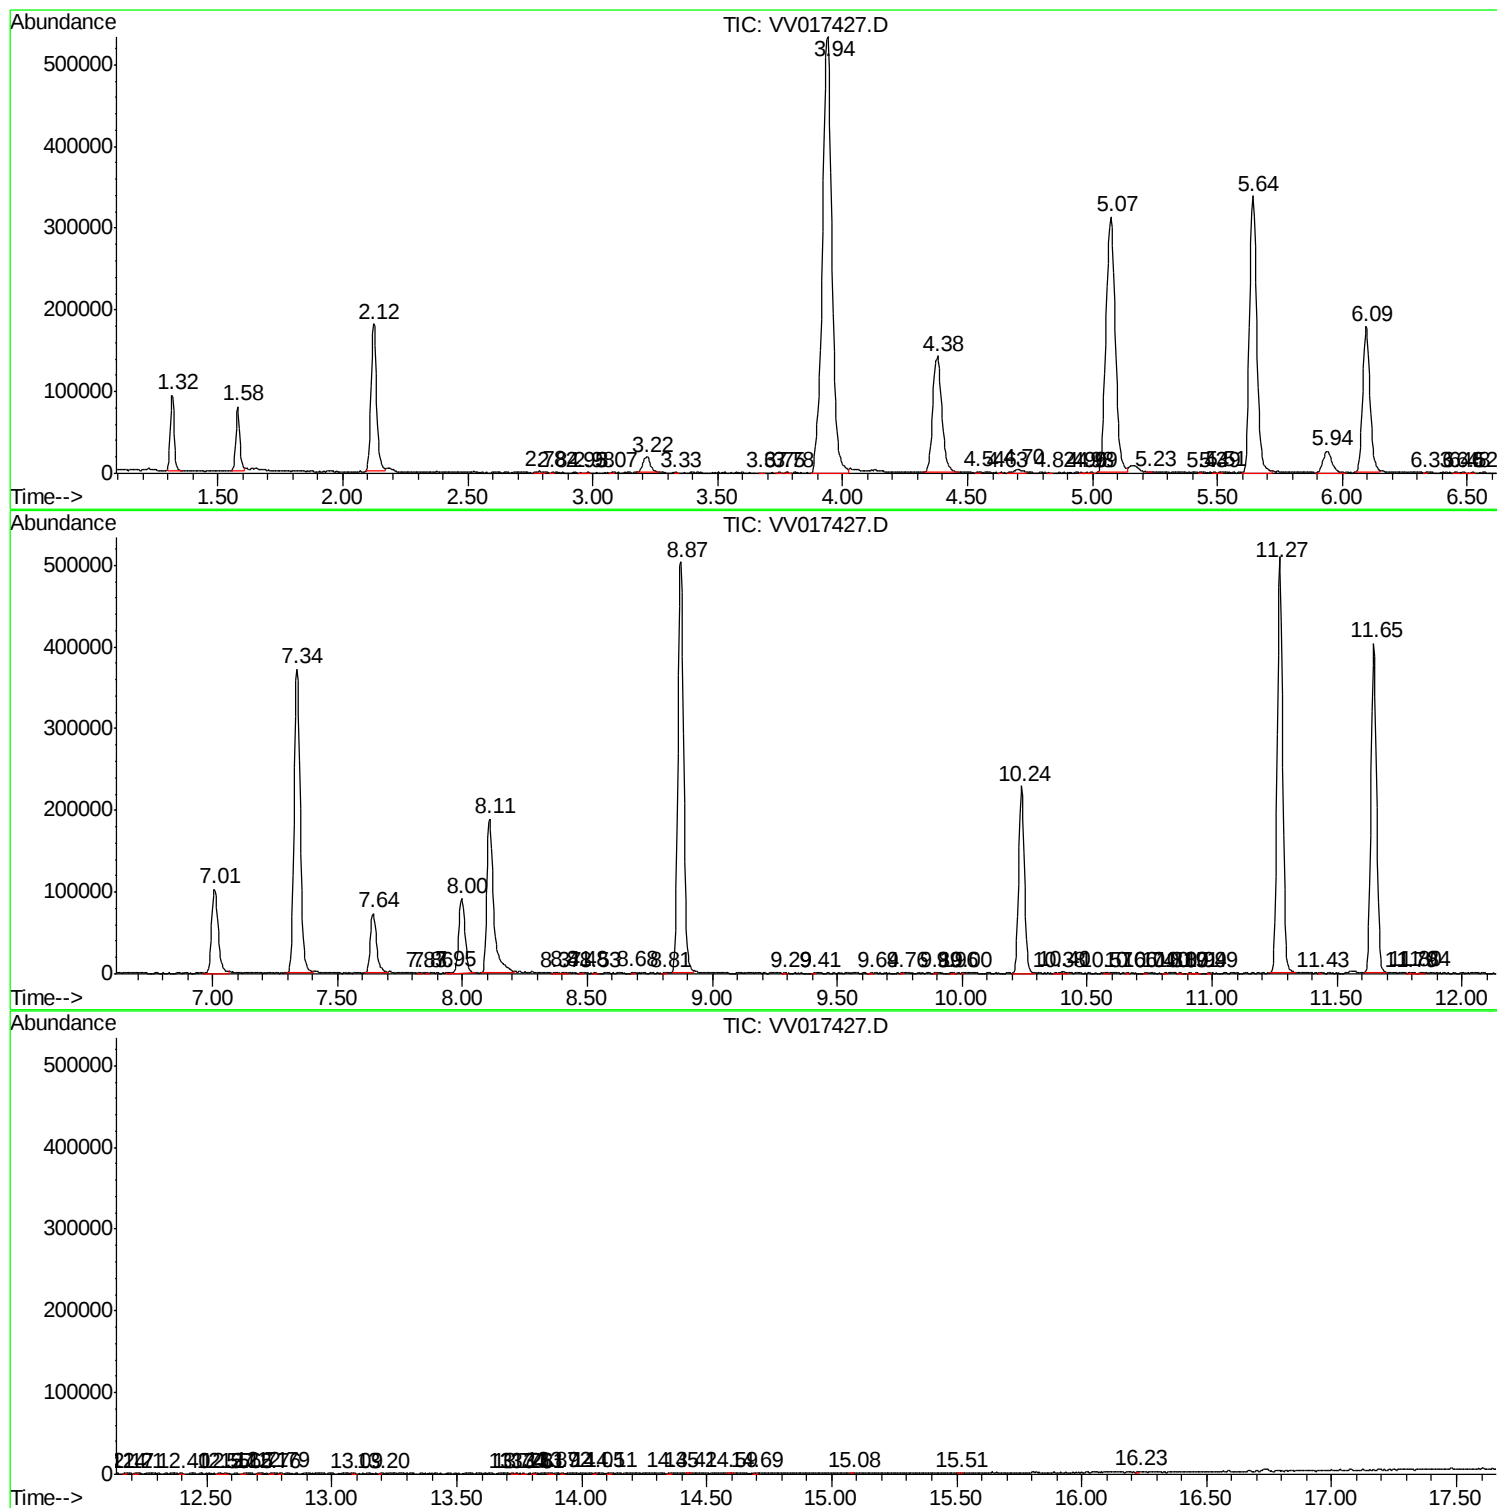

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV070920\
Data File : VV017427.D
Acq On : 10 Jul 2020 02:52
Operator : SY/MD
Sample : L3253-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A40

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM070820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV070920\
Data File : VV017427.D
Acq On : 10 Jul 2020 02:52
Operator : SY/MD
Sample : L3253-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A40

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM070820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc