


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV070920\
 Data File : VV017392.D
 Acq On : 09 Jul 2020 11:01
 Operator : SY/MD
 Sample : BFB98
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB98

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM070820WMA.M
 Title : VOC Analysis
 Last Update : Fri Jul 10 05:13:25 2020

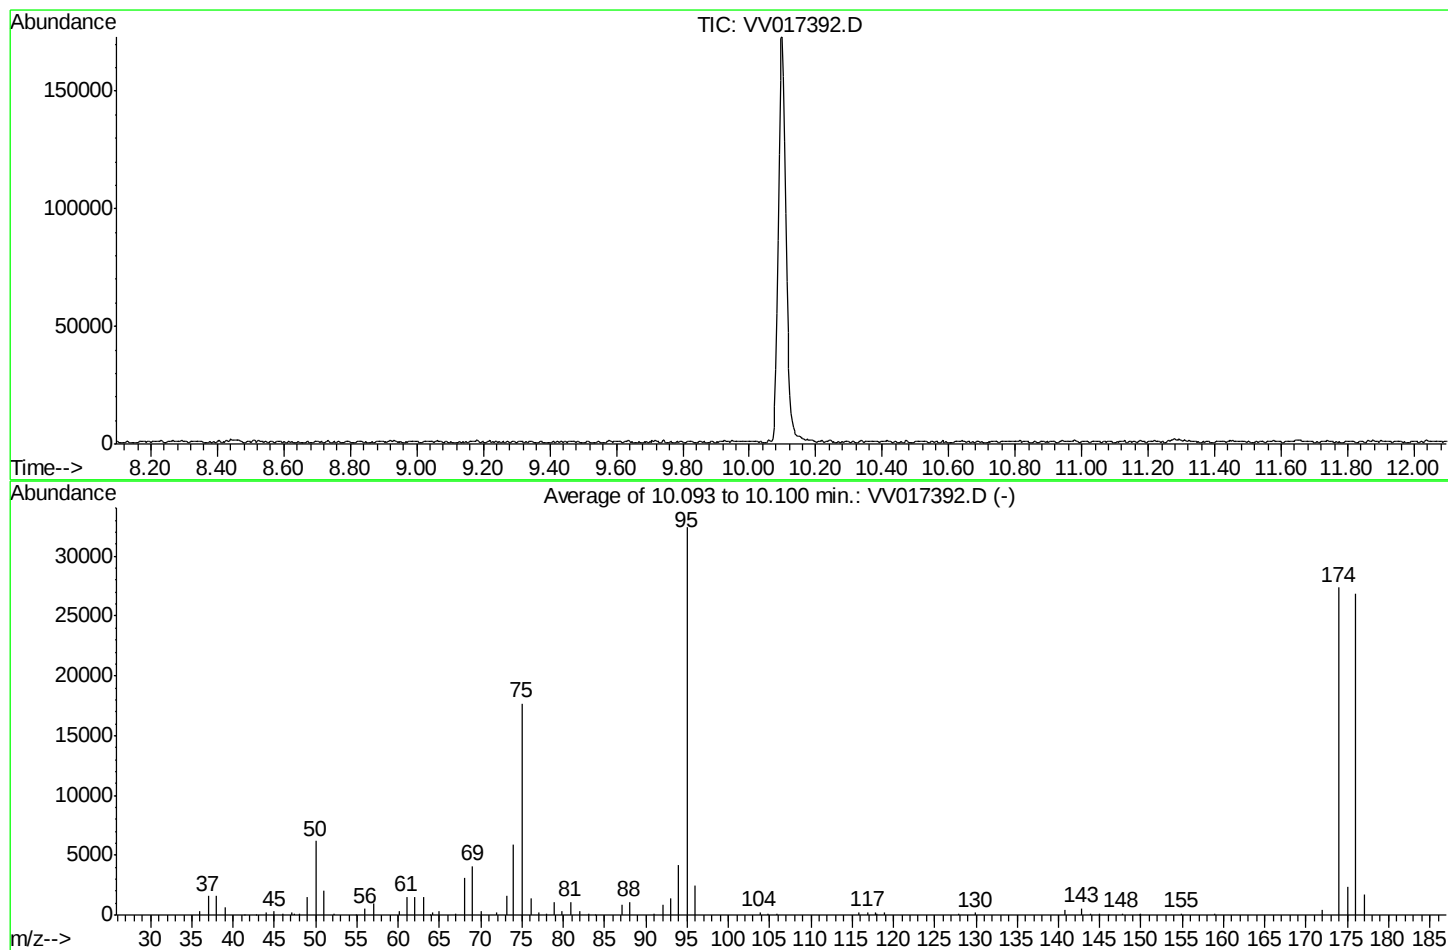

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2790

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	6161	PASS
75	95	30	80	54.5	17677	PASS
95	95	100	100	100.0	32421	PASS
96	95	5	9	7.4	2412	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	84.4	27368	PASS
175	174	5	9	8.8	2396	PASS
176	174	95	101	98.4	26920	PASS
177	176	5	9	6.3	1707	PASS

Scan 2790 (10.061 min): VV017392.D
BFB98

m/z	Abundance
37.10	131.0
38.10	106.0
39.90	298.0
41.90	110.0
44.00	262.0
45.50	109.0
48.10	144.0
51.00	114.0
54.80	101.0
74.30	104.0
82.20	105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB98

m/z	Abundance
36.00	275.0
37.00	1619.0
38.00	1624.0
39.00	568.0
40.00	268.0
42.70	118.0
43.90	395.0
44.90	304.0
46.00	108.0
47.00	188.0
47.40	181.0
47.90	277.0
49.00	1555.0
50.00	5759.0
51.00	2002.0
52.10	183.0
54.90	141.0
56.00	454.0
57.00	905.0
60.00	353.0
61.00	1580.0
62.00	1435.0
63.00	1468.0
64.10	136.0
64.90	356.0
66.90	125.0
68.00	2928.0
69.00	3823.0
69.90	305.0
71.90	192.0
73.10	1447.0
74.00	5635.0
75.00	16367.0
76.10	1520.0
76.90	242.0
77.90	179.0
78.90	894.0
79.80	367.0
80.90	1058.0
82.00	349.0
83.80	121.0
87.00	809.0
88.00	1000.0
90.90	125.0
92.10	732.0
93.00	1307.0
94.00	3910.0
95.00	30064.0
96.00	2365.0
103.80	215.0
104.80	123.0
106.00	156.0
115.80	243.0
116.90	233.0
117.80	148.0
118.90	256.0
128.00	143.0
130.00	183.0
141.00	437.0
142.80	483.0
147.60	140.0
150.00	118.0
154.90	132.0
158.80	105.0
172.10	433.0
174.00	24936.0
175.00	2097.0
176.00	24272.0
177.00	1701.0

Instrument :
MSVOA_V
ClientSampleId :
BFB98

m/z	Abundance
35.90	290.0
37.00	1757.0
38.00	1736.0
39.10	620.0
40.00	277.0
41.90	118.0
43.90	456.0
44.90	299.0
46.00	111.0
47.10	231.0
47.90	238.0
49.00	1565.0
50.00	6264.0
51.00	2255.0
52.10	159.0
54.80	159.0
56.00	531.0
57.00	982.0
60.10	354.0
61.00	1543.0
62.00	1488.0
63.00	1542.0
63.80	130.0
64.20	164.0
64.90	343.0
67.00	164.0
68.00	3259.0
69.00	4345.0
70.00	271.0
71.90	199.0
73.10	1636.0
74.00	6007.0
75.00	18352.0
76.10	1490.0
77.00	179.0
78.00	169.0
78.80	1115.0
79.80	345.0
80.90	1148.0
81.90	402.0
83.10	126.0
87.10	922.0
88.00	1150.0
91.00	138.0
92.10	872.0
93.00	1475.0
94.00	4359.0
95.00	33632.0
96.00	2496.0
103.80	235.0
104.80	130.0
106.00	143.0
115.80	255.0
116.90	284.0
117.70	181.0
118.00	185.0
118.90	269.0
128.00	157.0
129.90	178.0
140.80	465.0
142.80	572.0
144.00	110.0
144.90	114.0
147.70	137.0
149.90	124.0
154.90	144.0
158.80	126.0
172.00	425.0
174.00	28328.0
175.00	2563.0
176.00	28000.0
177.00	1777.0

Instrument :
MSVOA_V
ClientSampleId :
BFB98

m/z	Abundance
35.80	318.0
37.00	1812.0
38.00	1644.0
39.10	626.0
40.00	267.0
41.30	103.0
41.90	118.0
44.00	507.0
45.00	299.0
46.00	104.0
47.10	289.0
47.90	237.0
49.00	1440.0
50.00	6462.0
51.00	2301.0
52.20	130.0
54.90	159.0
56.00	566.0
57.00	1001.0
60.20	375.0
61.00	1475.0
62.00	1482.0
63.00	1396.0
64.20	253.0
65.00	345.0
67.10	200.0
68.00	3189.0
69.00	4209.0
70.10	262.0
71.80	211.0
73.10	1676.0
74.00	5890.0
75.00	18312.0
76.10	1333.0
77.10	189.0
78.00	118.0
78.80	1188.0
79.80	310.0
80.90	1156.0
81.90	354.0
83.10	134.0
87.10	951.0
88.00	1111.0
91.00	182.0
92.10	864.0
93.10	1480.0
94.00	4236.0
95.00	33568.0
96.00	2375.0
103.80	200.0
104.80	111.0
105.90	149.0
115.80	216.0
116.90	278.0
117.70	204.0
118.00	175.0
118.80	263.0
127.80	158.0
129.90	160.0
140.80	510.0
142.80	624.0
143.90	158.0
144.90	129.0
146.00	101.0
147.80	151.0
149.70	124.0
155.00	119.0
158.90	111.0
171.90	422.0
174.00	28840.0
175.00	2529.0
176.00	28488.0
177.00	1643.0

Instrument :
MSVOA_V
ClientSampleId :
BFB98