

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV071018\
 Data File : VV006568.D
 Acq On : 10 Jul 2018 14:57
 Operator : SY/MD
 Sample : J3919-09
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AJ4

Quant Time: Jul 11 03:38:06 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR070718WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Jul 11 03:34:14 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	322242	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	292004	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	128468	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	71617	4.09	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	81.80%
7) Chloroethane-d5	1.58	69	57991	3.79	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	75.80%
11) 1,1-Dichloroethene-d2	2.13	63	95513	2.93	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	58.60%#
20) 2-Butanone-d5	3.96	46	202594	45.53	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	91.06%
24) Chloroform-d	4.41	84	146551	4.25	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.00%
26) 1,2-Dichloroethane-d4	5.09	65	72495	4.53	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.60%
32) Benzene-d6	5.10	84	300000	4.50	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.00%
36) 1,2-Dichloropropane-d6	6.12	67	97949	4.53	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	90.60%
41) Toluene-d8	7.36	98	257066	4.32	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.40%
43) trans-1,3-Dichloropropene-	7.67	79	31143	4.25	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.00%
46) 2-Hexanone-d5	8.14	63	175503	47.43	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	94.86%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	73878	4.35	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	87.00%
64) 1,2-Dichlorobenzene-d4	11.68	152	106024	4.80	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.00%


Target Compounds					Ovalue
13) Acetone	2.21	43	11533	4.10 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV071018\
Data File : VV006568.D
Acq On : 10 Jul 2018 14:57
Operator : SY/MD
Sample : J3919-09
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AJ4

Quant Time: Jul 11 03:38:06 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR070718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Jul 11 03:34:14 2018
Response via : Initial Calibration

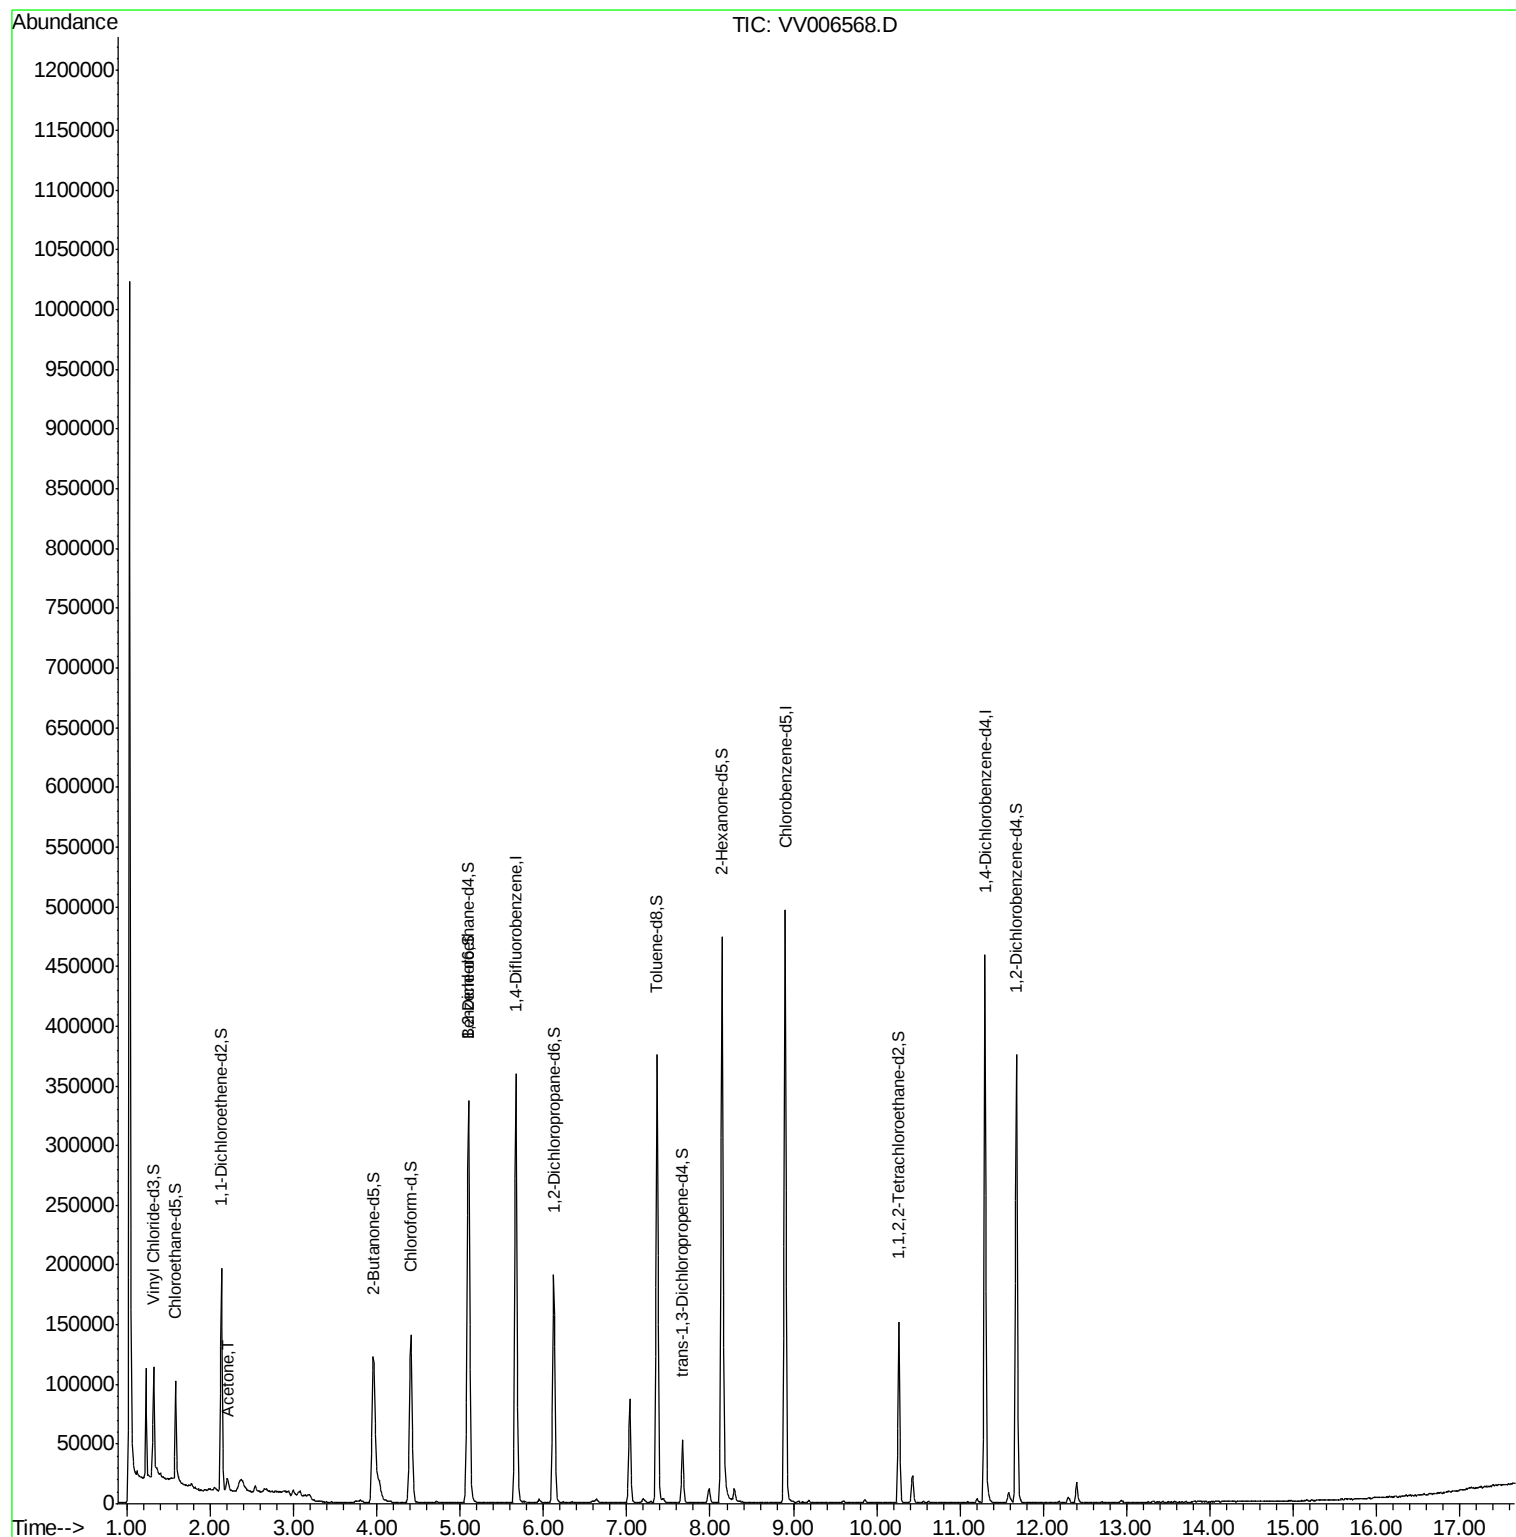

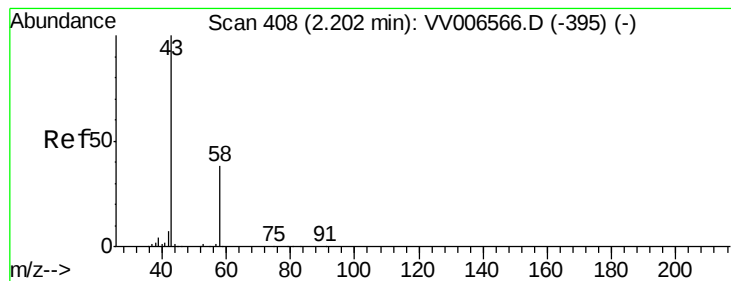

#13
 Acetone
 Concen: 4.10 ug/L
 RT: 2.21 min Scan# 409
 Delta R.T. 0.00 min
 Lab File: VV006568.D
 Acq: 10 Jul 2018 14:57

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AJ4

Tot Ion: 43 Resp: 11533
 Ion Ratio Lower Upper
 43 100
 58 38.5 0.0 76.2

