

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV071018\
 Data File : VV006571.D
 Acq On : 10 Jul 2018 16:18
 Operator : SY/MD
 Sample : J3920-02
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0SW2

Quant Time: Jul 11 03:43:42 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR070718WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Jul 11 03:34:14 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	305422	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	280487	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	122699	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	69929	4.21	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	84.20%
7) Chloroethane-d5	1.58	69	62488	4.31	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	86.20%
11) 1,1-Dichloroethene-d2	2.13	63	93373	3.02	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	60.40%
20) 2-Butanone-d5	3.97	46	208526	49.44	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	98.88%
24) Chloroform-d	4.41	84	145059	4.44	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.80%
26) 1,2-Dichloroethane-d4	5.09	65	71676	4.72	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.40%
32) Benzene-d6	5.10	84	298841	4.67	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.40%
36) 1,2-Dichloropropane-d6	6.12	67	97950	4.72	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.40%
41) Toluene-d8	7.37	98	254912	4.46	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.20%
43) trans-1,3-Dichloropropene-	7.67	79	31047	4.41	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	88.20%
46) 2-Hexanone-d5	8.14	63	180267	50.72	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	101.44%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	74609	4.57	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	91.40%
64) 1,2-Dichlorobenzene-d4	11.68	152	105293	4.99	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.80%


Target Compounds					Ovalue
13) Acetone	2.21	43	9758	3.66 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV071018\
Data File : VV006571.D
Acq On : 10 Jul 2018 16:18
Operator : SY/MD
Sample : J3920-02
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0SW2

Quant Time: Jul 11 03:43:42 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR070718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Jul 11 03:34:14 2018
Response via : Initial Calibration

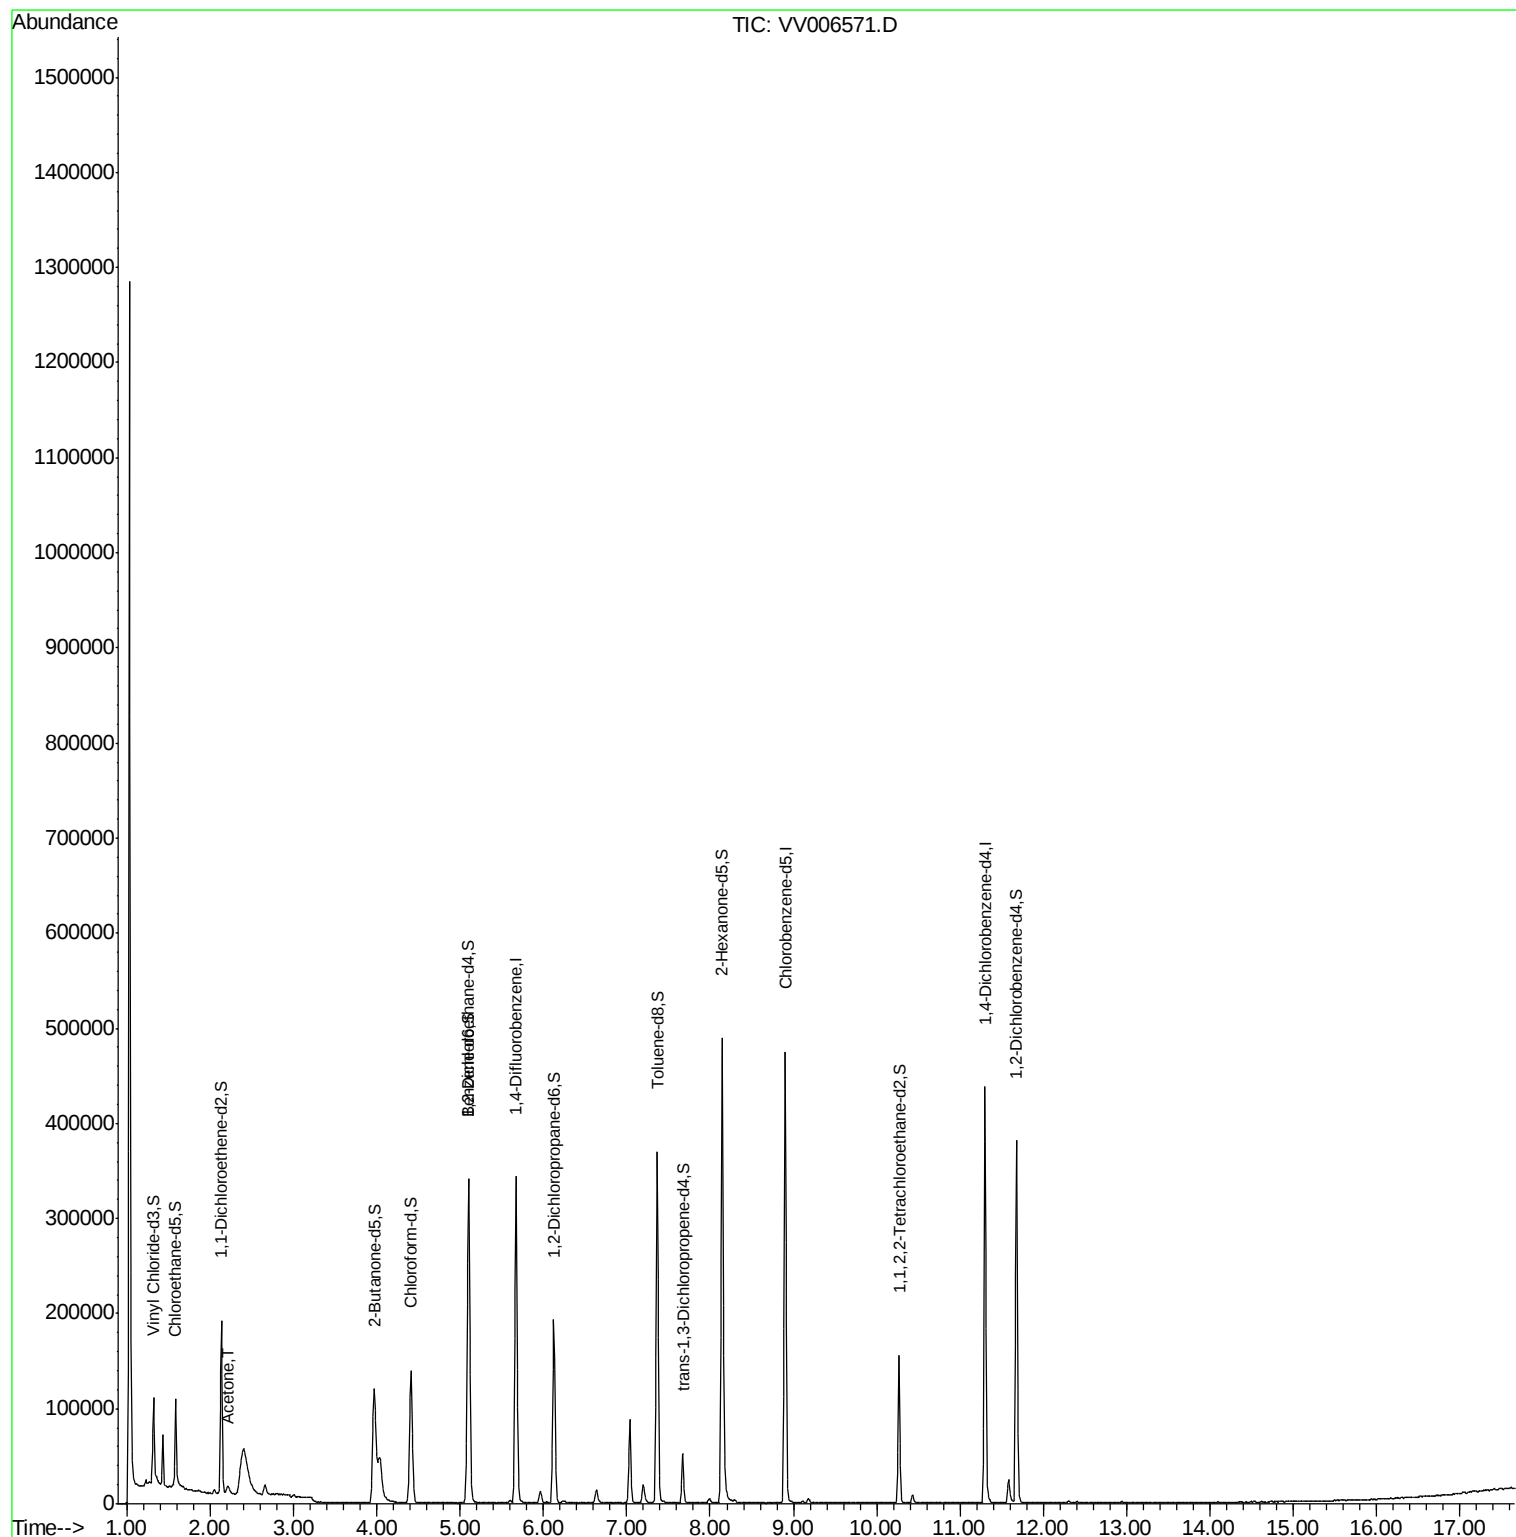

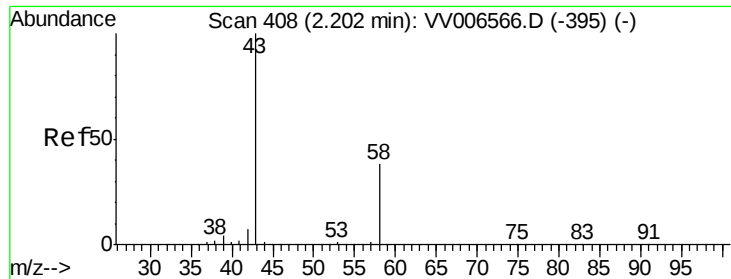

#13

Acetone

Concen: 3.66 ug/L

RT: 2.21 min Scan# 412

Delta R.T. 0.01 min

Lab File: VV006571.D

Acq: 10 Jul 2018 16:18

Instrument :
MSVOA_V
ClientSampleId :
C0SW2

Tot Ion: 43 Resp: 9758

Ion Ratio Lower Upper

43 100

58 40.6 0.0 76.2

