

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV071018\
 Data File : VV006576.D
 Acq On : 10 Jul 2018 18:35
 Operator : SY/MD
 Sample : J3919-04
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AJ1

Quant Time: Jul 11 03:54:41 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR070718WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Jul 11 03:34:14 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	299376	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	273898	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	120587	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	67790	4.16	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	83.20%
7) Chloroethane-d5	1.58	69	60859	4.28	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	85.60%
11) 1,1-Dichloroethene-d2	2.13	63	89060	2.94	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	58.80%#
20) 2-Butanone-d5	3.95	46	203932	49.33	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	98.66%
24) Chloroform-d	4.41	84	137910	4.31	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.20%
26) 1,2-Dichloroethane-d4	5.09	65	68152	4.58	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.60%
32) Benzene-d6	5.10	84	283029	4.53	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.60%
36) 1,2-Dichloropropane-d6	6.12	67	92198	4.55	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	91.00%
41) Toluene-d8	7.37	98	242216	4.34	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.80%
43) trans-1,3-Dichloropropene-	7.67	79	27508	4.00	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	80.00%
46) 2-Hexanone-d5	8.14	63	186046	53.60	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	107.20%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	72474	4.55	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	91.00%
64) 1,2-Dichlorobenzene-d4	11.68	152	99467	4.80	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.00%


Target Compounds					Ovalue
34) Trichloroethene	5.96	95	14942	0.71 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV071018\
Data File : VV006576.D
Acq On : 10 Jul 2018 18:35
Operator : SY/MD
Sample : J3919-04
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AJ1

Quant Time: Jul 11 03:54:41 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR070718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Jul 11 03:34:14 2018
Response via : Initial Calibration

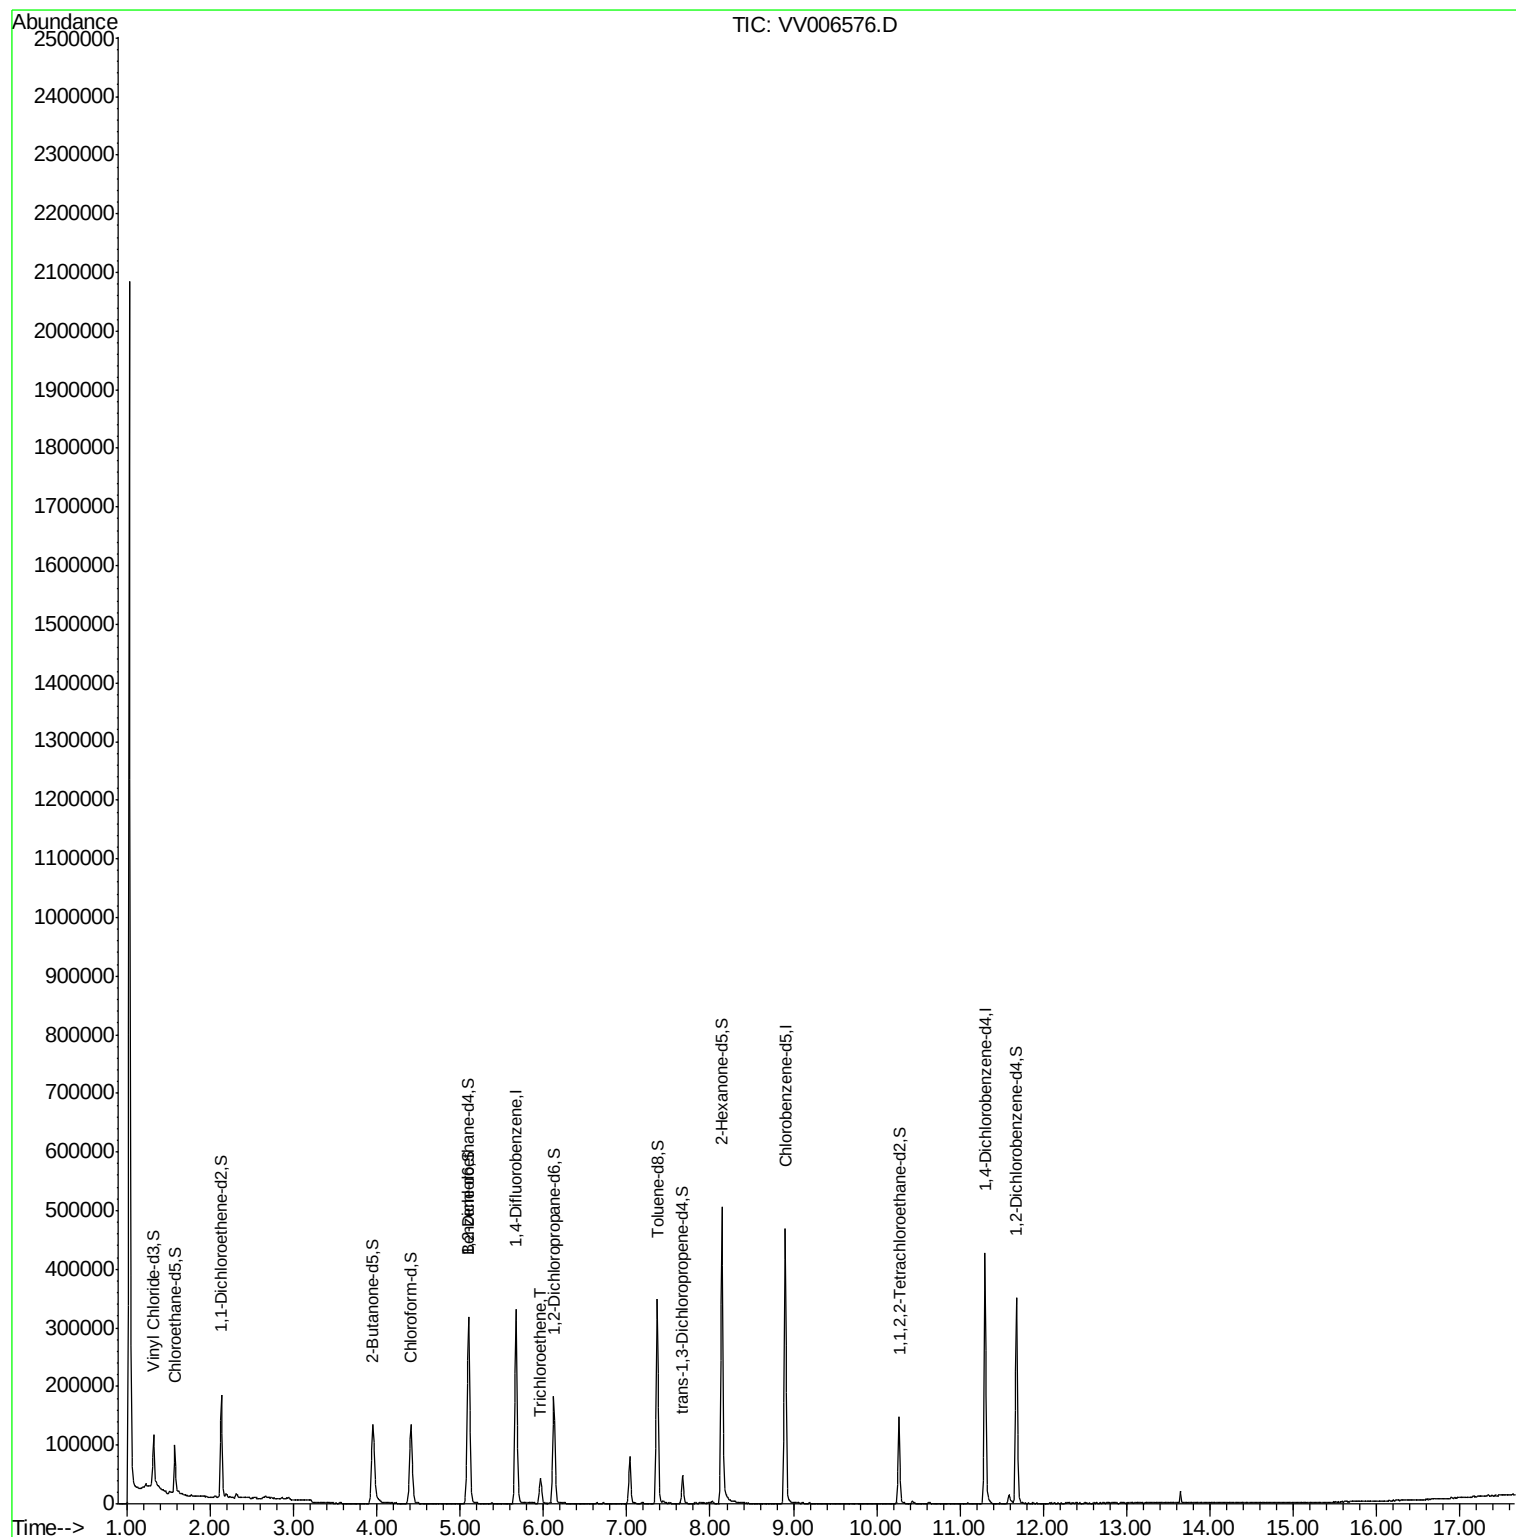

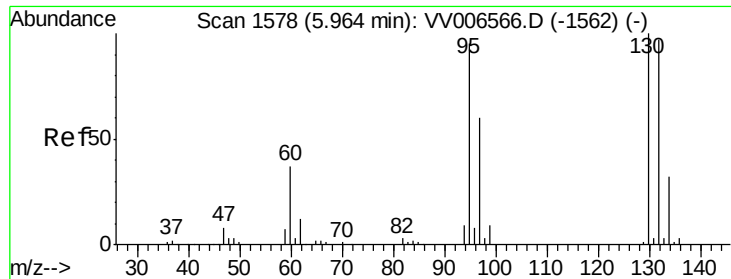

#34

Trichloroethene

Concen: 0.71 ua/L

RT: 5.96 min Scan# 1578

Delta R.T. -0.00 min

Lab File: VV006576.D

Acq: 10 Jul 2018 18:35

Instrument :

MSVOA_V

ClientSampleId :

C0AJ1

Tot Ion: 95 Resp: 14942


Ion Ratio Lower Upper

95 100

97 62.4 44.3 82.3

132 98.9 70.0 130.0

130 104.4 72.7 134.9

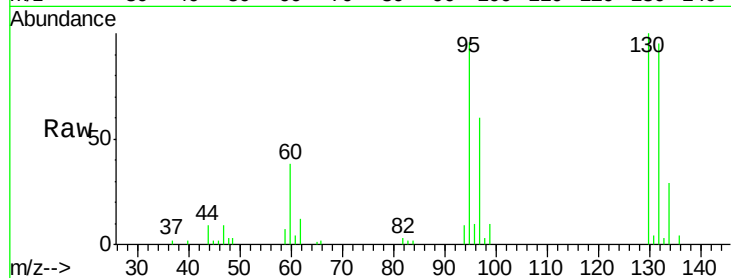

Abundance Ion 95.00 (94.70 to 95.70): VV0

Ion 96.95 (96.65 to 97.65): VV0

Ion 131.95 (131.65 to 132.65): V

Ion 129.95 (129.65 to 130.65): V

