


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV071019\
Data File : VV011848.D
Acq On : 10 Jul 2019 09:28
Operator : SY/MD
Sample : BFB11
Misc : 25ML/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB11

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR070819SIM.M
Title : TRACE VOA SOM01.0
Last Update : Mon Jul 15 07:13:53 2019

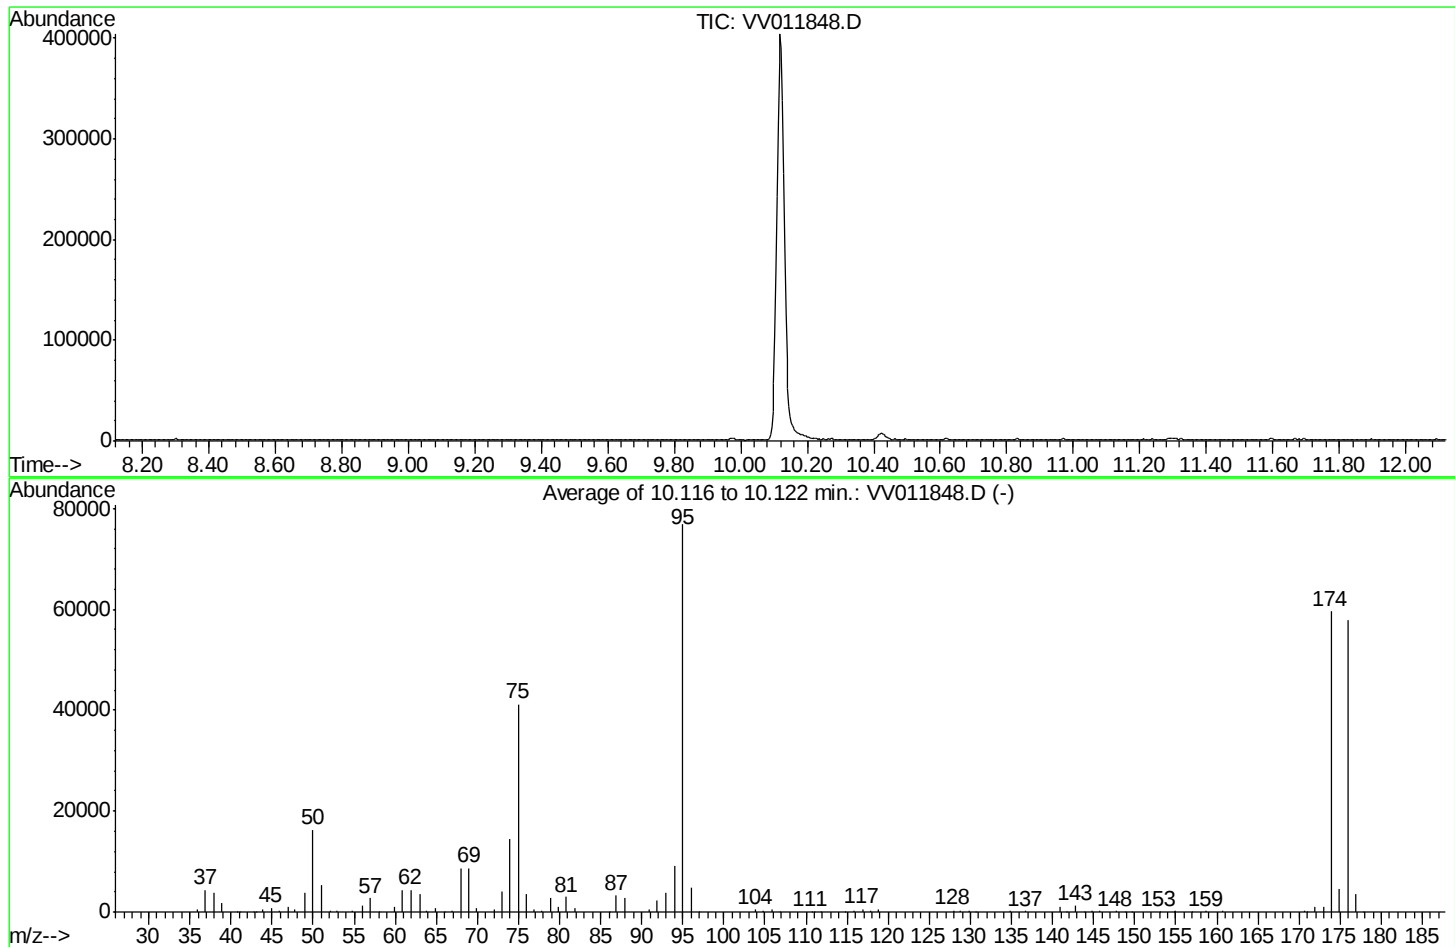

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.3	16368	PASS
75	95	30	80	53.5	41138	PASS
95	95	100	100	100.0	76866	PASS
96	95	5	9	6.4	4942	PASS
173	174	0.00	2	1.7	1031	PASS
174	95	50	120	77.6	59640	PASS
175	174	5	9	7.9	4693	PASS
176	174	95	101	97.2	57989	PASS
177	176	5	9	6.1	3542	PASS

m/z	Abundance
36.10	109.0
38.10	124.0
39.90	317.0
42.10	104.0
43.90	371.0
63.80	129.0

Instrument :
MSVOA_V
ClientSampleId :
BFB11

m/z	Abundance
35.90	724.0
36.90	4159.0
38.00	4016.0
39.00	1790.0
39.90	312.0
40.80	139.0
43.10	138.0
44.00	978.0
44.90	814.0
45.90	190.0
47.00	1116.0
47.80	652.0
49.00	3649.0
50.00	16114.0
51.00	5316.0
52.10	259.0
52.90	140.0
54.80	307.0
55.90	1360.0
57.00	2511.0
58.00	138.0
60.00	996.0
60.90	4360.0
61.90	4217.0
63.00	3663.0
63.80	352.0
64.90	703.0
66.10	128.0
66.90	262.0
68.00	8109.0
69.00	8609.0
69.90	652.0
72.00	455.0
73.00	3984.0
74.00	13796.0
75.00	40320.0
76.00	3350.0
76.90	559.0
77.80	324.0
78.90	2891.0
79.80	909.0
80.90	2832.0
81.80	733.0
86.10	111.0
86.90	3350.0
87.90	2794.0
91.00	432.0
91.90	2281.0
93.00	3751.0
94.00	9081.0
95.00	74496.0
96.00	4783.0
103.80	400.0
104.80	136.0
105.90	387.0
111.00	107.0
111.70	122.0
115.90	316.0
116.80	615.0
117.90	306.0
118.80	528.0
128.00	304.0
128.80	178.0
129.80	285.0
130.70	135.0
134.80	152.0
136.80	205.0
140.90	802.0
141.70	131.0
142.90	1159.0
143.80	121.0
144.80	302.0
145.80	173.0
147.80	235.0
153.00	118.0
154.70	189.0
158.70	180.0
160.60	159.0
170.70	154.0
171.00	153.0
172.00	921.0
173.00	1006.0
173.90	56208.0
174.90	4402.0
175.90	54448.0
176.90	3445.0
177.80	126.0

Instrument :
MSVOA_V
ClientSampleId :
BFB11

m/z	Abundance
36.00	751.0
36.90	4533.0
38.00	4232.0
39.00	1772.0
39.90	312.0
41.00	143.0
43.10	121.0
44.00	998.0
44.90	917.0
46.00	209.0
47.00	1152.0
47.80	653.0
48.90	3930.0
50.00	16928.0
51.00	5553.0
52.00	288.0
52.90	154.0
54.80	391.0
56.00	1376.0
57.00	2796.0
58.00	123.0
60.00	982.0
60.90	4337.0
61.90	4545.0
63.00	3801.0
63.90	356.0
64.90	691.0
66.10	121.0
66.90	283.0
68.00	8855.0
69.00	9073.0
69.90	694.0
72.00	501.0
73.00	4151.0
74.00	15075.0
75.00	42552.0
76.00	3623.0
76.90	521.0
77.80	347.0
78.90	2996.0
79.80	1000.0
80.90	3027.0
81.90	787.0
86.90	3376.0
87.90	2882.0
90.90	443.0
91.90	2284.0
92.90	3972.0
94.00	9546.0
95.00	79696.0
96.00	5106.0
97.00	102.0
103.90	450.0
104.80	148.0
105.90	400.0
106.80	103.0
110.60	135.0
111.70	110.0
115.90	344.0
116.80	681.0
117.80	394.0
118.80	482.0
127.90	367.0
128.80	191.0
129.80	278.0
130.70	119.0
134.80	177.0
136.70	255.0
140.90	939.0
141.70	140.0
142.90	1238.0
144.80	328.0
145.80	188.0
147.70	260.0
148.80	113.0
154.90	201.0
156.90	105.0
158.70	185.0
160.60	167.0
170.70	160.0
172.00	950.0
173.00	1038.0
173.90	61752.0
174.90	4890.0
175.90	60256.0
176.90	3663.0
177.80	123.0

Instrument :
MSVOA_V
ClientSampleId :
BFB11

m/z	Abundance
35.90	717.0
36.90	4410.0
38.00	3854.0
38.90	1674.0
39.90	311.0
41.00	127.0
42.80	116.0
43.20	114.0
43.90	1029.0
44.90	909.0
46.00	209.0
47.00	1012.0
47.80	606.0
48.90	3710.0
50.00	16063.0
51.00	5113.0
52.00	288.0
52.90	170.0
54.80	414.0
56.00	1251.0
57.00	2758.0
59.90	826.0
60.90	3941.0
61.90	4335.0
63.00	3528.0
63.90	369.0
64.90	642.0
66.00	115.0
66.90	251.0
67.90	8690.0
69.00	8429.0
69.90	693.0
72.00	499.0
72.90	3868.0
74.00	14721.0
75.00	40544.0
76.00	3571.0
76.90	476.0
77.80	341.0
78.90	2825.0
79.90	978.0
80.80	3001.0
81.90	757.0
86.90	3111.0
87.90	2822.0
90.80	443.0
91.90	2148.0
92.90	3878.0
94.00	9111.0
95.00	76408.0
96.00	4939.0
96.90	128.0
103.90	493.0
104.80	139.0
105.90	400.0
106.70	113.0
110.70	136.0
114.70	122.0
115.90	314.0
116.90	635.0
117.80	399.0
118.80	384.0
127.90	396.0
128.80	201.0
129.80	255.0
130.60	103.0
134.80	171.0
136.70	223.0
140.90	1012.0
141.70	123.0
142.80	1161.0
144.90	312.0
145.80	160.0
147.70	249.0
148.80	114.0
149.70	138.0
154.90	234.0
157.00	139.0
158.70	162.0
160.70	149.0
170.70	172.0
171.90	901.0
173.00	1049.0
173.90	60960.0
174.90	4789.0
175.90	59264.0
176.90	3519.0
177.80	127.0

Instrument :
MSVOA_V
ClientSampleId :
BFB11