
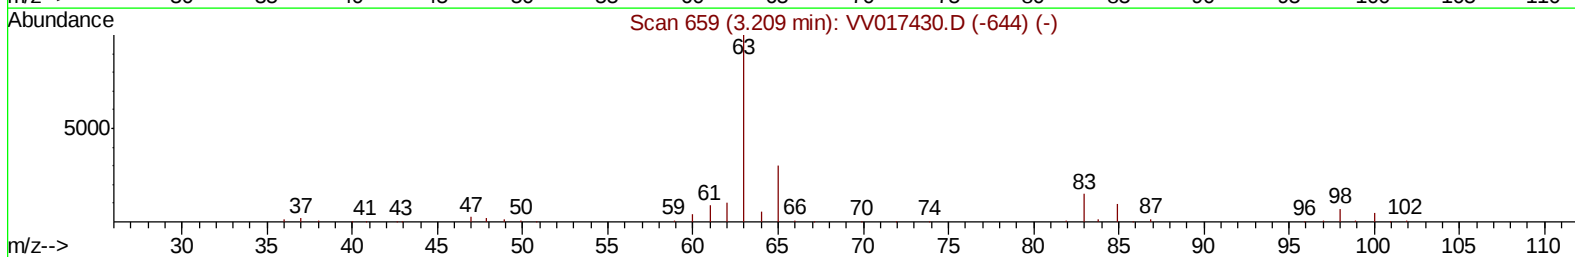
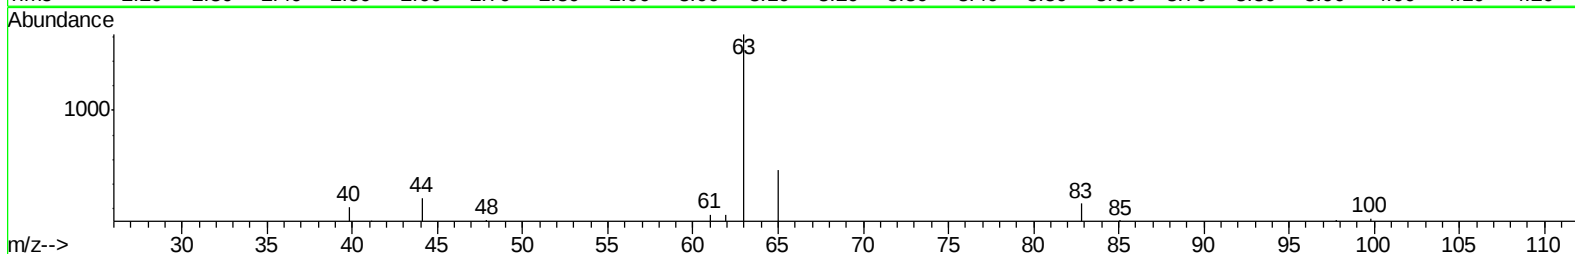


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV071020\
 Data File : VV017447.D
 Acq On : 10 Jul 2020 18:02
 Operator : SY/MD
 Sample : L3270-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Quant Time: Jul 11 00:26:52 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM070820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jul 11 00:23:19 2020
 Response via : Initial Calibration

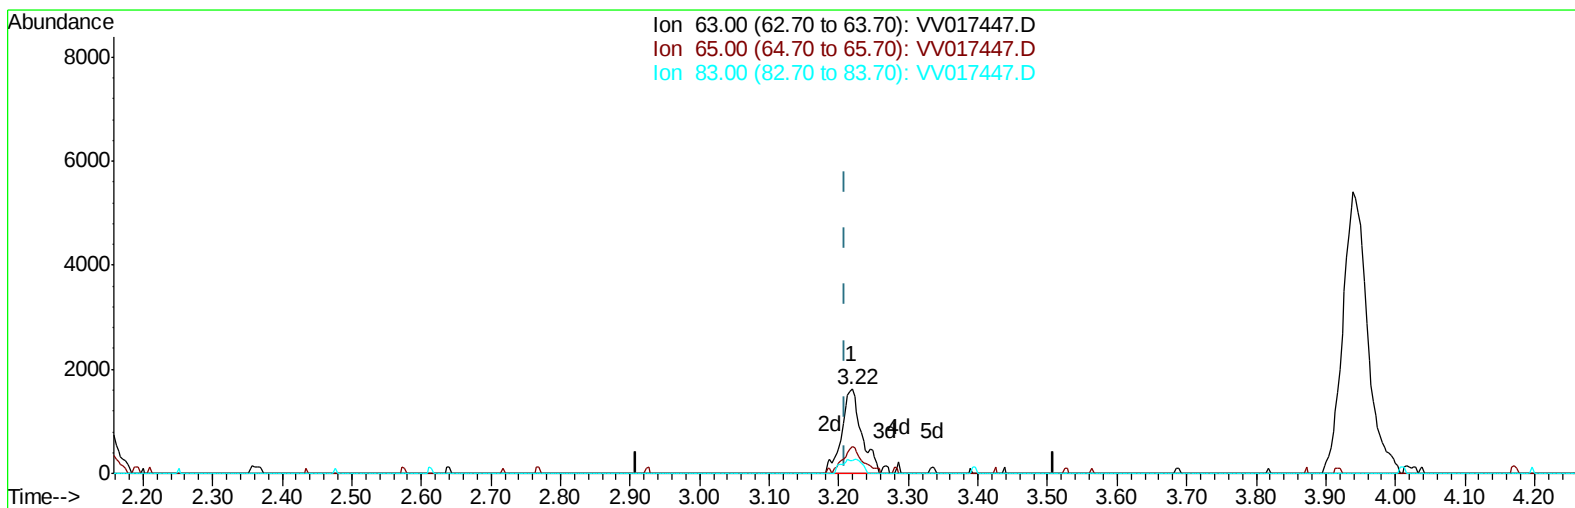

TIC: VV017447.D

(19) 1,1-Dichloroethane (T)

3.219min (+0.010) 1.01ug/L m

response 3222

Ion	Exp%	Act%
63.00	100	100
65.00	31.60	31.73
83.00	14.50	14.97
0.00	0.00	0.00