

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV071020\
 Data File : VV017433.D
 Acq On : 10 Jul 2020 12:37
 Operator : SY/MD
 Sample : L3264-04
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Quant Time: Jul 11 00:24:54 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM070820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jul 11 00:23:19 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	275808	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	261950	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	128642	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	59479	41.42	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	82.84%
7) Chloroethane-d5	1.58	69	43108	42.74	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	85.48%
11) 1,1-Dichloroethene-d2	2.12	63	101713	31.29	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	62.58%
21) 2-Butanone-d5	3.91	46	93031	94.86	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	94.86%
24) Chloroform-d	4.38	84	147741	44.48	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.96%
26) 1,2-Dichloroethane-d4	5.06	65	109532	48.05	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.10%
32) Benzene-d6	5.08	84	258785	45.73	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.46%
36) 1,2-Dichloropropane-d6	6.09	67	75455	46.31	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	92.62%
41) Toluene-d8	7.34	98	245656	45.16	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	90.32%
43) trans-1,3-Dichloropropene-	7.64	79	43969	46.36	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	92.72%
47) 2-Hexanone-d5	8.11	63	60386	90.30	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	90.30%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	98889	43.22	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	86.44%
64) 1,2-Dichlorobenzene-d4	11.65	152	104875	48.76	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	97.52%


Target Compounds					Ovalue
59) 1,2,3-Trichloropropane	11.27	75	11903	5.072 ug/L	# 75


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV071020\
Data File : VV017433.D
Acq On : 10 Jul 2020 12:37
Operator : SY/MD
Sample : L3264-04
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Time: Jul 11 00:24:54 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM070820WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jul 11 00:23:19 2020
Response via : Initial Calibration

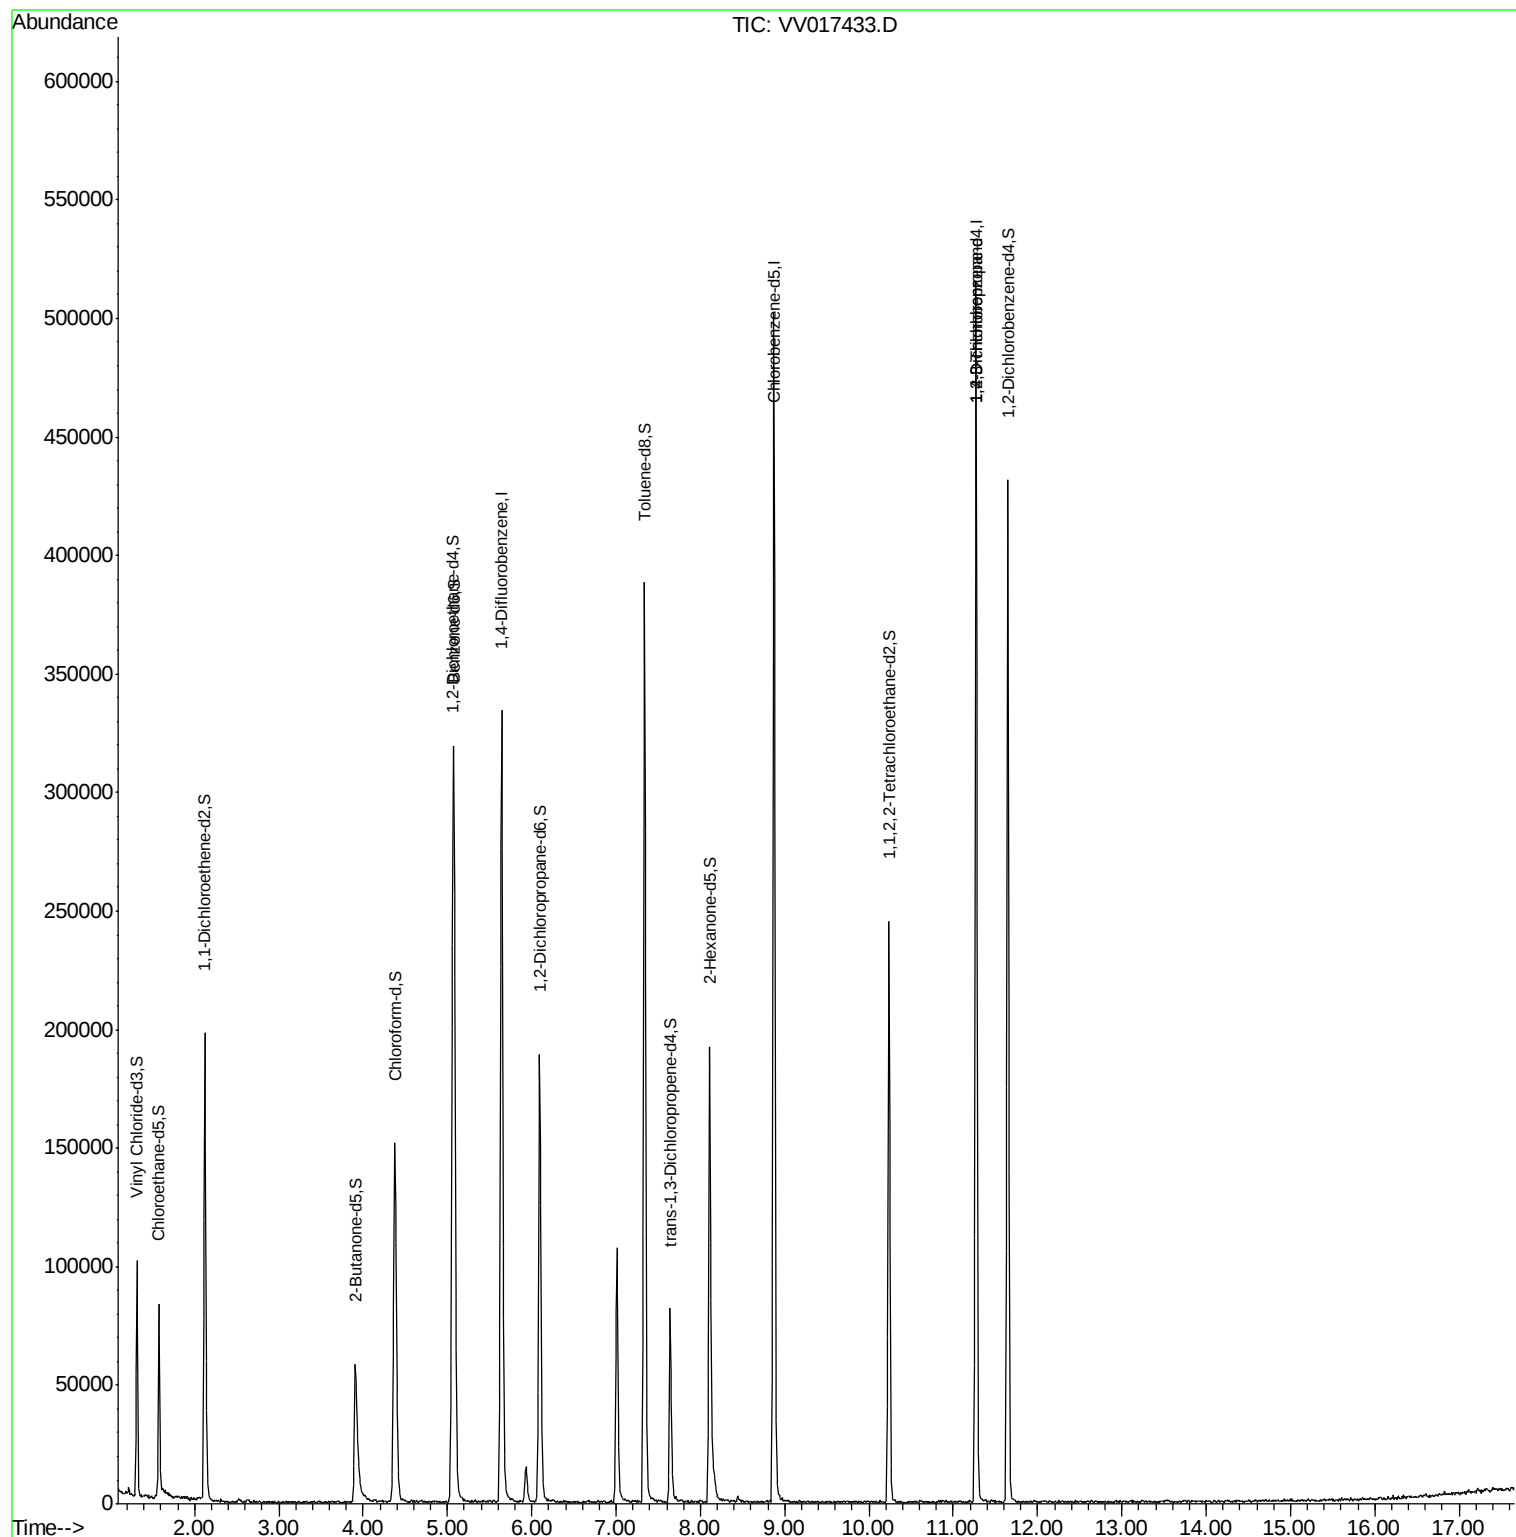

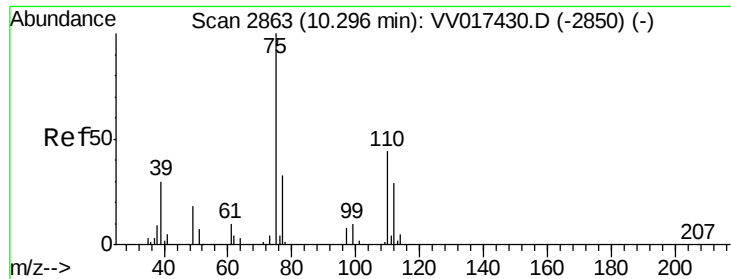

#59

1,2,3-Trichloropropane

Concen: 5.072 ug/L

RT: 11.27 min Scan# 3165

Delta R.T. 0.97 min

Lab File: VV017433.D

Acq: 10 Jul 2020 12:37

Instrument :

MSVOA_V

ClientSampleId :

VHBLK01

Tot Ion: 75 Resp: 11903

Ion Ratio Lower Upper

75 100

77 47.4 26.5 39.7#

