

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV071020\
 Data File : VV017447.D
 Acq On : 10 Jul 2020 18:02
 Operator : SY/MD
 Sample : L3270-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A06

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM070820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.123	313	321	339	rVB	178193	264710	33.84%	4.939%
2	2.296	371	375	380	rBV5	1029	1090	0.14%	0.020%
3	2.833	541	542	545	rBV3	408	251	0.03%	0.005%
4	2.872	551	554	555	rBV	892	396	0.05%	0.007%
5	2.917	566	568	569	rBV2	645	189	0.02%	0.004%
6	2.959	579	581	582	rBV	685	248	0.03%	0.005%
7	3.145	636	639	642	rBV2	691	648	0.08%	0.012%
8	3.312	688	691	692	rBV2	587	278	0.04%	0.005%
9	3.332	692	697	703	rVV5	902	975	0.12%	0.018%
10	3.454	732	735	739	rBV2	638	613	0.08%	0.011%
11	3.476	739	742	743	rBV2	810	292	0.04%	0.005%
12	3.505	750	751	752	rBV	332	68	0.01%	0.001%
13	3.717	816	817	818	rBV	482	143	0.02%	0.003%
14	3.769	830	833	840	rVB3	1205	946	0.12%	0.018%
15	3.801	840	843	844	rBV2	278	120	0.02%	0.002%
16	3.811	844	846	847	rBV	395	168	0.02%	0.003%
17	3.936	867	885	910	rBV2	82233	304607	38.94%	5.684%
18	4.669	1110	1113	1117	rBV3	798	645	0.08%	0.012%
19	4.756	1137	1140	1142	rBV2	723	537	0.07%	0.010%
20	4.795	1151	1152	1154	rVB2	568	178	0.02%	0.003%
21	5.000	1215	1216	1218	rVB	590	149	0.02%	0.003%
22	5.360	1326	1328	1330	rBV2	746	358	0.05%	0.007%
23	5.640	1402	1415	1440	rBV	327734	662308	84.67%	12.358%
24	6.093	1545	1556	1576	rBV	180909	362269	46.31%	6.760%
25	6.489	1677	1679	1680	rBV	781	385	0.05%	0.007%
26	6.547	1692	1697	1701	rBV4	1093	1194	0.15%	0.022%
27	6.891	1802	1804	1807	rBV2	723	477	0.06%	0.009%
28	7.007	1828	1840	1861	rBV	102681	194189	24.82%	3.623%
29	7.338	1932	1943	1972	rBV	372146	638365	81.61%	11.911%
30	7.843	2098	2100	2102	rBV2	705	394	0.05%	0.007%
31	8.061	2167	2168	2172	rBV3	574	434	0.06%	0.008%
32	8.109	2173	2183	2211	rBV	196103	366896	46.90%	6.846%
33	8.708	2367	2369	2370	rBV	516	201	0.03%	0.004%
34	8.872	2409	2420	2440	rBV	482013	782259	100.00%	14.596%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV071020\
 Data File : VV017447.D
 Acq On : 10 Jul 2020 18:02
 Operator : SY/MD
 Sample : L3270-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A06

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM070820WMA.M
 Title : VOC Analysis

35	9.338	2562	2565	2567	rBV	713	358	0.05%	0.007%
36	9.531	2624	2625	2627	rBV	644	245	0.03%	0.005%
37	9.572	2637	2638	2641	rBV2	574	304	0.04%	0.006%
38	9.823	2711	2716	2717	rBV2	303	304	0.04%	0.006%
39	10.048	2783	2786	2787	rBV2	523	225	0.03%	0.004%
40	10.238	2834	2845	2860	rBV	248067	382326	48.87%	7.134%
41	10.634	2967	2968	2970	rBV2	742	306	0.04%	0.006%
42	10.743	2998	3002	3003	rBV2	825	542	0.07%	0.010%
43	10.817	3023	3025	3026	rBV	947	424	0.05%	0.008%
44	11.138	3122	3125	3129	rVB4	931	749	0.10%	0.014%
45	11.161	3129	3132	3137	rBV3	994	825	0.11%	0.015%
46	11.187	3138	3140	3143	rVB2	818	338	0.04%	0.006%
47	11.206	3143	3146	3147	rBV	932	416	0.05%	0.008%
48	11.270	3156	3166	3186	rVB	493104	744258	95.14%	13.887%
49	11.646	3273	3283	3302	rVB	415415	639318	81.73%	11.929%
50	12.514	3552	3553	3554	rBV	487	138	0.02%	0.003%
51	12.611	3581	3583	3587	rBV2	776	507	0.06%	0.009%
52	13.810	3954	3956	3958	rBV2	822	379	0.05%	0.007%
53	14.293	4105	4106	4109	rBV	635	363	0.05%	0.007%


Sum of corrected areas: 5359305

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV071020\
Data File : VV017447.D
Acq On : 10 Jul 2020 18:02
Operator : SY/MD
Sample : L3270-05
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A06

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM070820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

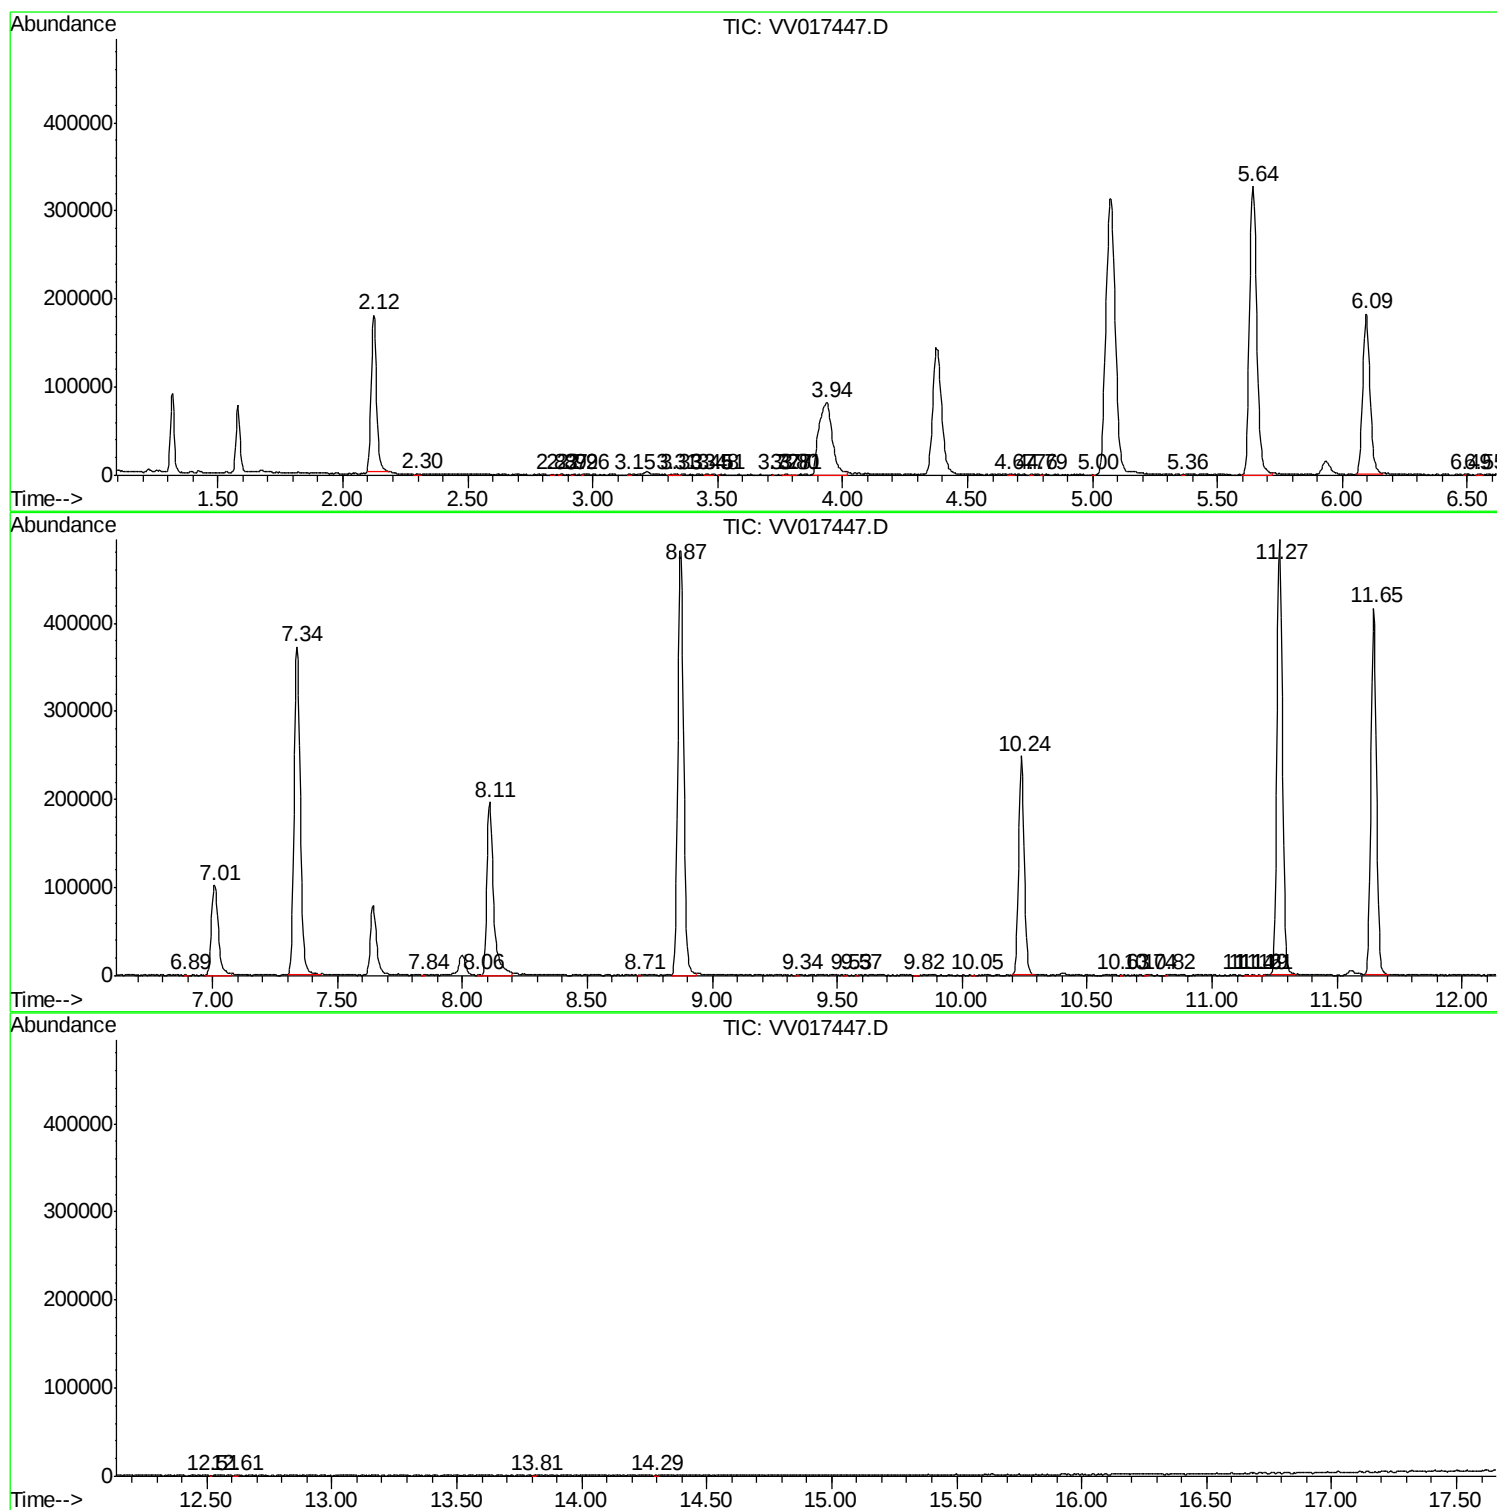

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV071020\
Data File : VV017447.D
Acq On : 10 Jul 2020 18:02
Operator : SY/MD
Sample : L3270-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A06

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM070820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV071020\
Data File : VV017447.D
Acq On : 10 Jul 2020 18:02
Operator : SY/MD
Sample : L3270-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A06

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM070820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc