


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV071020\
 Data File : VV017429.D
 Acq On : 10 Jul 2020 10:31
 Operator : SY/MD
 Sample : BFB99
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB99

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM070820WMA.M
 Title : VOC Analysis
 Last Update : Mon Jul 13 06:24:40 2020

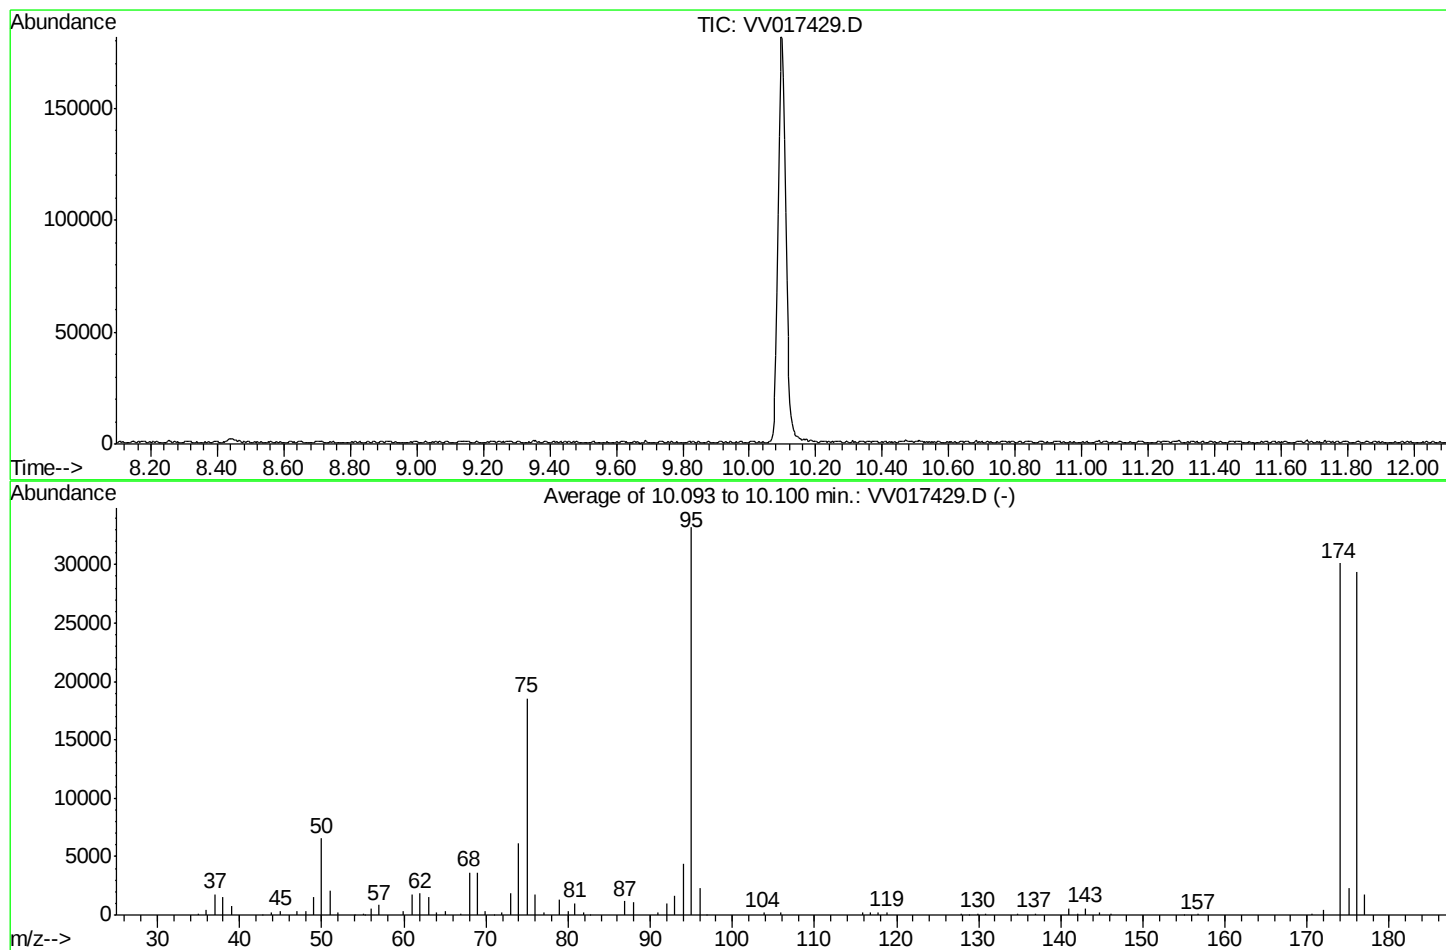

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2789

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	6570	PASS
75	95	30	80	55.9	18570	PASS
95	95	100	100	100.0	33192	PASS
96	95	5	9	6.9	2281	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	90.7	30093	PASS
175	174	5	9	7.8	2353	PASS
176	174	95	101	97.5	29346	PASS
177	176	5	9	5.9	1740	PASS

Scan 2789 (10.058 min): VV017429.D
BFB99

m/z	Abundance
39.20	122.0
39.90	170.0
41.60	108.0
43.90	186.0

Instrument :
MSVOA_V
ClientSampleId :
BFB99

m/z	Abundance
35.00	175.0
35.90	353.0
37.00	1822.0
38.00	1489.0
39.00	732.0
39.90	143.0
43.90	331.0
45.00	403.0
46.90	359.0
48.00	289.0
49.00	1527.0
50.00	6286.0
51.00	2028.0
52.00	194.0
54.00	130.0
55.10	137.0
56.00	476.0
57.00	852.0
59.90	321.0
61.00	1655.0
62.00	1962.0
63.00	1591.0
64.00	214.0
65.10	373.0
67.00	152.0
68.00	3323.0
69.00	3269.0
69.90	326.0
70.90	120.0
72.00	190.0
73.10	1720.0
74.00	5727.0
75.00	17848.0
76.00	1517.0
77.00	228.0
78.90	1209.0
79.90	300.0
80.90	980.0
81.90	243.0
82.70	109.0
86.90	1169.0
87.90	913.0
90.90	185.0
91.90	981.0
93.00	1602.0
94.00	4325.0
95.00	31208.0
96.00	2217.0
103.80	177.0
105.80	226.0
115.90	179.0
116.80	261.0
117.70	189.0
118.90	242.0
127.80	101.0
128.80	112.0
130.10	134.0
130.90	118.0
134.80	129.0
136.80	183.0
140.90	533.0
142.10	136.0
143.00	561.0
144.60	186.0
170.60	117.0
172.00	364.0
174.00	27896.0
175.10	2220.0
176.00	26800.0
176.90	1664.0

Instrument :
MSVOA_V
ClientSampleId :
BFB99

m/z	Abundance
35.00	166.0
35.90	450.0
37.00	1810.0
38.00	1552.0
39.00	882.0
39.80	160.0
43.90	376.0
45.00	372.0
47.00	328.0
48.00	298.0
49.00	1573.0
50.00	6864.0
51.00	2194.0
52.00	205.0
55.10	120.0
56.00	537.0
57.00	888.0
60.00	353.0
61.00	1866.0
62.00	1905.0
63.00	1574.0
64.00	272.0
65.00	384.0
68.00	3735.0
69.00	3723.0
69.90	345.0
72.00	223.0
73.00	1965.0
74.00	6403.0
75.00	19160.0
76.00	1833.0
77.00	190.0
78.90	1308.0
80.00	325.0
80.80	1050.0
81.90	245.0
86.90	1154.0
88.00	1094.0
90.90	178.0
92.00	971.0
93.00	1715.0
94.00	4528.0
95.00	34416.0
96.00	2304.0
103.90	215.0
105.80	180.0
115.90	198.0
116.80	242.0
117.80	176.0
118.80	275.0
127.80	146.0
129.90	166.0
130.80	140.0
134.80	103.0
136.80	163.0
140.90	525.0
142.10	125.0
143.00	568.0
144.60	182.0
146.10	114.0
156.80	124.0
170.60	125.0
172.00	412.0
174.00	31048.0
175.10	2410.0
176.00	30440.0
177.00	1762.0

Instrument :
MSVOA_V
ClientSampleId :
BFB99

m/z	Abundance
35.00	138.0
36.00	453.0
37.10	1693.0
38.00	1540.0
39.00	916.0
39.90	171.0
42.80	113.0
43.90	384.0
45.00	315.0
47.00	331.0
48.00	269.0
49.00	1426.0
50.00	6562.0
51.00	2093.0
52.00	175.0
55.00	104.0
55.30	121.0
56.00	512.0
57.00	839.0
59.90	413.0
61.00	1901.0
62.00	1611.0
63.00	1544.0
64.00	278.0
65.00	352.0
67.00	106.0
68.00	3900.0
69.00	3831.0
69.90	379.0
71.90	217.0
73.00	2024.0
74.00	6395.0
75.00	18704.0
76.00	1880.0
77.00	167.0
78.80	1341.0
80.00	364.0
80.80	1068.0
81.90	286.0
86.90	1168.0
88.00	1157.0
90.90	143.0
91.90	1008.0
93.00	1646.0
94.00	4476.0
95.00	33952.0
96.00	2324.0
96.80	121.0
103.90	234.0
105.90	158.0
115.80	170.0
116.90	292.0
117.90	195.0
118.80	296.0
127.80	182.0
129.80	180.0
130.70	132.0
136.90	125.0
140.90	496.0
143.00	533.0
144.70	173.0
146.10	110.0
155.00	132.0
156.70	106.0
172.00	445.0
174.00	31336.0
175.10	2430.0
176.00	30800.0
176.90	1795.0

Instrument :
MSVOA_V
ClientSampleId :
BFB99