

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW071023\
 Data File : VW031662.D
 Acq On : 10 Jul 2023 13:21
 Operator : SY/MD
 Sample : 03551-02ME
 Misc : 7.41g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCHB1ME

Quant Time: Jul 11 01:07:50 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 07 02:34:55 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.539	114	174308	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.793	117	190308	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	93483	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	39329	33.902	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	67.800%
7) Chloroethane-d5	1.519	69	17306	17.097	ug/L	-0.01
Spiked Amount	50.000	Range	70 - 130	Recovery	=	34.200%#
11) 1,1-Dichloroethene-d2	2.044	65	17726	29.648	ug/L	-0.02
Spiked Amount	50.000	Range	60 - 125	Recovery	=	59.300%#
21) 2-Butanone-d5	3.812	46	88696	94.423	ug/L	0.02
Spiked Amount	100.000	Range	40 - 130	Recovery	=	94.420%
24) Chloroform-d	4.256	84	111509	38.381	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	76.760%
26) 1,2-Dichloroethane-d4	4.947	65	74728	41.110	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	82.220%
32) Benzene-d6	4.963	84	167806	31.326	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	62.660%#
36) 1,2-Dichloropropane-d6	5.995	67	67326	35.461	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	70.920%
41) Toluene-d8	7.249	98	132077	26.869	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	53.740%#
43) trans-1,3-Dichloroprop...	7.561	79	30164	32.590	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	65.180%
47) 2-Hexanone-d5	8.063	63	57921	77.266	ug/L	0.03
Spiked Amount	100.000	Range	45 - 130	Recovery	=	77.270%
56) 1,1,2,2-Tetrachloroeth...	10.165	84	114825	40.068	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	80.140%
66) 1,2-Dichlorobenzene-d4	11.571	152	69067	38.759	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	77.520%#
Target Compounds						Qvalue
13) Acetone	2.134	43	14434	15.572	ug/L	99
61) 1,2,3-Trichloropropane	11.194	75	11167	6.048	ug/L #	64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071023\
Data File : VV031662.D
Acq On : 10 Jul 2023 13:21
Operator : SY/MD
Sample : 03551-02ME
Misc : 7.41g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCHB1ME

Quant Time: Jul 11 01:07:50 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jul 07 02:34:55 2023
Response via : Initial Calibration

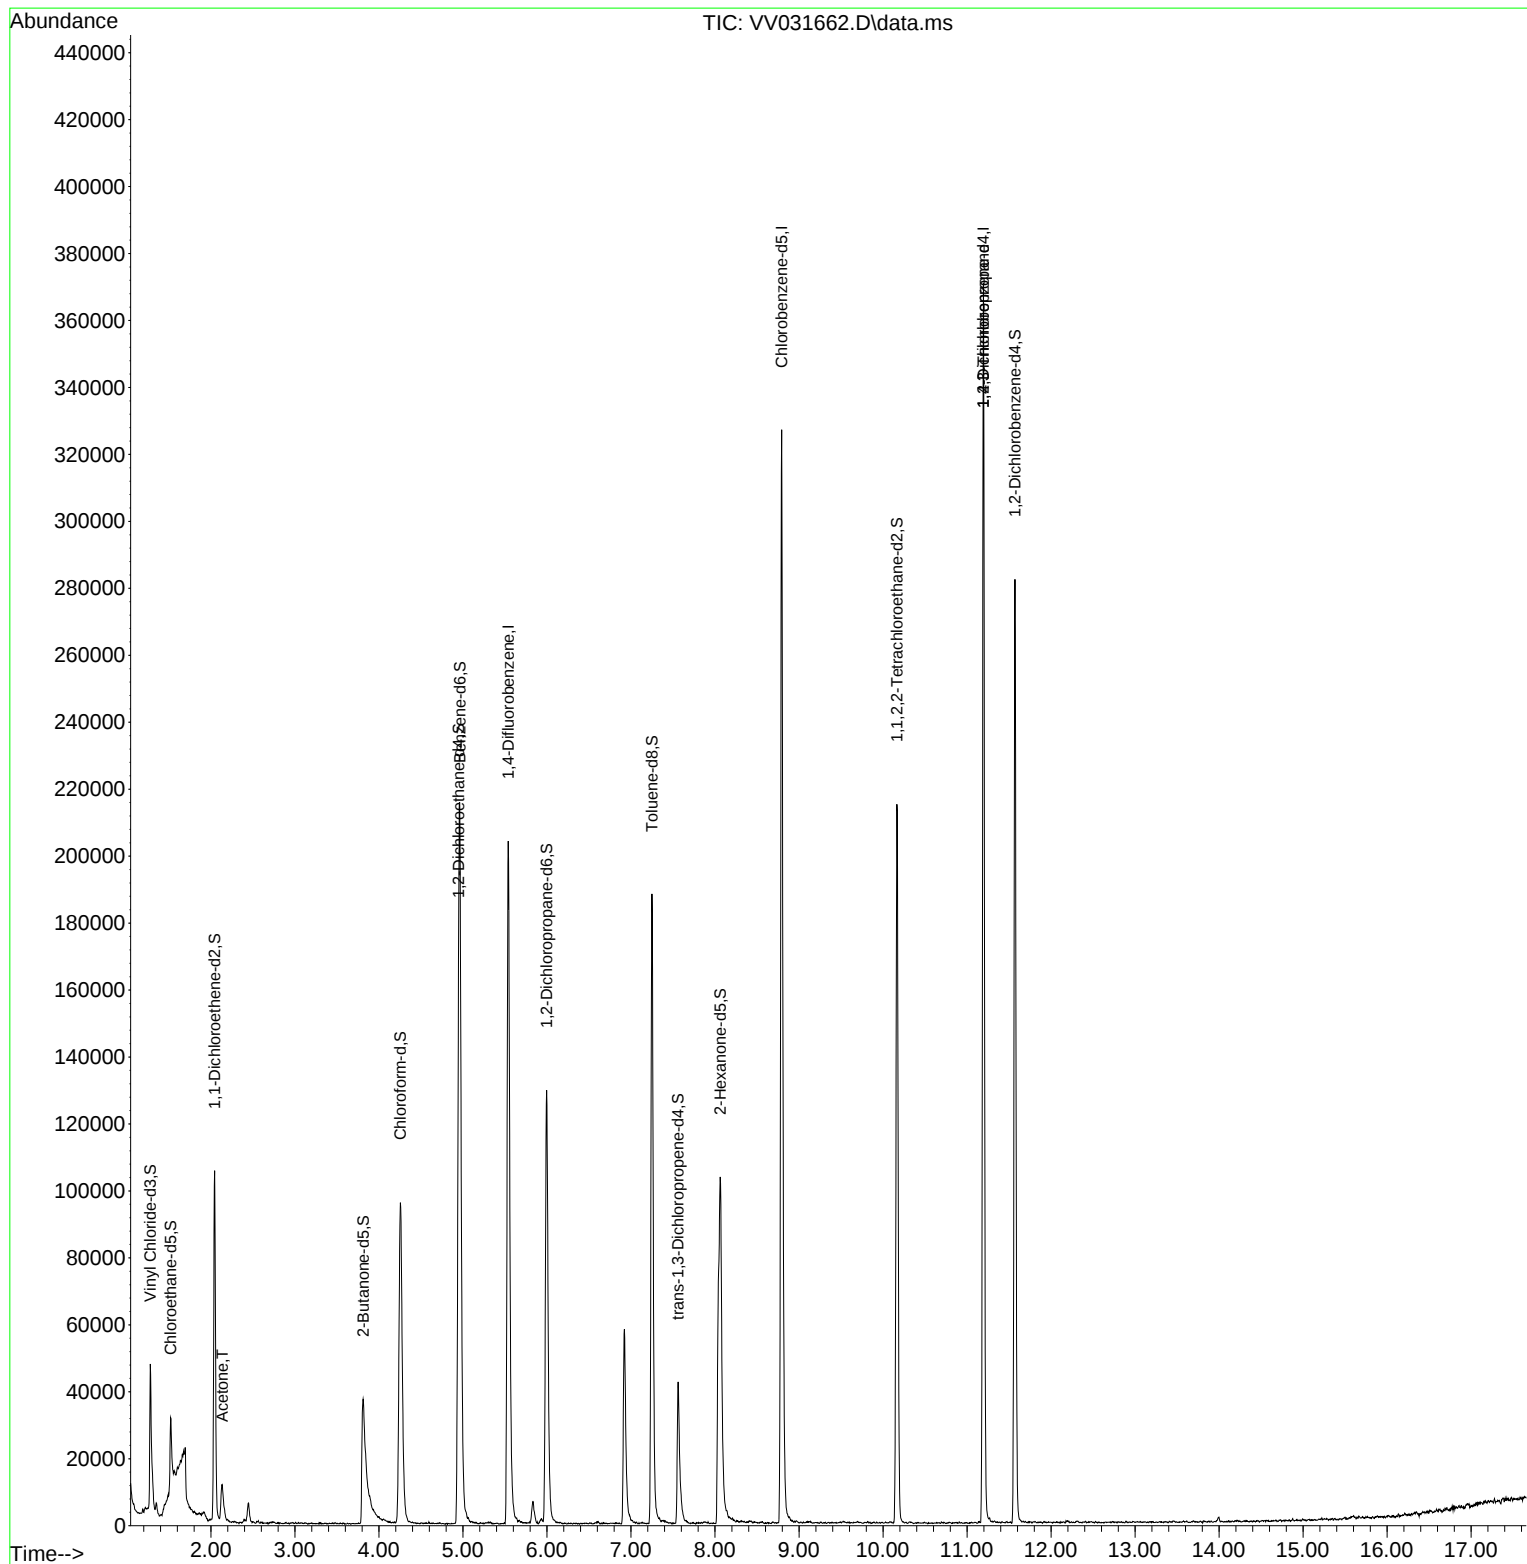

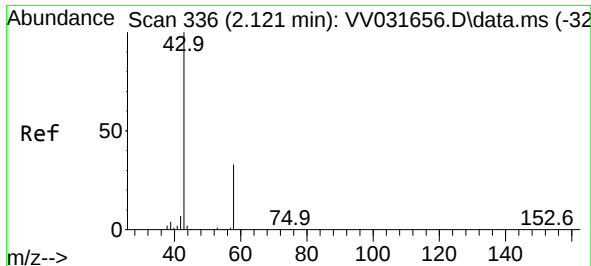

#13

Acetone

Concen: 15.572 ug/L

RT: 2.134 min Scan# 34

Delta R.T. 0.019 min

Lab File: VV031662.D

Acq: 10 Jul 2023 13:21

Instrument :

MSVOA_V

ClientSampleId :





DCHB1ME

Tgt Ion: 43 Resp: 14434

Ion Ratio Lower Upper

43 100

58 33.8 0.0 68.6

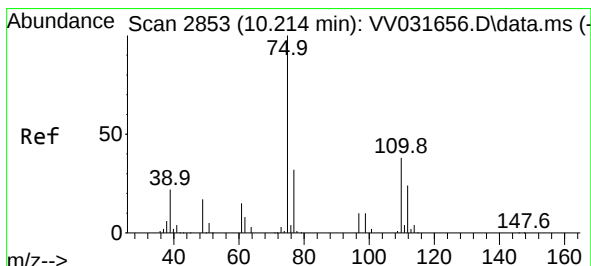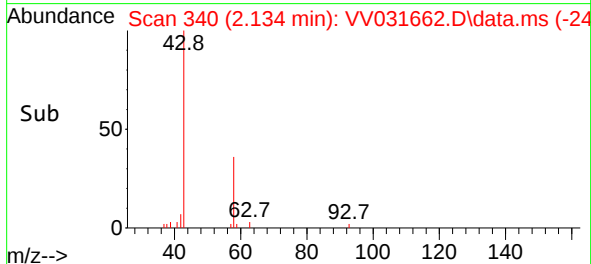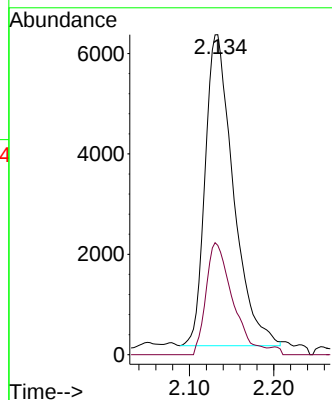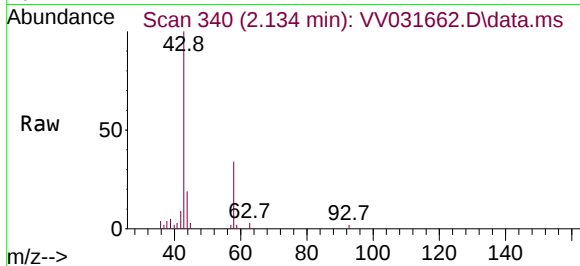

#61

1,2,3-Trichloropropane

Concen: 6.048 ug/L

RT: 11.194 min Scan# 3158

Delta R.T. 0.981 min

Lab File: VV031662.D

Acq: 10 Jul 2023 13:21

Tgt Ion: 75 Resp: 11167

Ion Ratio Lower Upper

75 100

77 35.2 25.4 38.0

110 2.4 31.3 46.9#

