

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071023\
 Data File : VV031658.D
 Acq On : 10 Jul 2023 11:20
 Operator : SY/MD
 Sample : VV0710WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK367

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M

Title : VOC Analysis

Signal : TIC: VV031658.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	91	rVB	107885	117659	16.41%	2.171%
2	1.532	146	153	167	rVB	82403	96772	13.50%	1.785%
3	2.063	307	318	332	rBV	167278	245070	34.18%	4.521%
4	2.339	402	404	409	rBV2	267	304	0.04%	0.006%
5	2.388	416	419	426	rVB3	440	413	0.06%	0.008%
6	2.452	429	439	448	rVB5	3303	5775	0.81%	0.107%
7	2.507	448	456	460	rBV	377	437	0.06%	0.008%
8	2.603	483	486	489	rBV	301	225	0.03%	0.004%
9	2.873	563	570	577	rBV2	272	417	0.06%	0.008%
10	2.979	600	603	607	rBV2	277	208	0.03%	0.004%
11	3.034	615	620	623	rVB	308	202	0.03%	0.004%
12	3.053	623	626	630	rBV2	327	296	0.04%	0.005%
13	3.082	630	635	638	rBV2	242	225	0.03%	0.004%
14	3.252	684	688	691	rVB2	325	208	0.03%	0.004%
15	3.359	718	721	724	rBV2	254	208	0.03%	0.004%
16	3.478	753	758	763	rBV	382	361	0.05%	0.007%
17	3.645	806	810	812	rBV	320	248	0.03%	0.005%
18	3.699	823	827	829	rVB	357	231	0.03%	0.004%
19	3.732	834	837	839	rBV	369	276	0.04%	0.005%
20	3.796	847	857	899	rBV	41892	123009	17.15%	2.269%
21	3.979	911	914	917	rBV3	605	388	0.05%	0.007%
22	4.252	983	999	1026	rBV2	116948	297697	41.52%	5.492%
23	4.478	1066	1069	1072	rVB3	508	366	0.05%	0.007%
24	4.497	1072	1075	1078	rBV2	491	387	0.05%	0.007%
25	4.561	1091	1095	1098	rBV2	364	213	0.03%	0.004%
26	4.600	1103	1107	1113	rVB	274	259	0.04%	0.005%
27	4.857	1183	1187	1191	rBV	300	280	0.04%	0.005%
28	4.960	1202	1219	1246	rBV2	270478	717058	100.00%	13.229%
29	5.240	1304	1306	1312	rVB2	488	356	0.05%	0.007%
30	5.539	1386	1399	1423	rBV	220521	445092	62.07%	8.211%
31	5.738	1459	1461	1464	rVB	473	234	0.03%	0.004%
32	5.831	1479	1490	1504	rBV3	4856	9858	1.37%	0.182%
33	5.992	1527	1540	1566	rBV	166278	345543	48.19%	6.375%
34	6.143	1584	1587	1589	rVB3	488	245	0.03%	0.005%
35	6.175	1593	1597	1604	rBV4	312	409	0.06%	0.008%
36	6.342	1646	1649	1658	rVB2	479	625	0.09%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071023\
 Data File : VV031658.D
 Acq On : 10 Jul 2023 11:20
 Operator : SY/MD
 Sample : VV0710WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK367

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

37	6.381	1658	1661	1664	rBV2	354	260	0.04%	0.005%
38	6.490	1692	1695	1701	rVB2	366	434	0.06%	0.008%
39	6.513	1701	1702	1708	rBV2	344	311	0.04%	0.006%
40	6.558	1710	1716	1719	rBV2	289	331	0.05%	0.006%
41	6.838	1800	1803	1806	rVB2	353	236	0.03%	0.004%
42	6.857	1806	1809	1813	rBV2	322	233	0.03%	0.004%
43	6.918	1817	1828	1848	rBV	78367	145840	20.34%	2.691%
44	7.121	1887	1891	1893	rBV	432	365	0.05%	0.007%
45	7.188	1909	1912	1917	rVV4	297	301	0.04%	0.006%
46	7.249	1919	1931	1966	rVV	284648	509055	70.99%	9.391%
47	7.558	2016	2027	2047	rBV	58912	106688	14.88%	1.968%
48	7.821	2104	2109	2110	rBV	516	383	0.05%	0.007%
49	7.841	2113	2115	2121	rVB	388	346	0.05%	0.006%
50	7.879	2121	2127	2129	rBV3	582	633	0.09%	0.012%
51	8.030	2158	2174	2201	rBV	137397	261929	36.53%	4.832%
52	8.259	2243	2245	2248	rVB2	531	254	0.04%	0.005%
53	8.365	2275	2278	2281	rVB2	345	220	0.03%	0.004%
54	8.526	2326	2328	2333	rVB2	351	303	0.04%	0.006%
55	8.558	2333	2338	2339	rBV2	346	246	0.03%	0.005%
56	8.722	2387	2389	2395	rVB2	371	285	0.04%	0.005%
57	8.789	2399	2410	2435	rBV	340981	562934	78.51%	10.385%
58	8.953	2458	2461	2463	rBV3	446	294	0.04%	0.005%
59	9.217	2539	2543	2548	rBV2	402	367	0.05%	0.007%
60	9.516	2633	2636	2639	rVB3	358	269	0.04%	0.005%
61	9.545	2639	2645	2646	rBV2	386	297	0.04%	0.005%
62	9.590	2653	2659	2663	rBV2	327	413	0.06%	0.008%
63	9.612	2663	2666	2670	rVV2	350	263	0.04%	0.005%
64	9.722	2697	2700	2703	rVB	286	205	0.03%	0.004%
65	10.159	2824	2836	2851	rBV	219349	348047	48.54%	6.421%
66	10.278	2870	2873	2876	rBV	270	226	0.03%	0.004%
67	10.368	2898	2901	2906	rVB3	244	215	0.03%	0.004%
68	10.439	2920	2923	2927	rVV2	395	287	0.04%	0.005%
69	10.484	2933	2937	2939	rBV2	567	400	0.06%	0.007%
70	10.751	3016	3020	3026	rVB2	450	450	0.06%	0.008%
71	10.834	3042	3046	3047	rBV2	364	212	0.03%	0.004%
72	11.117	3131	3134	3137	rBV	298	267	0.04%	0.005%
73	11.191	3146	3157	3178	rBV	371944	571117	79.65%	10.536%
74	11.407	3221	3224	3226	rBV2	374	217	0.03%	0.004%
75	11.567	3262	3274	3288	rBV	305650	483086	67.37%	8.912%
76	11.712	3315	3319	3321	rBV3	464	408	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071023\
 Data File : VV031658.D
 Acq On : 10 Jul 2023 11:20
 Operator : SY/MD
 Sample : VV0710WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK367

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

77	11.812	3347	3350	3353	rBV	443	273	0.04%	0.005%
78	11.931	3385	3387	3391	rVB2	510	300	0.04%	0.006%
79	12.079	3431	3433	3438	rBV2	286	259	0.04%	0.005%
80	12.468	3551	3554	3557	rVB2	402	242	0.03%	0.004%
81	12.535	3573	3575	3579	rVB2	417	235	0.03%	0.004%
82	12.622	3599	3602	3605	rVB3	451	283	0.04%	0.005%
83	12.683	3619	3621	3625	rVB2	550	295	0.04%	0.005%
84	12.767	3644	3647	3650	rBV	441	281	0.04%	0.005%
85	12.902	3685	3689	3692	rBV	361	303	0.04%	0.006%
86	13.159	3767	3769	3774	rBV2	412	361	0.05%	0.007%
87	13.214	3781	3786	3789	rBV3	698	568	0.08%	0.010%
88	13.287	3805	3809	3813	rVB4	484	479	0.07%	0.009%
89	13.320	3816	3819	3825	rVV2	388	424	0.06%	0.008%
90	13.693	3933	3935	3937	rBV	687	326	0.05%	0.006%
91	13.783	3961	3963	3966	rBV	334	251	0.04%	0.005%
92	13.834	3975	3979	3980	rBV	342	236	0.03%	0.004%
93	13.844	3980	3982	3985	rVB	448	228	0.03%	0.004%
94	13.879	3991	3993	3996	rVB	742	336	0.05%	0.006%
95	13.902	3996	4000	4002	rBV2	817	594	0.08%	0.011%
96	13.992	4021	4028	4040	rVB3	1670	2824	0.39%	0.052%
97	14.246	4104	4107	4108	rBV2	356	203	0.03%	0.004%
98	14.718	4252	4254	4258	rVB2	478	350	0.05%	0.006%
99	14.738	4258	4260	4262	rBV3	392	216	0.03%	0.004%
100	15.204	4402	4405	4409	rBV3	531	403	0.06%	0.007%




Sum of corrected areas: 5420451

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071023\
Data File : VV031658.D
Acq On : 10 Jul 2023 11:20
Operator : SY/MD
Sample : VV0710WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK367

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

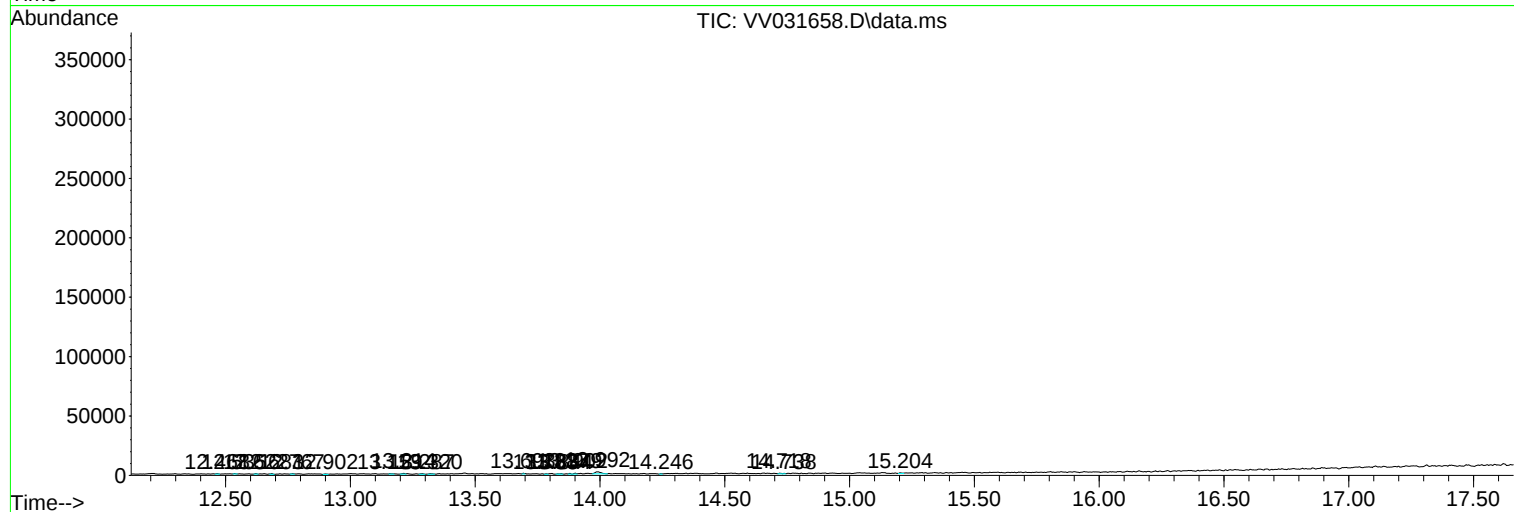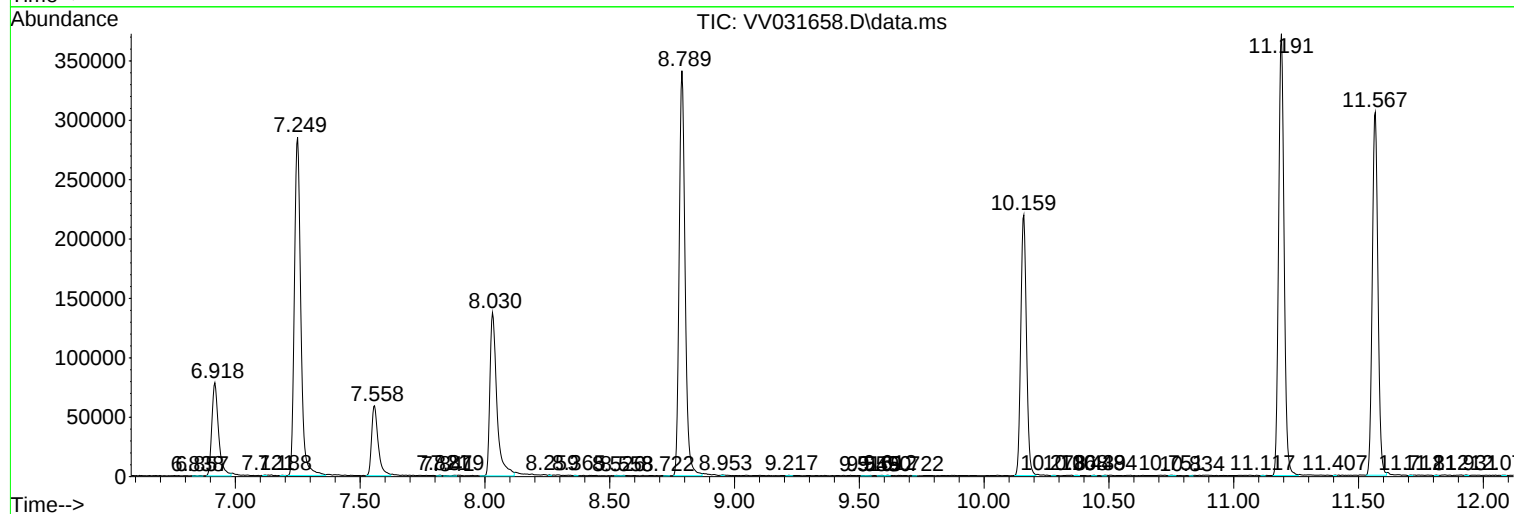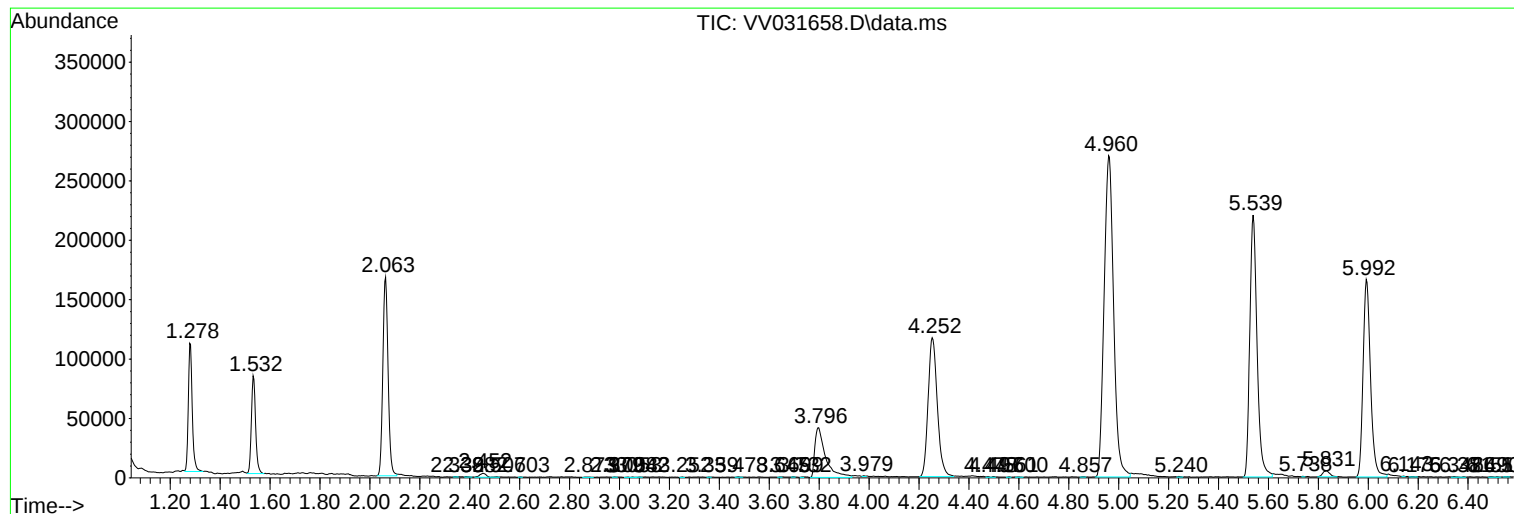

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071023\
Data File : VV031658.D
Acq On : 10 Jul 2023 11:20
Operator : SY/MD
Sample : VV0710WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK367

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071023\
Data File : VV031658.D
Acq On : 10 Jul 2023 11:20
Operator : SY/MD
Sample : VV0710WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK367

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------