

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071023\
 Data File : VV031662.D
 Acq On : 10 Jul 2023 13:21
 Operator : SY/MD
 Sample : 03551-02ME
 Misc : 7.41g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCHB1ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

Signal : TIC: VV031662.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	91	rVB	43514	64010	10.78%	1.320%
2	1.519	144	149	159	rBV	21179	31119	5.24%	0.642%
3	2.044	302	312	330	rBV	104103	153893	25.92%	3.173%
4	2.134	330	340	356	rVB	10608	23180	3.90%	0.478%
5	2.262	374	380	382	rBV3	326	323	0.05%	0.007%
6	2.343	402	405	407	rBV2	488	360	0.06%	0.007%
7	2.394	415	421	424	rBV5	1040	1044	0.18%	0.022%
8	2.446	428	437	446	rVB3	5547	9398	1.58%	0.194%
9	2.500	451	454	457	rBV2	318	254	0.04%	0.005%
10	2.545	465	468	470	rBV3	476	298	0.05%	0.006%
11	2.671	505	507	510	rVB3	485	286	0.05%	0.006%
12	2.690	510	513	514	rBV	411	230	0.04%	0.005%
13	2.703	514	517	520	rVV3	361	299	0.05%	0.006%
14	2.732	524	526	531	rBV2	405	349	0.06%	0.007%
15	2.822	551	554	562	rBV2	312	366	0.06%	0.008%
16	2.892	572	576	580	rVB4	334	258	0.04%	0.005%
17	2.944	588	592	594	rBV2	311	256	0.04%	0.005%
18	2.966	595	599	601	rVV2	404	336	0.06%	0.007%
19	3.008	607	612	616	rVB3	397	308	0.05%	0.006%
20	3.163	657	660	664	rBV	310	279	0.05%	0.006%
21	3.288	696	699	702	rBV2	419	223	0.04%	0.005%
22	3.307	702	705	709	rVB	490	341	0.06%	0.007%
23	3.622	799	803	808	rBV3	284	221	0.04%	0.005%
24	3.812	849	862	885	rBV	37166	123469	20.79%	2.546%
25	4.256	982	1000	1030	rBV2	95685	262825	44.26%	5.419%
26	4.462	1062	1064	1072	rVB2	253	216	0.04%	0.004%
27	4.507	1075	1078	1084	rVB2	309	333	0.06%	0.007%
28	4.725	1144	1146	1152	rVB3	339	255	0.04%	0.005%
29	4.806	1166	1171	1174	rVB	333	281	0.05%	0.006%
30	4.960	1203	1219	1248	rBV2	215377	553893	93.28%	11.420%
31	5.204	1290	1295	1296	rBV3	354	218	0.04%	0.004%
32	5.269	1310	1315	1316	rBV	352	258	0.04%	0.005%
33	5.323	1327	1332	1336	rVV4	522	467	0.08%	0.010%
34	5.539	1387	1399	1425	rBV	203890	443936	74.76%	9.153%
35	5.831	1480	1490	1505	rBV5	6517	13851	2.33%	0.286%
36	5.886	1505	1507	1510	rVB2	576	232	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW071023\
 Data File : VW031662.D
 Acq On : 10 Jul 2023 13:21
 Operator : SY/MD
 Sample : 03551-02ME
 Misc : 7.41g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCHB1ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

37	5.921	1510	1518	1519	rBV	1133	1112	0.19%	0.023%
38	5.995	1528	1541	1567	rBV	128885	279553	47.08%	5.764%
39	6.156	1589	1591	1598	rVB3	425	381	0.06%	0.008%
40	6.281	1629	1630	1637	rVB2	269	251	0.04%	0.005%
41	6.375	1656	1659	1663	rVB2	283	222	0.04%	0.005%
42	6.404	1663	1668	1671	rBV2	329	357	0.06%	0.007%
43	6.609	1730	1732	1735	rVV3	526	302	0.05%	0.006%
44	6.645	1739	1743	1746	rBV3	341	280	0.05%	0.006%
45	6.818	1794	1797	1802	rBV2	303	279	0.05%	0.006%
46	6.921	1817	1829	1856	rBV2	58175	122590	20.64%	2.528%
47	7.063	1870	1873	1878	rVB2	531	493	0.08%	0.010%
48	7.121	1884	1891	1894	rBV3	293	365	0.06%	0.008%
49	7.137	1894	1896	1900	rVV2	322	224	0.04%	0.005%
50	7.249	1919	1931	1958	rBV	188106	350291	58.99%	7.222%
51	7.404	1977	1979	1983	rVB3	504	309	0.05%	0.006%
52	7.561	2016	2028	2054	rBV2	42326	88903	14.97%	1.833%
53	7.789	2096	2099	2103	rVV2	261	240	0.04%	0.005%
54	7.873	2118	2125	2126	rBV2	456	495	0.08%	0.010%
55	7.918	2136	2139	2145	rVB3	516	330	0.06%	0.007%
56	8.063	2167	2184	2206	rBV	103601	312249	52.58%	6.438%
57	8.410	2288	2292	2293	rBV2	399	322	0.05%	0.007%
58	8.539	2329	2332	2335	rBV2	283	217	0.04%	0.004%
59	8.561	2336	2339	2344	rVB2	419	347	0.06%	0.007%
60	8.629	2355	2360	2362	rBV2	396	278	0.05%	0.006%
61	8.693	2373	2380	2384	rBV3	402	620	0.10%	0.013%
62	8.793	2399	2411	2438	rBV	326495	593807	100.00%	12.243%
63	8.969	2462	2466	2475	rVB3	610	807	0.14%	0.017%
64	9.252	2551	2554	2557	rBV3	385	302	0.05%	0.006%
65	9.313	2571	2573	2577	rVB	411	215	0.04%	0.004%
66	9.526	2633	2639	2642	rBV	475	528	0.09%	0.011%
67	9.622	2666	2669	2675	rBV	214	225	0.04%	0.005%
68	9.818	2728	2730	2734	rVB3	511	333	0.06%	0.007%
69	9.844	2735	2738	2742	rVB2	463	369	0.06%	0.008%
70	9.870	2742	2746	2748	rBV3	326	218	0.04%	0.004%
71	10.165	2826	2838	2860	rVV	214637	374067	62.99%	7.713%
72	10.313	2880	2884	2885	rBV2	343	223	0.04%	0.005%
73	10.493	2937	2940	2945	rVB2	306	272	0.05%	0.006%
74	10.542	2953	2955	2960	rBV	407	301	0.05%	0.006%
75	10.696	2999	3003	3006	rBV2	463	331	0.06%	0.007%
76	10.725	3010	3012	3018	rVB2	359	292	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071023\
 Data File : VV031662.D
 Acq On : 10 Jul 2023 13:21
 Operator : SY/MD
 Sample : 03551-02ME
 Misc : 7.41g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCHB1ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

77	11.194	3147	3158	3177	rBV	370169	578564	97.43%	11.929%
78	11.416	3223	3227	3231	rBV2	405	468	0.08%	0.010%
79	11.571	3262	3275	3292	rBV	281960	441047	74.27%	9.094%
80	11.789	3338	3343	3346	rBV2	408	462	0.08%	0.010%
81	12.178	3461	3464	3467	rBV3	694	545	0.09%	0.011%
82	12.194	3467	3469	3473	rVB3	403	334	0.06%	0.007%
83	12.378	3523	3526	3528	rBV	303	244	0.04%	0.005%
84	12.413	3534	3537	3541	rVB2	464	344	0.06%	0.007%
85	12.529	3569	3573	3576	rBV2	454	364	0.06%	0.008%
86	12.796	3653	3656	3658	rBV2	357	261	0.04%	0.005%
87	12.892	3682	3686	3689	rBV2	487	412	0.07%	0.008%
88	13.062	3736	3739	3745	rVB2	343	254	0.04%	0.005%
89	13.172	3770	3773	3775	rBV3	322	247	0.04%	0.005%
90	13.207	3781	3784	3789	rBV	299	266	0.04%	0.005%
91	13.972	4019	4022	4023	rBV3	466	280	0.05%	0.006%
92	13.998	4024	4030	4035	rVB3	1445	1836	0.31%	0.038%
93	14.095	4057	4060	4062	rBV	337	218	0.04%	0.004%
94	14.114	4064	4066	4071	rVB2	476	316	0.05%	0.007%
95	14.214	4094	4097	4102	rVB3	449	341	0.06%	0.007%
96	14.490	4180	4183	4186	rBV	334	291	0.05%	0.006%
97	14.564	4203	4206	4209	rBV3	400	326	0.05%	0.007%
98	14.792	4274	4277	4280	rBV	421	372	0.06%	0.008%
99	15.371	4454	4457	4459	rBV3	559	383	0.06%	0.008%
100	15.660	4545	4547	4556	rBV4	741	733	0.12%	0.015%


Sum of corrected areas: 4850073

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071023\
Data File : VV031662.D
Acq On : 10 Jul 2023 13:21
Operator : SY/MD
Sample : 03551-02ME
Misc : 7.41g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCHB1ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

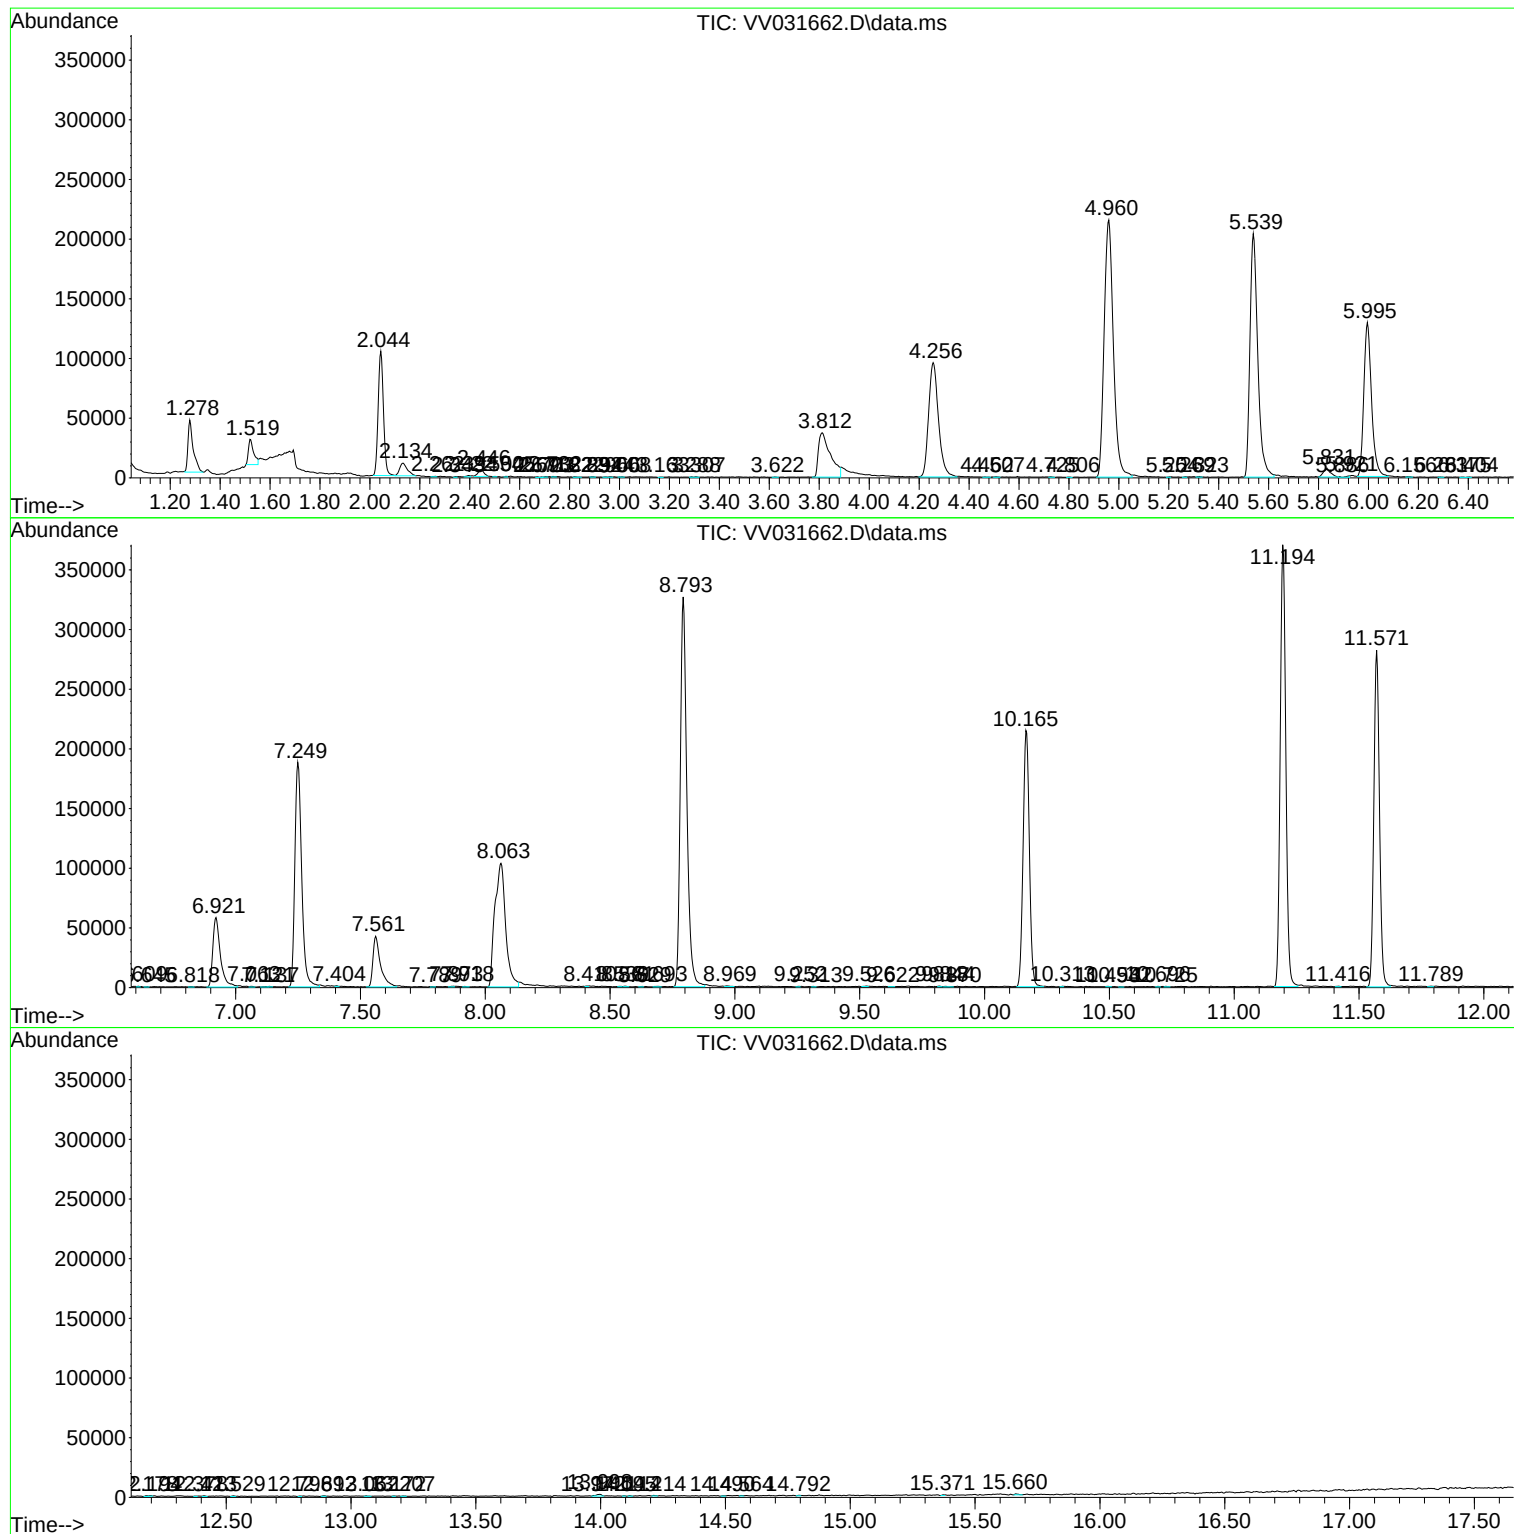

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071023\
Data File : VV031662.D
Acq On : 10 Jul 2023 13:21
Operator : SY/MD
Sample : 03551-02ME
Misc : 7.41g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCHB1ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071023\
Data File : VV031662.D
Acq On : 10 Jul 2023 13:21
Operator : SY/MD
Sample : 03551-02ME
Misc : 7.41g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCHB1ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
