

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071023\
 Data File : VV031664.D
 Acq On : 10 Jul 2023 14:07
 Operator : SY/MD
 Sample : 03551-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

Signal : TIC: VV031664.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	92	rVB	103527	113899	15.88%	2.087%
2	1.532	146	153	166	rVB	81606	97406	13.58%	1.784%
3	1.667	191	195	202	rBV4	1166	1583	0.22%	0.029%
4	2.063	308	318	332	rBV	181104	259148	36.12%	4.748%
5	2.237	370	372	375	rBV3	536	299	0.04%	0.005%
6	2.388	416	419	421	rVV4	409	266	0.04%	0.005%
7	2.413	421	427	428	rVV2	266	297	0.04%	0.005%
8	2.452	431	439	451	rVB2	4566	7828	1.09%	0.143%
9	2.593	478	483	487	rVB2	231	248	0.03%	0.005%
10	2.626	487	493	498	rBV2	358	442	0.06%	0.008%
11	2.745	526	530	534	rVB2	322	327	0.05%	0.006%
12	2.770	534	538	543	rBV	305	292	0.04%	0.005%
13	2.812	548	551	558	rVB3	370	415	0.06%	0.008%
14	2.886	571	574	577	rBV	283	225	0.03%	0.004%
15	2.928	582	587	590	rBV2	290	294	0.04%	0.005%
16	3.298	697	702	706	rVB	253	236	0.03%	0.004%
17	3.323	706	710	713	rBV2	227	205	0.03%	0.004%
18	3.661	812	815	817	rVB2	336	212	0.03%	0.004%
19	3.793	847	856	888	rBV	46777	126592	17.65%	2.319%
20	4.037	929	932	939	rVB2	337	296	0.04%	0.005%
21	4.166	969	972	978	rVB2	408	460	0.06%	0.008%
22	4.256	984	1000	1035	rBV	122636	313238	43.66%	5.739%
23	4.481	1067	1070	1072	rBV2	363	227	0.03%	0.004%
24	4.687	1130	1134	1139	rBV2	291	299	0.04%	0.005%
25	4.963	1202	1220	1249	rBV2	268583	717404	100.00%	13.143%
26	5.150	1276	1278	1280	rVB	627	261	0.04%	0.005%
27	5.249	1308	1309	1316	rVB2	376	318	0.04%	0.006%
28	5.281	1316	1319	1322	rBV	292	243	0.03%	0.004%
29	5.301	1322	1325	1329	rVB3	298	217	0.03%	0.004%
30	5.542	1388	1400	1421	rBV	194468	398986	55.62%	7.309%
31	5.780	1471	1474	1481	rBV3	276	379	0.05%	0.007%
32	5.831	1481	1490	1505	rVB2	5163	10292	1.43%	0.189%
33	5.921	1516	1518	1522	rVB2	304	212	0.03%	0.004%
34	5.995	1527	1541	1561	rBV	164171	339101	47.27%	6.212%
35	6.195	1602	1603	1608	rVV3	376	204	0.03%	0.004%
36	6.278	1626	1629	1637	rVB	286	307	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071023\
 Data File : VV031664.D
 Acq On : 10 Jul 2023 14:07
 Operator : SY/MD
 Sample : 03551-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

37	6.574	1717	1721	1722	rBV2	484	372	0.05%	0.007%
38	6.918	1817	1828	1853	rBV	77353	145131	20.23%	2.659%
39	7.079	1876	1878	1885	rBV3	420	432	0.06%	0.008%
40	7.143	1895	1898	1904	rVB2	346	268	0.04%	0.005%
41	7.249	1918	1931	1964	rBV	284492	508204	70.84%	9.310%
42	7.497	2005	2008	2013	rVB3	352	322	0.04%	0.006%
43	7.558	2014	2027	2048	rBV	58408	106755	14.88%	1.956%
44	7.687	2061	2067	2071	rBV4	492	471	0.07%	0.009%
45	7.738	2080	2083	2086	rVB2	346	221	0.03%	0.004%
46	7.760	2086	2090	2092	rBV2	197	198	0.03%	0.004%
47	7.780	2094	2096	2100	rVB2	431	259	0.04%	0.005%
48	7.812	2100	2106	2108	rBV	303	300	0.04%	0.005%
49	7.876	2121	2126	2130	rVV3	235	306	0.04%	0.006%
50	7.950	2146	2149	2155	rBV	272	243	0.03%	0.004%
51	7.982	2155	2159	2165	rVB2	337	376	0.05%	0.007%
52	8.031	2165	2174	2210	rBV	152310	295743	41.22%	5.418%
53	8.246	2238	2241	2244	rBV3	454	292	0.04%	0.005%
54	8.320	2262	2264	2268	rVB2	516	283	0.04%	0.005%
55	8.346	2268	2272	2274	rBV3	417	325	0.05%	0.006%
56	8.413	2291	2293	2296	rVB	418	279	0.04%	0.005%
57	8.455	2302	2306	2308	rBV3	365	312	0.04%	0.006%
58	8.590	2346	2348	2351	rBV3	332	221	0.03%	0.004%
59	8.715	2384	2387	2390	rVB2	279	223	0.03%	0.004%
60	8.793	2396	2411	2440	rBV	338974	570143	79.47%	10.445%
61	8.953	2458	2461	2463	rBV3	573	377	0.05%	0.007%
62	8.995	2471	2474	2476	rBV3	409	265	0.04%	0.005%
63	9.014	2476	2480	2482	rBV	436	258	0.04%	0.005%
64	9.079	2497	2500	2503	rBV3	523	289	0.04%	0.005%
65	9.156	2522	2524	2529	rVB	535	324	0.05%	0.006%
66	9.432	2604	2610	2612	rBV	318	301	0.04%	0.006%
67	9.465	2617	2620	2623	rBV2	334	201	0.03%	0.004%
68	9.497	2628	2630	2634	rVV2	442	284	0.04%	0.005%
69	9.870	2742	2746	2752	rBV3	473	516	0.07%	0.009%
70	10.159	2824	2836	2860	rBV	238367	375189	52.30%	6.873%
71	10.371	2898	2902	2906	rBV3	361	270	0.04%	0.005%
72	10.423	2911	2918	2923	rVB2	449	551	0.08%	0.010%
73	10.680	2994	2998	2999	rBV	387	265	0.04%	0.005%
74	10.690	2999	3001	3003	rVV	418	211	0.03%	0.004%
75	10.841	3045	3048	3051	rBV	289	247	0.03%	0.005%
76	10.857	3051	3053	3056	rVV2	361	217	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071023\
 Data File : VV031664.D
 Acq On : 10 Jul 2023 14:07
 Operator : SY/MD
 Sample : 03551-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

77	11.005	3093	3099	3101	rBV	260	305	0.04%	0.006%
78	11.037	3107	3109	3114	rVB	293	232	0.03%	0.004%
79	11.130	3136	3138	3145	rVB3	304	296	0.04%	0.005%
80	11.191	3145	3157	3185	rBV	346078	534477	74.50%	9.792%
81	11.426	3227	3230	3233	rBV2	327	242	0.03%	0.004%
82	11.567	3262	3274	3291	rBV	328776	512743	71.47%	9.393%
83	11.735	3324	3326	3331	rBV2	223	254	0.04%	0.005%
84	12.198	3468	3470	3475	rVB3	650	429	0.06%	0.008%
85	12.432	3535	3543	3546	rBV2	311	492	0.07%	0.009%
86	12.554	3578	3581	3583	rBV	460	292	0.04%	0.005%
87	12.593	3589	3593	3596	rBV4	531	383	0.05%	0.007%
88	12.722	3630	3633	3639	rVB	503	385	0.05%	0.007%
89	12.931	3692	3698	3700	rBV2	282	296	0.04%	0.005%
90	13.149	3763	3766	3772	rBV2	512	495	0.07%	0.009%
91	13.522	3879	3882	3884	rBV	364	230	0.03%	0.004%
92	13.571	3894	3897	3901	rVB	343	216	0.03%	0.004%
93	13.786	3960	3964	3968	rBV2	452	492	0.07%	0.009%
94	13.985	4022	4026	4027	rBV2	863	634	0.09%	0.012%
95	14.194	4089	4091	4094	rBV2	376	253	0.04%	0.005%
96	14.281	4116	4118	4123	rBV	298	264	0.04%	0.005%
97	14.554	4200	4203	4204	rBV	459	229	0.03%	0.004%
98	14.590	4212	4214	4218	rVB2	508	315	0.04%	0.006%
99	15.082	4365	4367	4369	rBV2	399	203	0.03%	0.004%
100	15.538	4507	4509	4510	rBV	564	240	0.03%	0.004%




Sum of corrected areas: 5458499

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071023\
Data File : VV031664.D
Acq On : 10 Jul 2023 14:07
Operator : SY/MD
Sample : 03551-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

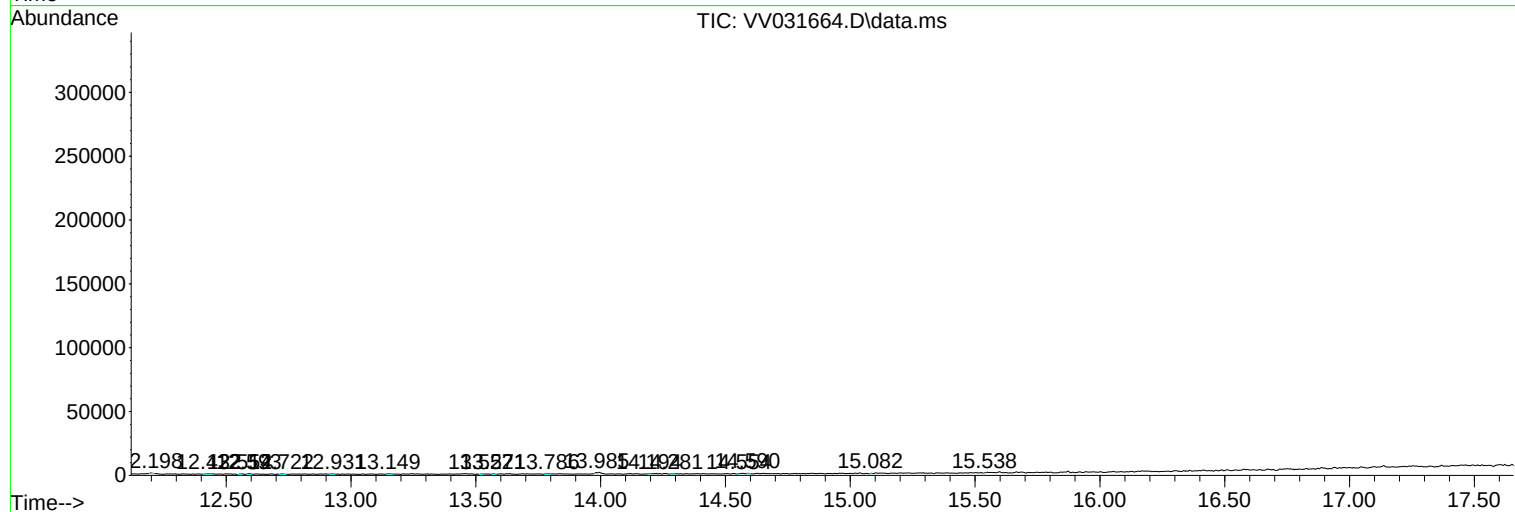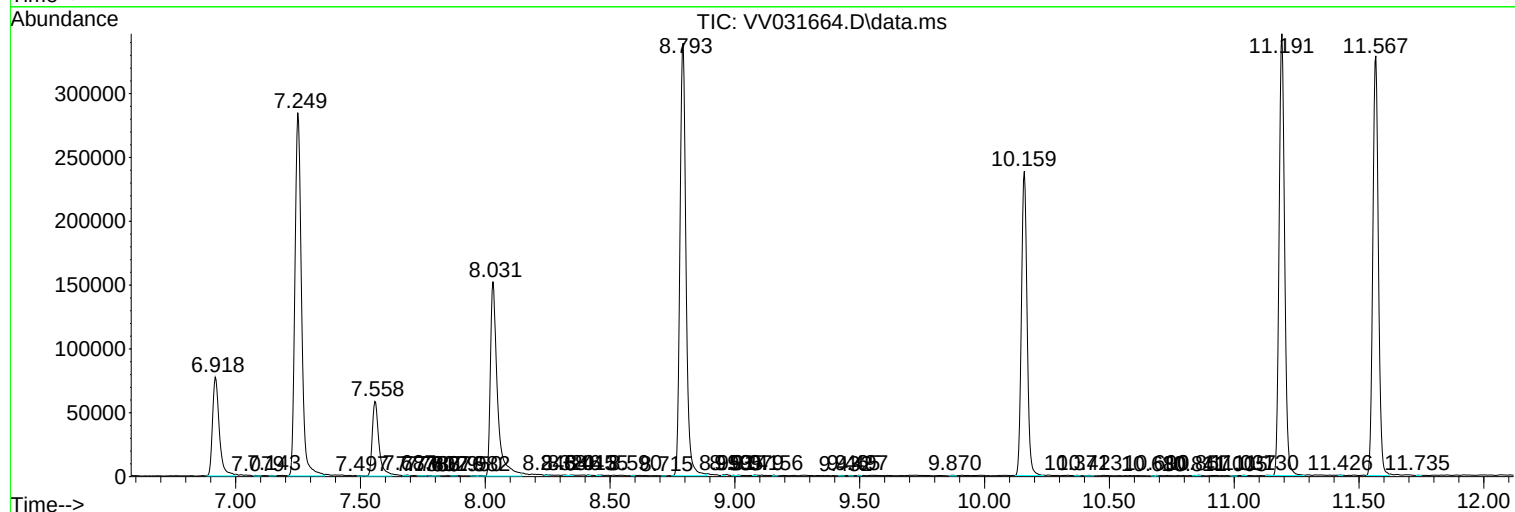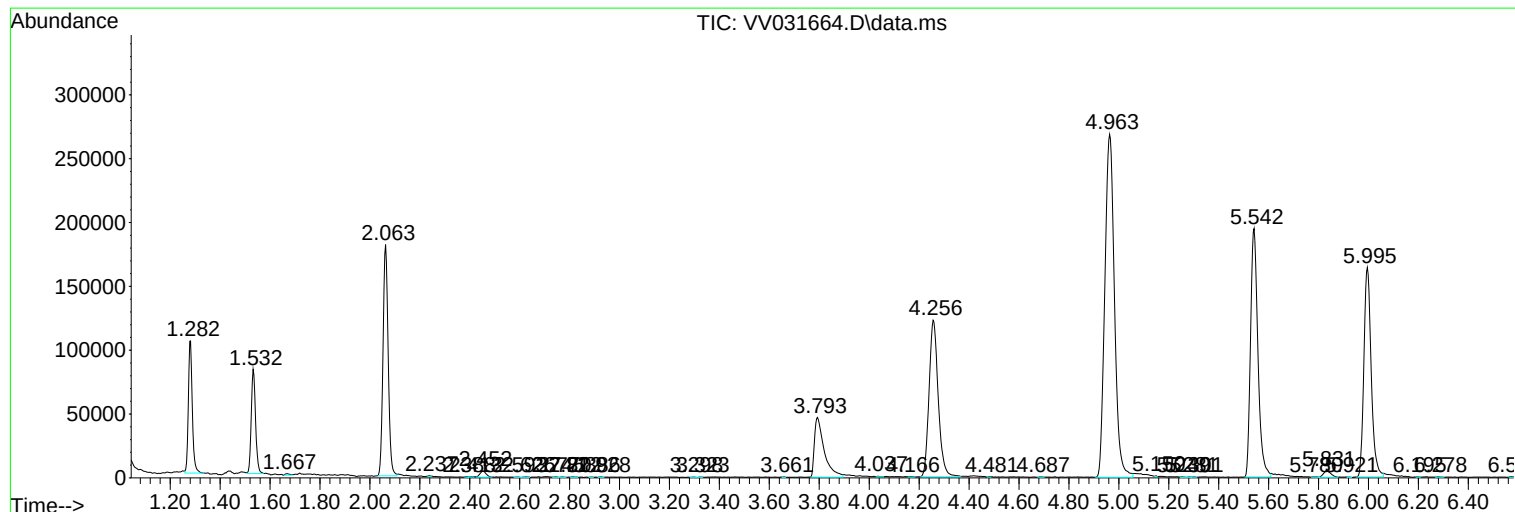

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071023\
Data File : VV031664.D
Acq On : 10 Jul 2023 14:07
Operator : SY/MD
Sample : 03551-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071023\
Data File : VV031664.D
Acq On : 10 Jul 2023 14:07
Operator : SY/MD
Sample : 03551-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------