

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071023\
 Data File : VV031667.D
 Acq On : 10 Jul 2023 15:17
 Operator : SY/MD
 Sample : VIBLK223
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK223

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

Signal : TIC: VV031667.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	91	rVB	85458	93647	14.39%	1.919%
2	1.532	147	153	165	rVB	71859	83601	12.84%	1.713%
3	2.063	308	318	331	rBV	143997	209016	32.11%	4.284%
4	2.455	431	440	449	rVB5	2513	4146	0.64%	0.085%
5	2.510	454	457	459	rBV2	288	186	0.03%	0.004%
6	2.645	495	499	505	rBV4	377	447	0.07%	0.009%
7	2.670	505	507	510	rVV	176	140	0.02%	0.003%
8	2.703	512	517	524	rVB5	997	1429	0.22%	0.029%
9	2.735	524	527	531	rBV	260	193	0.03%	0.004%
10	2.757	531	534	536	rBV2	250	196	0.03%	0.004%
11	2.899	574	578	581	rVB2	286	231	0.04%	0.005%
12	2.918	581	584	587	rBV2	430	319	0.05%	0.007%
13	2.963	596	598	599	rBV2	258	115	0.02%	0.002%
14	3.018	611	615	619	rVB2	259	223	0.03%	0.005%
15	3.047	619	624	627	rBV3	375	316	0.05%	0.006%
16	3.082	632	635	637	rBV2	155	111	0.02%	0.002%
17	3.111	641	644	647	rBV2	184	135	0.02%	0.003%
18	3.150	654	656	658	rBV2	146	92	0.01%	0.002%
19	3.166	658	661	663	rVV	207	128	0.02%	0.003%
20	3.188	666	668	672	rBV2	172	138	0.02%	0.003%
21	3.288	696	699	704	rVB	257	214	0.03%	0.004%
22	3.336	704	714	720	rBV2	412	610	0.09%	0.013%
23	3.371	723	725	729	rBV2	146	93	0.01%	0.002%
24	3.413	732	738	739	rBV2	232	245	0.04%	0.005%
25	3.461	751	753	756	rVV	237	133	0.02%	0.003%
26	3.510	765	768	769	rBV	183	85	0.01%	0.002%
27	3.574	783	788	794	rBV3	278	332	0.05%	0.007%
28	3.609	796	799	803	rBV2	218	193	0.03%	0.004%
29	3.670	813	818	820	rBV	275	211	0.03%	0.004%
30	3.686	821	823	826	rVB2	184	121	0.02%	0.002%
31	3.706	826	829	831	rBV2	261	175	0.03%	0.004%
32	3.760	843	846	848	rBV	144	83	0.01%	0.002%
33	3.796	848	857	888	rBV	49817	137496	21.12%	2.818%
34	4.256	984	1000	1026	rBV2	107956	277784	42.68%	5.693%
35	4.574	1096	1099	1100	rBV	158	85	0.01%	0.002%
36	4.622	1111	1114	1119	rBV2	343	271	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071023\
 Data File : VV031667.D
 Acq On : 10 Jul 2023 15:17
 Operator : SY/MD
 Sample : VIBLK223
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK223

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

37	4.744	1150	1152	1155	rVB	317	200	0.03%	0.004%
38	4.963	1203	1220	1243	rBV2	246745	650881	100.00%	13.340%
39	5.294	1320	1323	1328	rBV3	288	284	0.04%	0.006%
40	5.381	1348	1350	1353	rBV2	149	77	0.01%	0.002%
41	5.400	1353	1356	1358	rVB	307	168	0.03%	0.003%
42	5.413	1358	1360	1363	rVB2	149	83	0.01%	0.002%
43	5.436	1363	1367	1368	rBV2	192	108	0.02%	0.002%
44	5.445	1368	1370	1372	rBV2	191	87	0.01%	0.002%
45	5.490	1380	1384	1386	rBV	327	244	0.04%	0.005%
46	5.542	1388	1400	1425	rVV	180281	375458	57.68%	7.695%
47	5.767	1466	1470	1473	rBV3	251	282	0.04%	0.006%
48	5.831	1479	1490	1505	rBV8	5232	11172	1.72%	0.229%
49	5.902	1510	1512	1513	rBV8	211	99	0.02%	0.002%
50	5.995	1528	1541	1566	rBV	150878	312807	48.06%	6.411%
51	6.185	1598	1600	1603	rVB2	530	274	0.04%	0.006%
52	6.204	1603	1606	1613	rVB	356	351	0.05%	0.007%
53	6.239	1613	1617	1618	rBV	289	205	0.03%	0.004%
54	6.326	1641	1644	1645	rBV	179	95	0.01%	0.002%
55	6.368	1655	1657	1659	rBV	267	116	0.02%	0.002%
56	6.426	1669	1675	1678	rBV2	362	360	0.06%	0.007%
57	6.567	1716	1719	1720	rBV	347	208	0.03%	0.004%
58	6.612	1731	1733	1737	rBV	299	120	0.02%	0.002%
59	6.651	1744	1745	1748	rBV	249	155	0.02%	0.003%
60	6.789	1786	1788	1790	rBV	199	101	0.02%	0.002%
61	6.879	1813	1816	1817	rBV	157	106	0.02%	0.002%
62	6.921	1818	1829	1855	rVV	71445	135829	20.87%	2.784%
63	7.124	1889	1892	1894	rBV2	520	332	0.05%	0.007%
64	7.249	1919	1931	1963	rBV	248429	448452	68.90%	9.191%
65	7.558	2015	2027	2054	rBV	54689	99209	15.24%	2.033%
66	7.738	2081	2083	2084	rBV	211	76	0.01%	0.002%
67	7.802	2101	2103	2106	rVB3	319	168	0.03%	0.003%
68	7.882	2118	2128	2136	rBV2	3018	5126	0.79%	0.105%
69	8.030	2165	2174	2202	rBV	143737	265135	40.73%	5.434%
70	8.288	2252	2254	2259	rBV3	540	485	0.07%	0.010%
71	8.365	2276	2278	2280	rBV	208	97	0.01%	0.002%
72	8.493	2314	2318	2322	rBV2	326	331	0.05%	0.007%
73	8.689	2376	2379	2382	rBV	220	187	0.03%	0.004%
74	8.702	2382	2383	2388	rVB	402	226	0.03%	0.005%
75	8.789	2396	2410	2433	rBV	281938	475278	73.02%	9.741%
76	8.998	2474	2475	2477	rBV	269	105	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071023\
 Data File : VV031667.D
 Acq On : 10 Jul 2023 15:17
 Operator : SY/MD
 Sample : VIBLK223
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK223

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

77	9.030	2483	2485	2489	rVB	399	207	0.03%	0.004%
78	9.088	2491	2503	2507	rBV4	897	1471	0.23%	0.030%
79	9.172	2525	2529	2532	rBV2	309	286	0.04%	0.006%
80	9.217	2539	2543	2547	rBV3	312	292	0.04%	0.006%
81	9.545	2642	2645	2647	rBV2	260	164	0.03%	0.003%
82	9.625	2668	2670	2673	rBV	277	155	0.02%	0.003%
83	9.689	2687	2690	2692	rBV	234	140	0.02%	0.003%
84	9.725	2699	2701	2703	rBV	317	196	0.03%	0.004%
85	9.873	2742	2747	2753	rBV3	914	1167	0.18%	0.024%
86	10.101	2817	2818	2821	rBV2	177	74	0.01%	0.002%
87	10.159	2824	2836	2859	rVV	208354	332032	51.01%	6.805%
88	10.300	2876	2880	2881	rBV	422	301	0.05%	0.006%
89	10.779	3027	3029	3033	rBB2	303	171	0.03%	0.004%
90	10.850	3048	3051	3053	rBV2	494	359	0.06%	0.007%
91	11.191	3146	3157	3177	rBV	314648	483403	74.27%	9.907%
92	11.455	3236	3239	3241	rBV2	332	255	0.04%	0.005%
93	11.567	3263	3274	3294	rBV	275283	427548	65.69%	8.762%
94	11.937	3386	3389	3393	rBV2	425	392	0.06%	0.008%
95	12.522	3568	3571	3573	rBV3	322	223	0.03%	0.005%
96	12.590	3587	3592	3602	rVB4	2442	3174	0.49%	0.065%
97	13.210	3777	3785	3795	rVB5	3784	5482	0.84%	0.112%
98	13.294	3806	3811	3813	rBV2	433	400	0.06%	0.008%
99	13.448	3852	3859	3873	rVB	10479	15191	2.33%	0.311%
100	13.689	3926	3934	3944	rVB3	5417	8204	1.26%	0.168%




Sum of corrected areas: 4879304

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071023\
Data File : VV031667.D
Acq On : 10 Jul 2023 15:17
Operator : SY/MD
Sample : VIBLK223
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK223

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

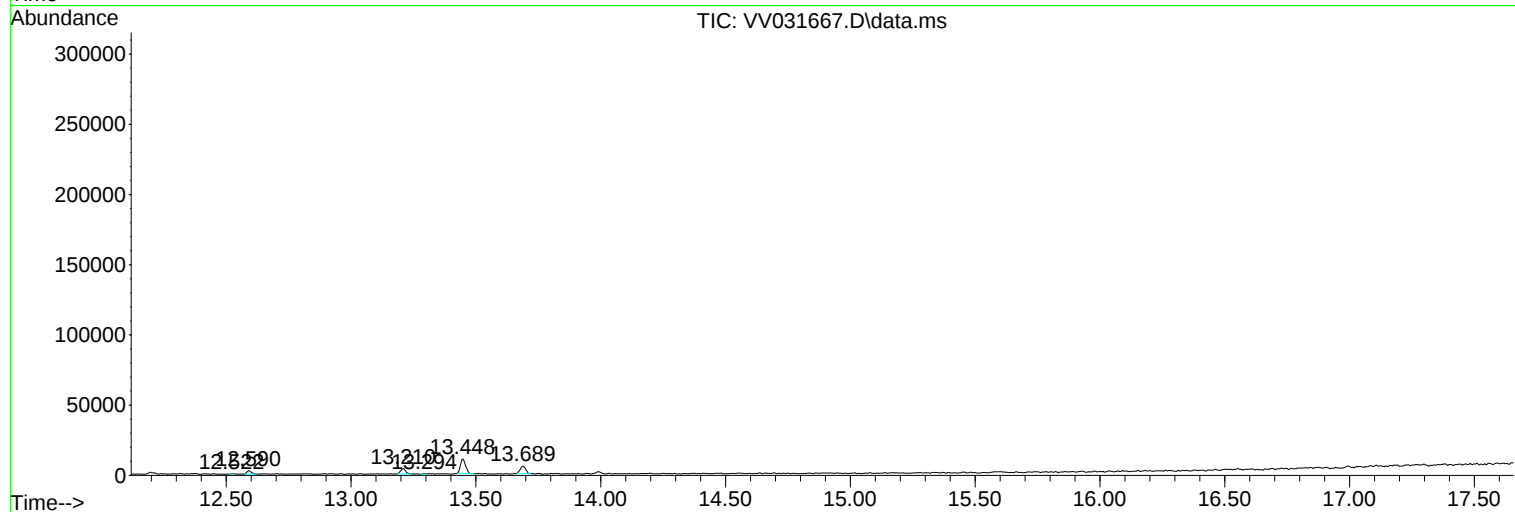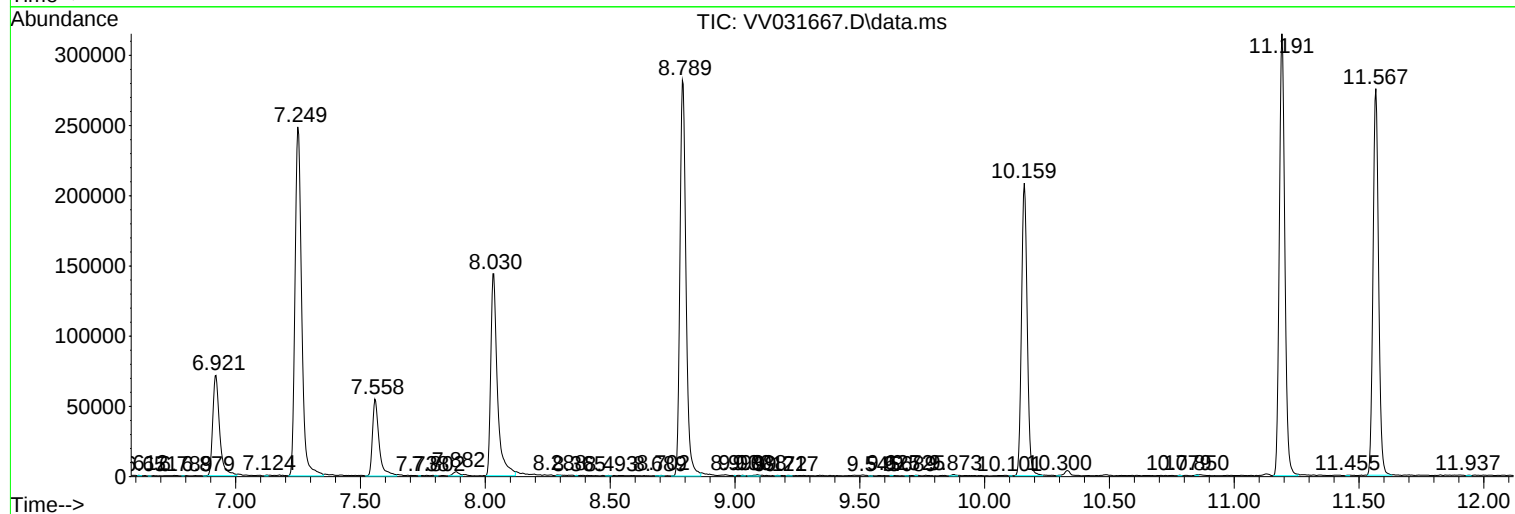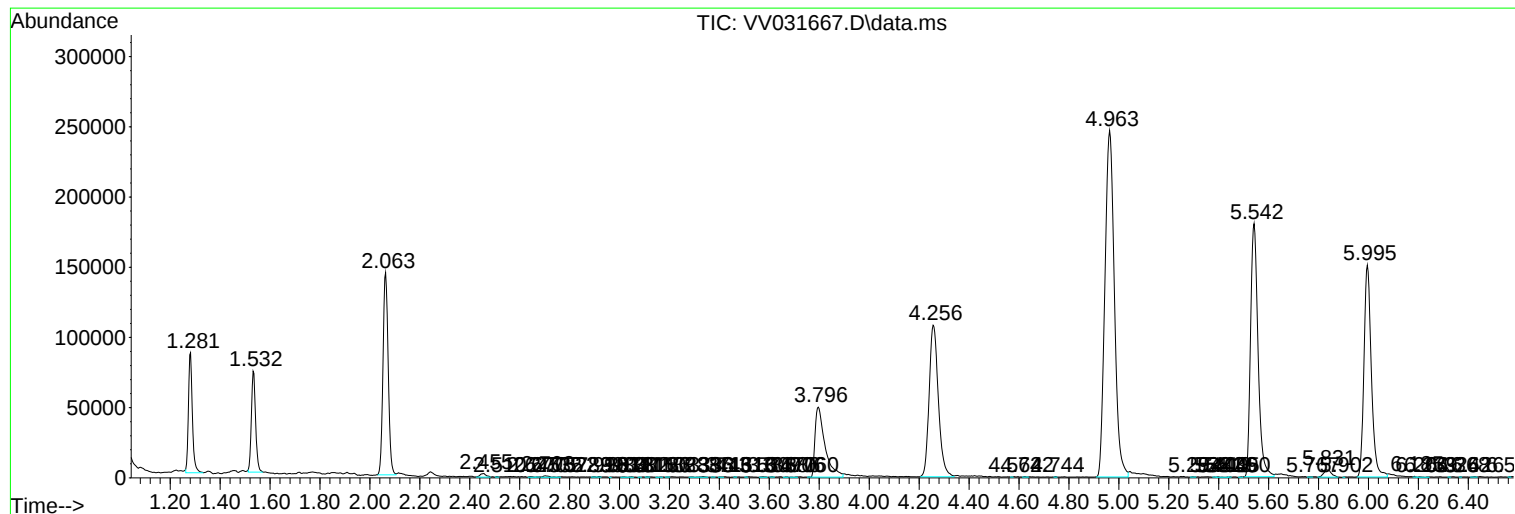

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071023\
Data File : VV031667.D
Acq On : 10 Jul 2023 15:17
Operator : SY/MD
Sample : VIBLK223
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK223

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071023\
Data File : VV031667.D
Acq On : 10 Jul 2023 15:17
Operator : SY/MD
Sample : VIBLK223
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK223

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------