
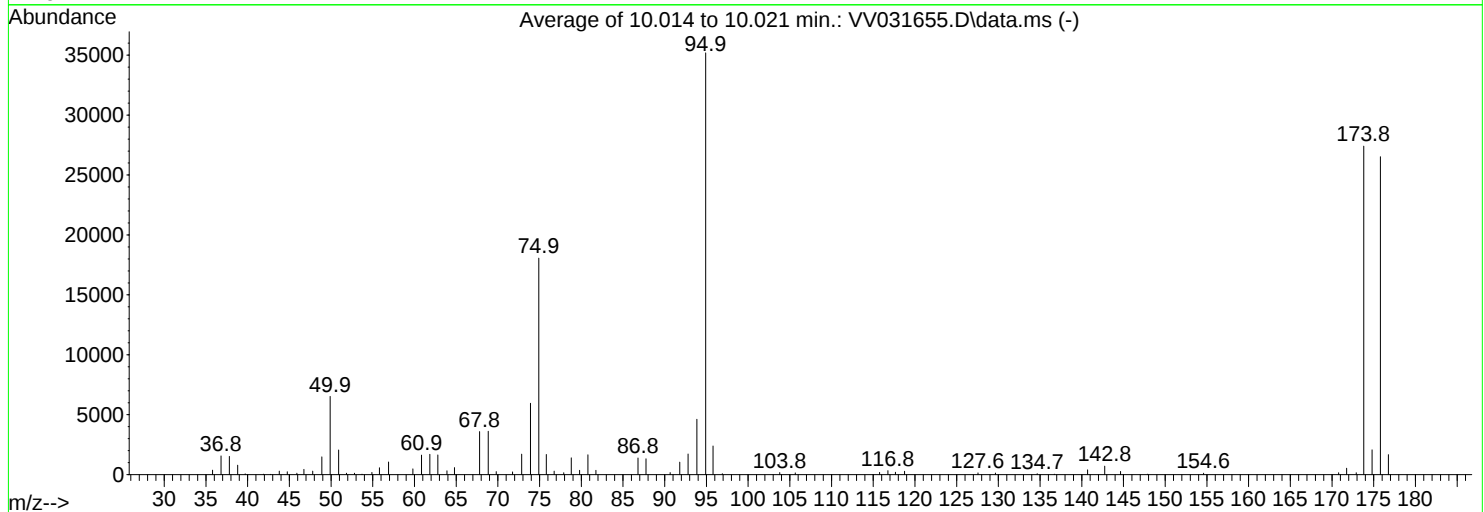


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071023\
Data File : VV031655.D
Acq On : 10 Jul 2023 08:56
Operator : SY/MD
Sample : BFB395
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB395

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Title : VOC Analysis
Last Update : Fri Jul 07 02:34:55 2023

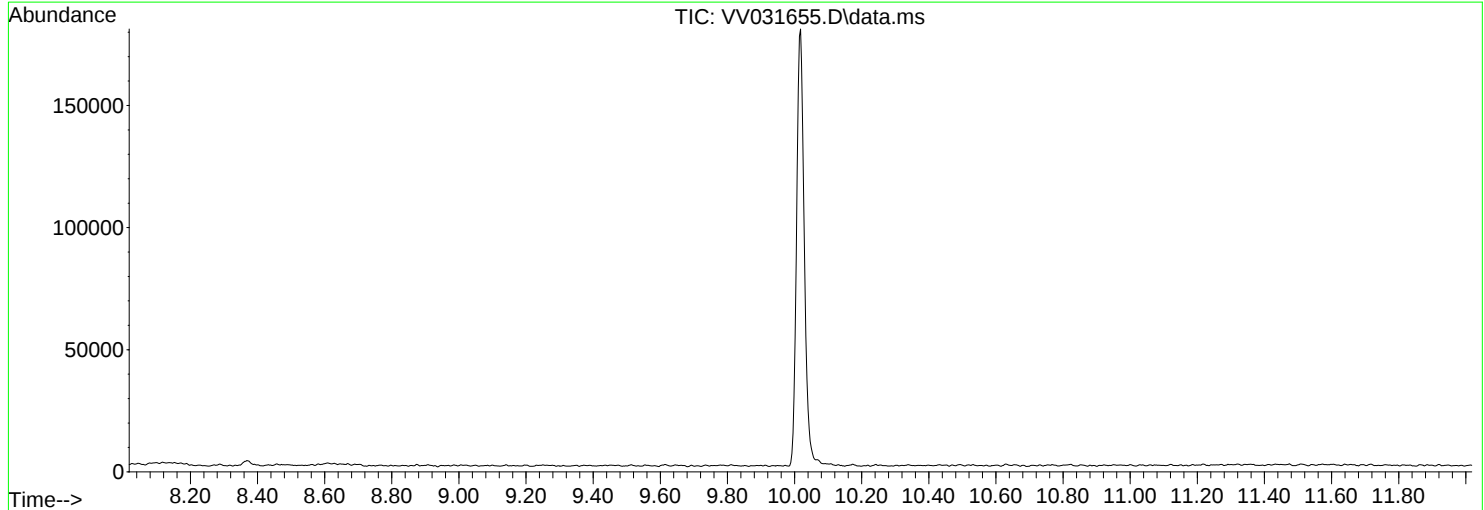

AutoFind: Scans 2791, 2792, 2793; Background Corrected with Scan 2780

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.5	6526	PASS
75	95	30	80	51.3	18056	PASS
95	95	100	100	100.0	35192	PASS
96	95	5	9	6.8	2390	PASS
173	174	0.00	2	0.6	167	PASS
174	95	50	120	77.9	27413	PASS
175	174	5	9	7.6	2073	PASS
176	174	95	105	96.8	26533	PASS
177	176	5	10	6.3	1671	PASS

m/z	Abundance
39.70	146.0
40.70	122.0
42.70	184.0
43.80	1807.0
44.80	191.0

Instrument :
MSVOA_V
ClientSampleId :
BFB395

m/z	Abundance
35.80	337.0
36.80	1641.0
37.80	1663.0
38.80	760.0
39.80	220.0
42.80	224.0
43.80	2081.0
44.70	444.0
45.90	112.0
46.80	433.0
47.90	262.0
48.90	1553.0
49.90	6747.0
50.90	2047.0
51.80	133.0
52.80	118.0
54.90	198.0
55.80	579.0
56.90	1184.0
59.80	532.0
60.90	1730.0
61.80	1587.0
62.80	1795.0
63.90	364.0
64.80	496.0
67.80	3744.0
68.80	3614.0
69.80	276.0
71.70	222.0
72.80	1675.0
73.90	5992.0
74.90	18496.0
75.80	1671.0
76.70	299.0
78.00	174.0
78.80	1458.0
79.80	407.0
80.80	1614.0
81.70	376.0
86.80	1484.0
87.80	1273.0
90.60	191.0
91.80	1162.0
92.80	1808.0
93.80	4711.0
94.90	35648.0
95.80	2540.0
96.90	125.0
103.80	196.0
105.60	143.0
115.80	181.0
116.70	307.0
117.60	238.0
118.70	289.0
127.50	119.0
129.60	135.0
136.70	108.0
140.70	424.0
142.80	730.0
144.70	284.0
154.60	113.0
170.80	173.0
171.70	527.0
172.90	501.0
173.80	27448.0
174.80	2082.0
175.80	26432.0
176.80	1633.0

Instrument :
MSVOA_V
ClientSampleId :
BFB395

m/z	Abundance
35.80	370.0
36.80	1633.0
37.80	1571.0
38.80	801.0
39.70	226.0
42.80	220.0
43.80	2111.0
44.70	438.0
45.90	129.0
46.70	468.0
47.80	316.0
48.90	1516.0
49.90	6760.0
50.90	2127.0
51.90	122.0
52.80	121.0
54.90	197.0
55.80	588.0
56.90	1098.0
59.80	501.0
60.90	1645.0
61.90	1706.0
62.80	1698.0
63.90	346.0
64.80	595.0
67.80	3726.0
68.80	3735.0
69.80	265.0
71.70	237.0
72.80	1757.0
73.90	6137.0
74.90	18632.0
75.80	1733.0
76.70	313.0
77.90	160.0
78.80	1412.0
79.80	366.0
80.80	1686.0
81.70	371.0
86.80	1444.0
87.80	1380.0
90.70	164.0
91.80	1086.0
92.80	1811.0
93.90	4806.0
94.90	36440.0
95.80	2449.0
96.90	105.0
103.80	176.0
105.70	160.0
115.80	192.0
116.80	345.0
117.60	209.0
118.80	283.0
127.60	151.0
129.70	136.0
134.60	126.0
140.70	393.0
142.80	725.0
144.60	284.0
154.60	130.0
170.80	159.0
171.80	535.0
173.80	28408.0
174.80	2085.0
175.80	27536.0
176.70	1756.0

Instrument :
MSVOA_V
ClientSampleId :
BFB395

m/z	Abundance
35.80	399.0
36.80	1398.0
37.80	1327.0
38.80	817.0
39.70	211.0
41.90	140.0
42.80	208.0
43.90	2111.0
44.80	431.0
45.90	126.0
46.80	425.0
47.70	290.0
48.90	1366.0
49.90	6071.0
50.90	1999.0
51.90	108.0
52.80	110.0
53.70	128.0
54.90	156.0
55.80	545.0
56.90	881.0
59.80	428.0
60.80	1531.0
61.90	1781.0
62.80	1435.0
63.90	270.0
64.80	669.0
67.80	3293.0
68.90	3492.0
69.80	232.0
71.80	245.0
72.90	1695.0
73.90	5742.0
74.90	17040.0
75.80	1629.0
76.80	257.0
77.80	153.0
78.80	1332.0
79.80	326.0
80.80	1661.0
81.80	330.0
86.80	1224.0
87.70	1321.0
90.70	150.0
91.80	886.0
92.80	1558.0
93.90	4326.0
94.90	33488.0
95.80	2182.0
103.80	136.0
105.70	141.0
115.70	184.0
116.80	338.0
117.70	165.0
118.80	257.0
127.60	162.0
129.70	138.0
134.70	114.0
140.70	400.0
142.70	675.0
144.70	255.0
147.90	106.0
154.60	122.0
170.80	134.0
171.80	543.0
173.80	26384.0
174.80	2051.0
175.80	25632.0
176.70	1625.0

Instrument :
MSVOA_V
ClientSampleId :
BFB395