
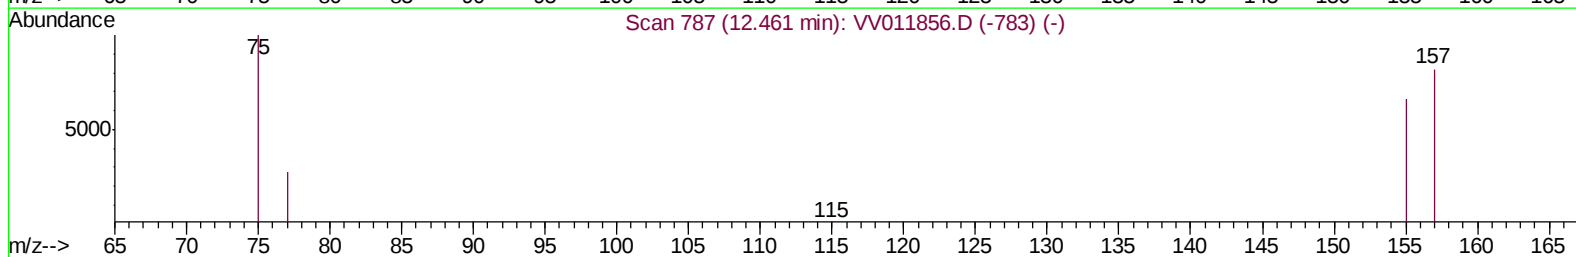
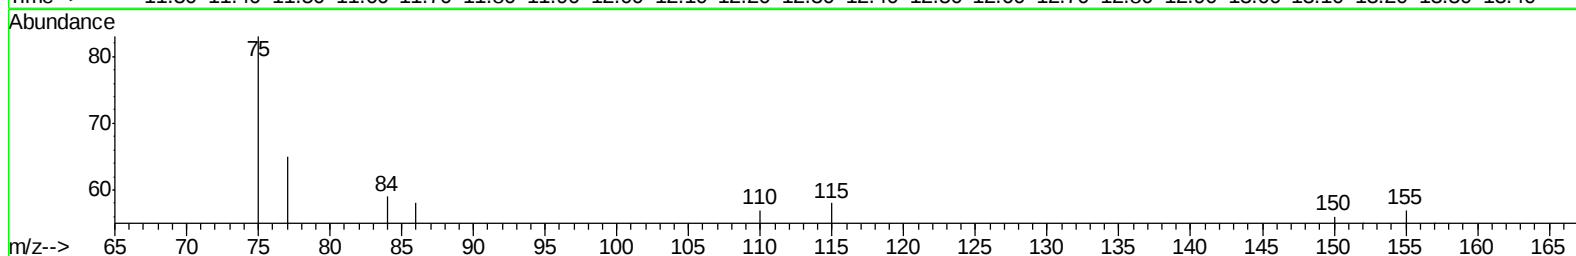


Data File : VV011858.D
Acq On : 11 Jul 2019 16:57
Operator : SY/MD
Sample : MDL06
Misc : 25ML/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Quant Time: Jul 12 03:47:32 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR070819SIM.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jul 12 03:44:53 2019
Response via : Initial Calibration

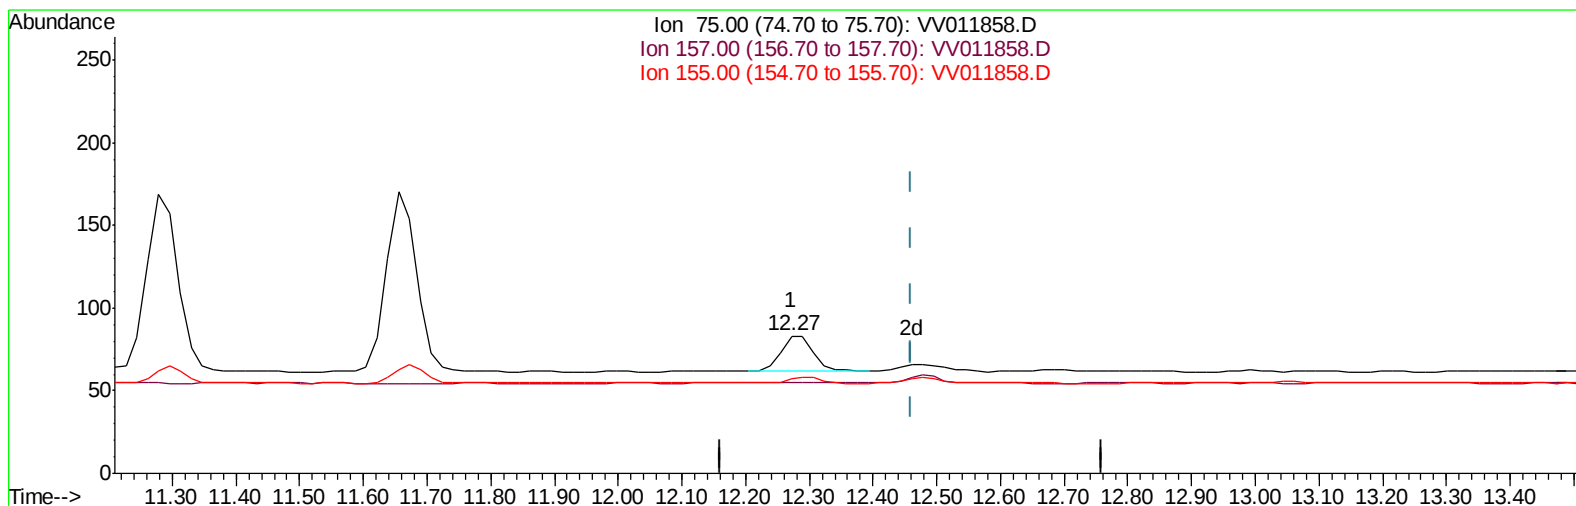

TIC: VV011858.D

(13) 1,2-Dibromo-3-chloropropane (T)

12.272min (-0.188) 0.11ug/L

response 74

Ion	Exp%	Act%
75.00	100	100
157.00	77.80	66.27
155.00	69.50	68.67
0.00	0.00	0.00