

Data File : VV011858.D
Acq On : 11 Jul 2019 16:57
Operator : SY/MD
Sample : MDL06
Misc : 25ML/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL06

Manual Integrations
APPROVED

MMDadoda
7/12/2019 5:31:26 PM

Quant Time: Jul 12 03:49:26 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR070819SIM.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jul 12 03:44:53 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	7494	0.50	ug/L	0.00
5) Chlorobenzene-d5	8.89	117	6985	0.50	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.30	152	3307	0.50	ug/L	0.00

System Monitoring Compounds

2) Vinyl Chloride-d3	1.32	65	3173	0.39	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	78.00%
4) 1,2-Dichloroethane-d4	5.07	65	3091	0.50	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	100.00%
7) 1,2-Dichloropropane-d6	6.12	67	3446	0.51	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	102.00%
8) Toluene-d8	7.35	98	9176	0.52	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	104.00%
10) 1,1,2,2-Tetrachloroethane-	10.25	84	1727	0.41	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	82.00%

Target Compounds

					Qvalue	
3) Vinyl chloride	1.32	62	205	0.026	ug/L #	28
6) Trichloroethene	5.95	95	190	0.030	ug/L #	88
9) 1,2-Dibromoethane	8.40	107	106	0.030	ug/L #	84
12) 1,2,3-Trichloropropane	10.30	75	93	0.026	ug/L #	88
13) 1,2-Dibromo-3-chloropropan	12.46	75	25m	0.038	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data File : VV011858.D
Acq On : 11 Jul 2019 16:57
Operator : SY/MD
Sample : MDL06
Misc : 25ML/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
MDL06

Manual Integrations
APPROVED

MMDadoda
7/12/2019 5:31:26 PM

Quant Time: Jul 12 03:49:26 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR070819SIM.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jul 12 03:44:53 2019
Response via : Initial Calibration

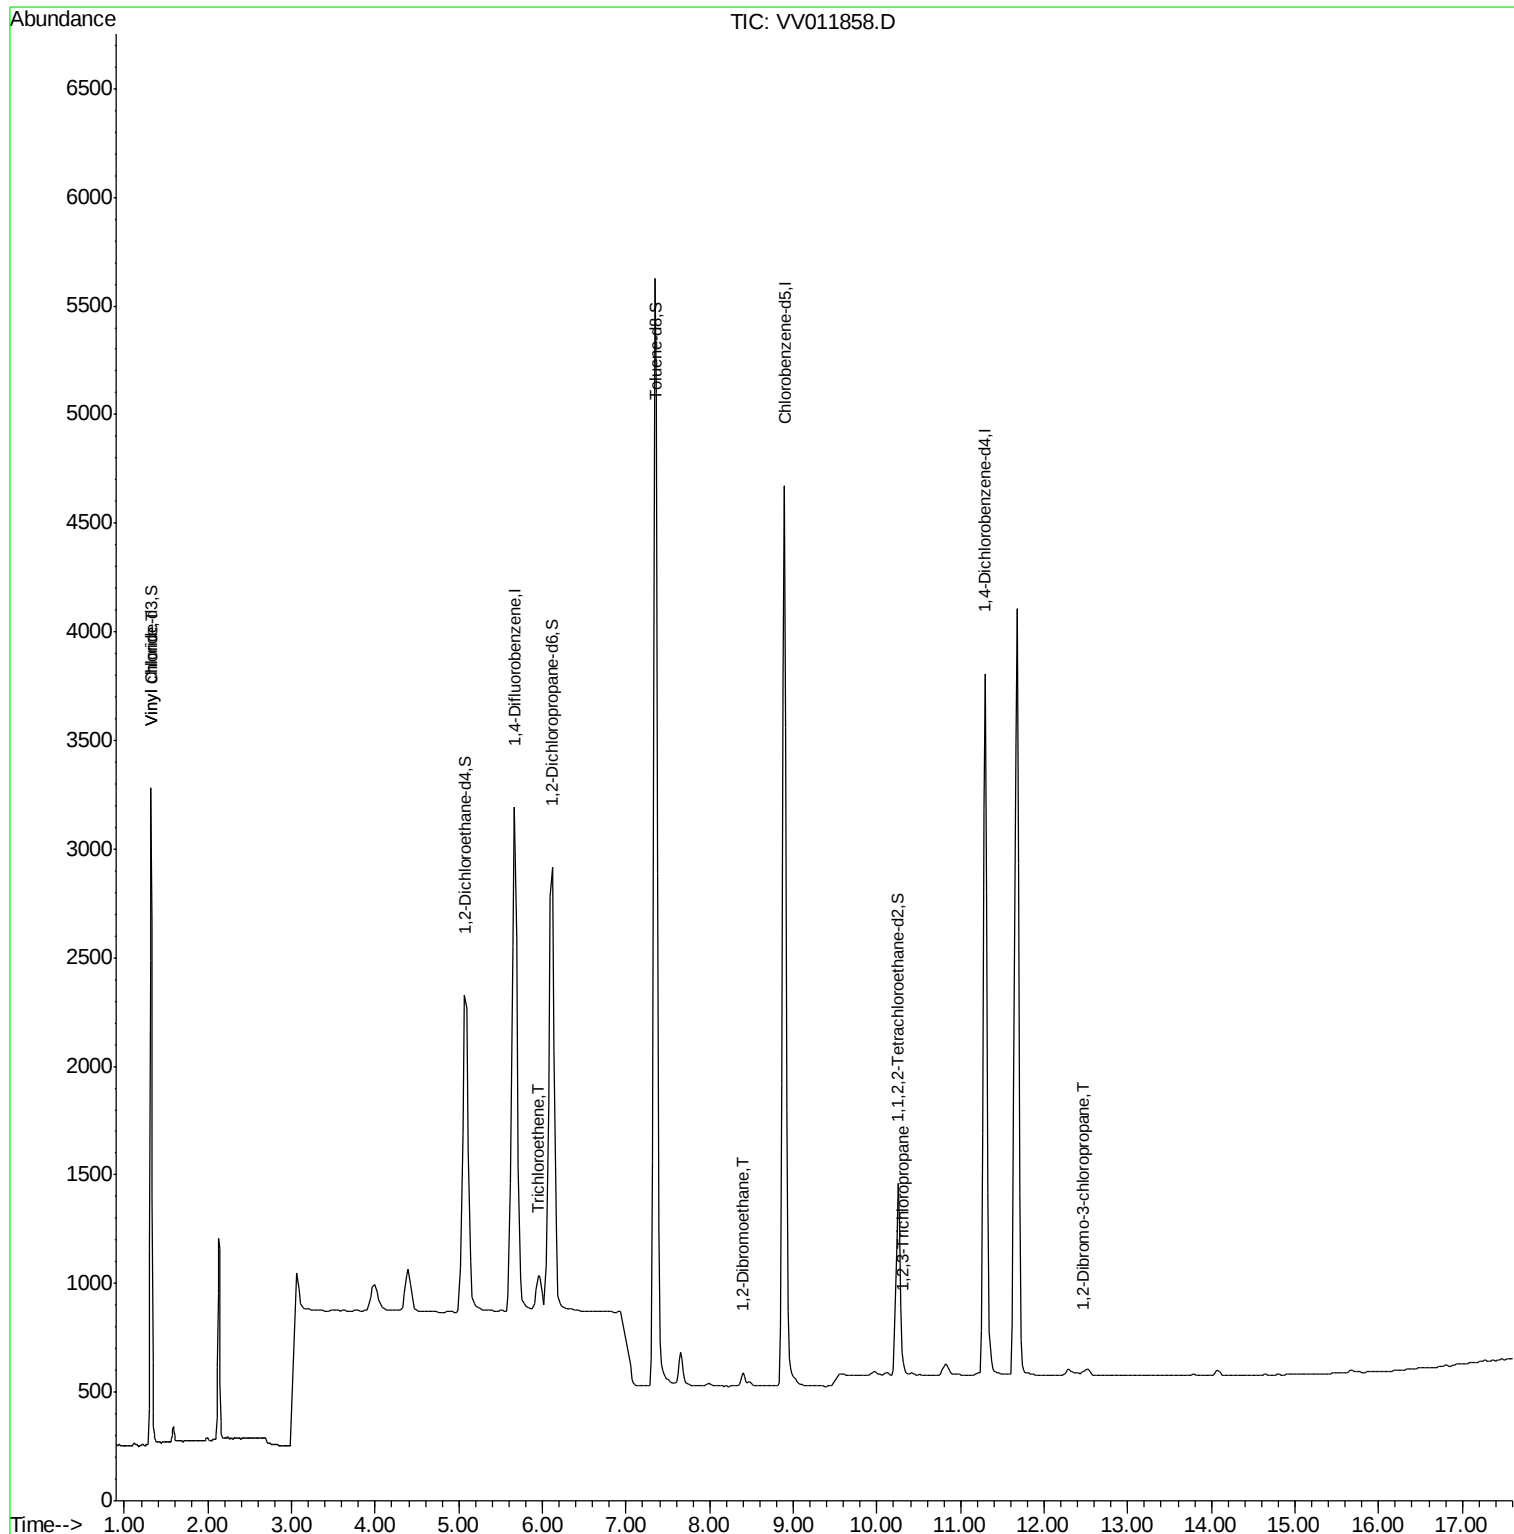

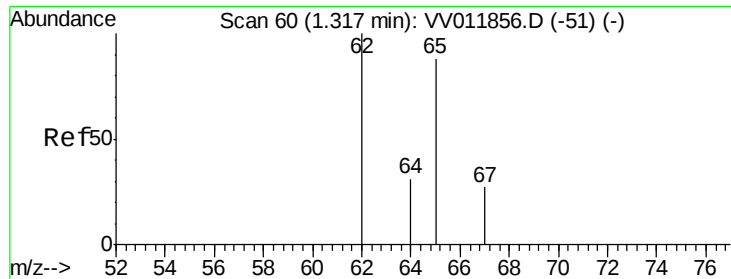

#3

Vinyl chloride

Concen: 0.026 ug/L

RT: 1.32 min Scan# 60

Delta R.T. 0.00 min

Lab File: VV011858.D

Acq: 11 Jul 2019 16:57

Instrument :

MSVOA_V

ClientSampled :

MDL06

Tgt Ion: 62 Resp: 205

Ion Ratio Lower Upper

62 100





64 74.1 23.2 43.2#

Manual Integrations

APPROVED

MMDadoda

7/12/2019 5:31:26 PM

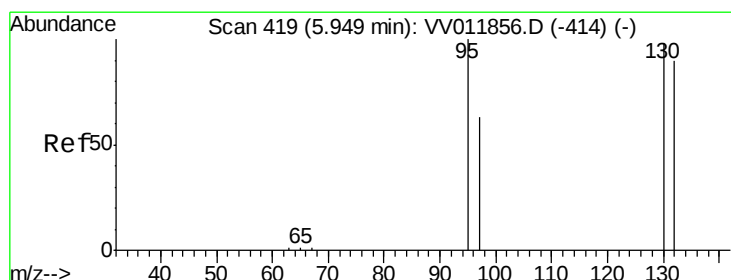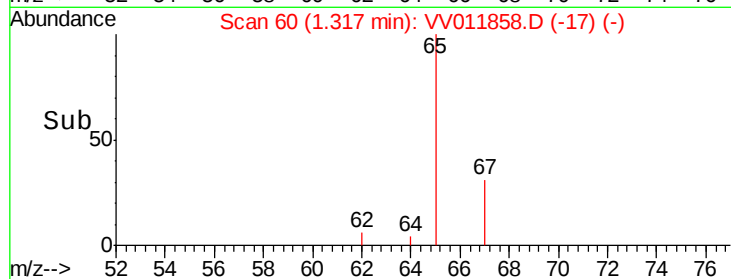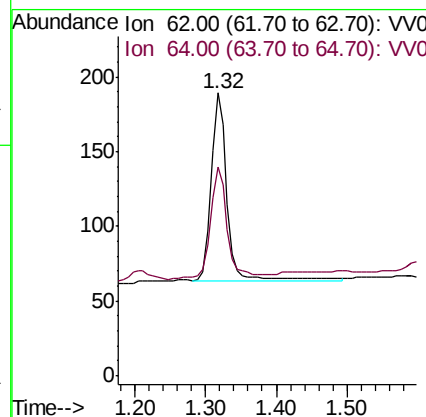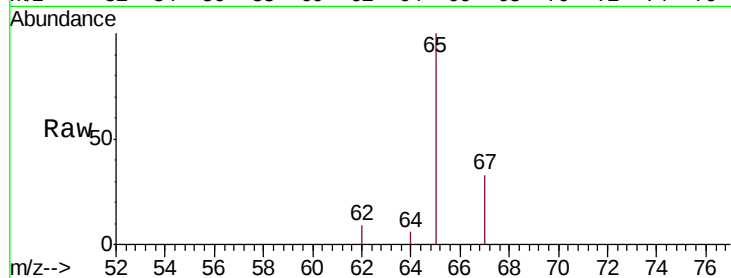

#6

Trichloroethene

Concen: 0.030 ug/L

RT: 5.95 min Scan# 419

Delta R.T. 0.00 min

Lab File: VV011858.D

Acq: 11 Jul 2019 16:57

Tgt Ion: 95 Resp: 190




Ion Ratio Lower Upper


95 100

97 86.1 46.2 85.8#

132 94.1 59.0 109.6

130 94.1 64.3 119.5

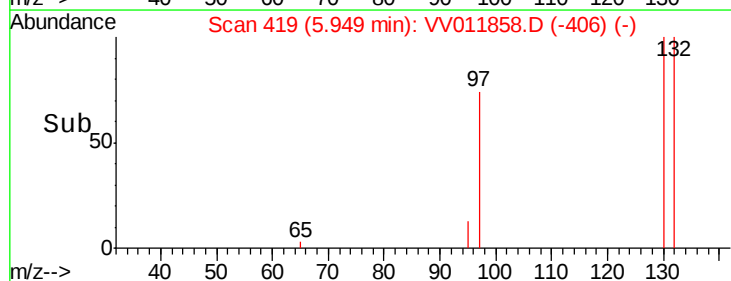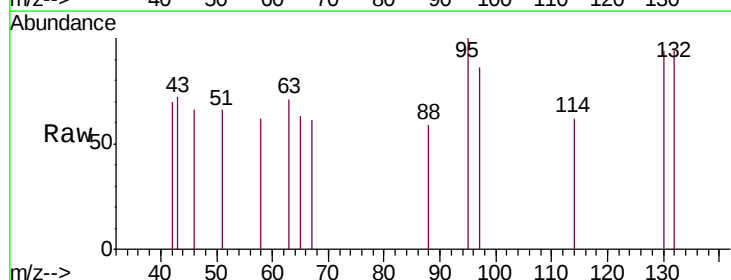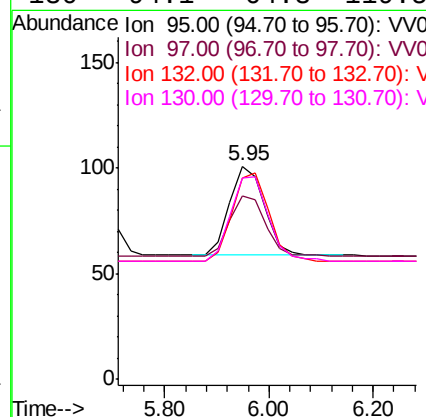

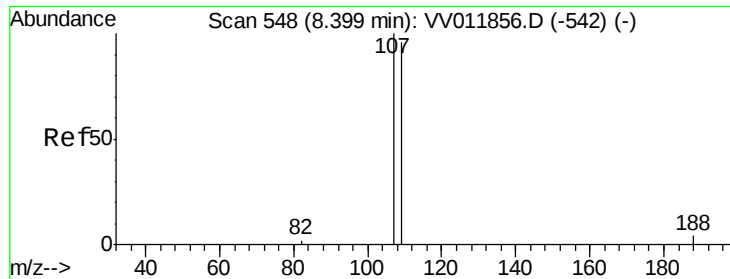

#9

1,2-Dibromoethane

Concen: 0.030 ug/L

RT: 8.40 min Scan# 548

Delta R.T. 0.00 min

Lab File: VV011858.D


Acq: 11 Jul 2019 16:57

Instrument :

MSVOA_V

ClientSampleId :




MDL06

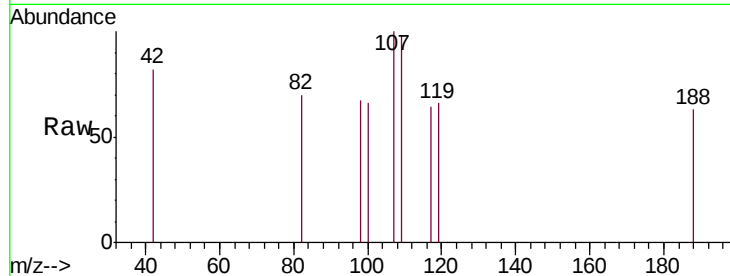

Tgt Ion	Ratio	Lower	Upper
107	100		
109	97.7	67.7	125.7
188	63.2	9.8	14.8#

Manual Integrations
APPROVED

MMDadoda
7/12/2019 5:31:26 PM

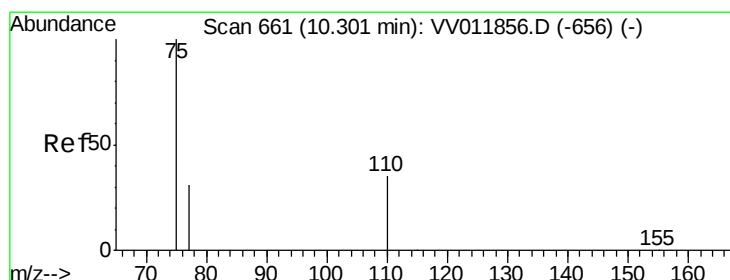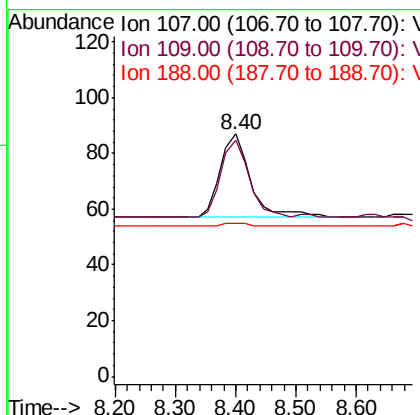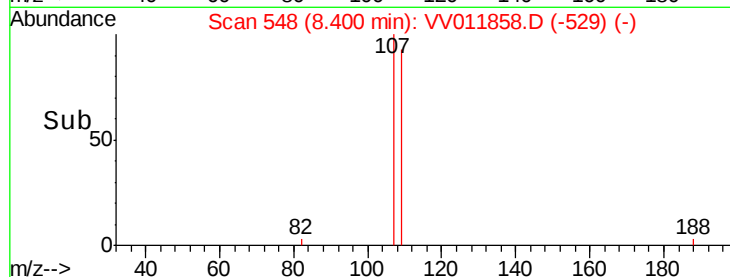

#12

1,2,3-Trichloropropane

Concen: 0.026 ug/L




RT: 10.30 min Scan# 661


Delta R.T. 0.00 min

Lab File: VV011858.D

Acq: 11 Jul 2019 16:57

Tgt Ion	Ratio	Lower	Upper
75	100		
110	44.1	32.2	48.4
77	41.9	25.3	37.9#

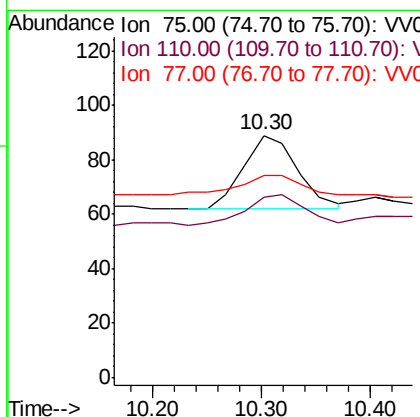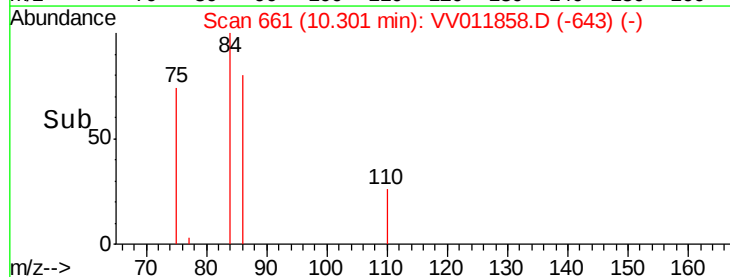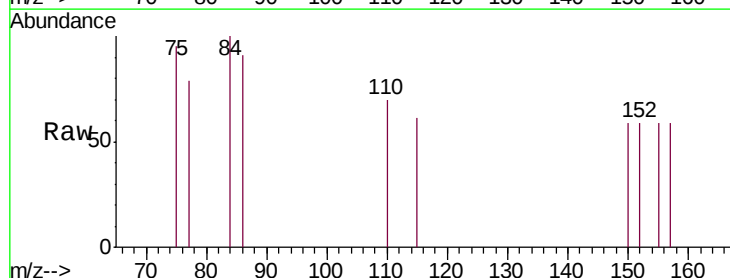

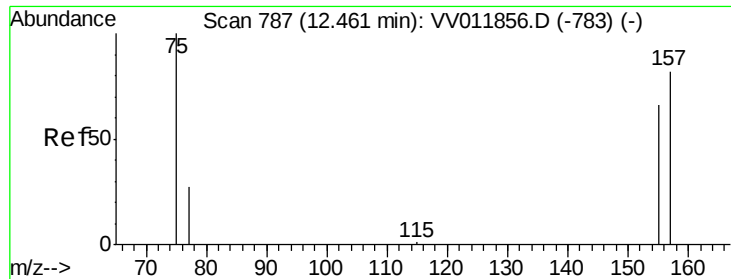

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.038 ug/L m
 RT: 12.46 min Scan# 787
 Delta R.T. 0.00 min
 Lab File: VV011858.D
 Acq: 11 Jul 2019 16:57

Instrument :
 MSVOA_V
 ClientSampleId :
 MDL06

Tgt Ion	Ratio	Lower	Upper
75	100		
157	87.9	62.2	93.4
155	86.4	55.6	83.4

Manual Integrations
 APPROVED

MMDadoda
 7/12/2019 5:31:26 PM

