


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV071119\
Data File : VV011855.D
Acq On : 11 Jul 2019 13:33
Operator : SY/MD
Sample : BFB12
Misc : 25ML/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB12

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR070819SIM.M
Title : TRACE VOA SOM01.0
Last Update : Mon Jul 15 07:23:05 2019

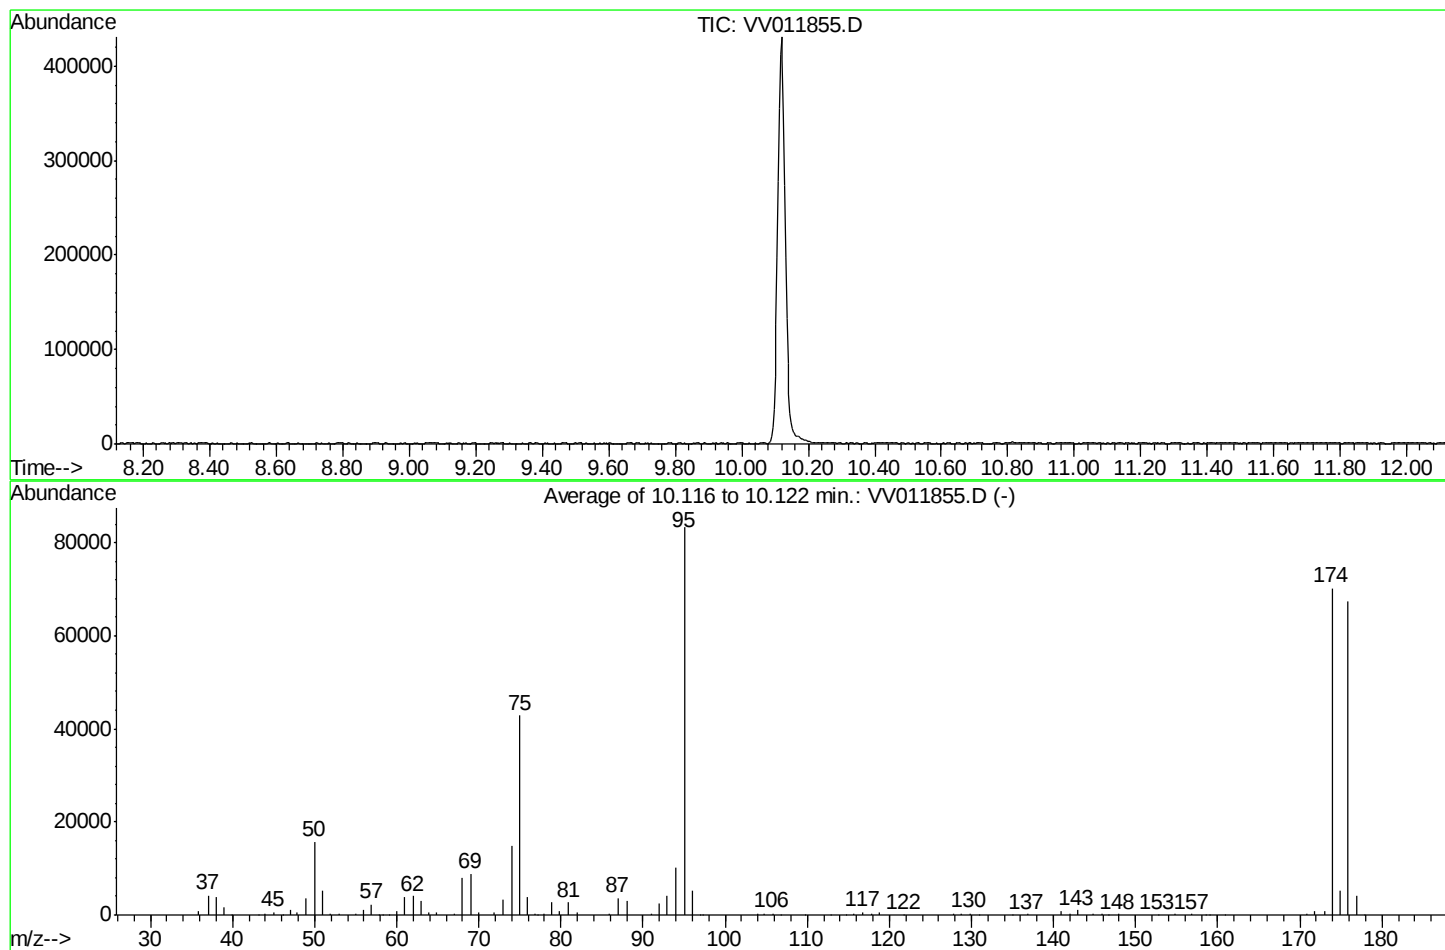

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	15794	PASS
75	95	30	80	51.5	42850	PASS
95	95	100	100	100.0	83277	PASS
96	95	5	9	6.4	5292	PASS
173	174	0.00	2	1.1	791	PASS
174	95	50	120	84.3	70162	PASS
175	174	5	9	7.5	5273	PASS
176	174	95	101	96.1	67434	PASS
177	176	5	9	6.3	4269	PASS

m/z	Abundance
39.80	179.0
43.90	457.0

Instrument :
MSVOA_V
ClientSampleId :
BFB12

m/z	Abundance
35.90	854.0
37.00	4464.0
38.00	3713.0
39.00	1545.0
39.80	249.0
43.10	110.0
43.90	764.0
44.90	730.0
47.00	1133.0
47.90	455.0
49.00	3610.0
50.00	15516.0
51.00	5107.0
51.90	186.0
52.90	196.0
54.90	261.0
56.00	1208.0
56.90	2425.0
57.70	105.0
58.30	128.0
59.10	101.0
60.00	724.0
60.90	3745.0
62.00	3939.0
63.00	3292.0
63.90	457.0
64.80	539.0
67.00	266.0
67.90	8144.0
69.00	9217.0
70.00	676.0
71.90	456.0
72.90	3359.0
74.00	14671.0
75.00	42832.0
75.90	3725.0
76.90	436.0
77.90	301.0
78.90	2655.0
79.90	891.0
80.90	2769.0
81.90	574.0
85.80	192.0
86.90	3750.0
88.00	3076.0
91.00	393.0
91.90	2572.0
92.90	4075.0
93.90	10175.0
95.00	83472.0
96.00	5370.0
97.20	144.0
103.90	342.0
104.80	136.0
105.80	400.0
106.70	117.0
109.70	118.0
114.70	129.0
115.70	407.0
116.80	720.0
117.90	357.0
118.80	490.0
127.80	320.0
128.80	208.0
129.80	407.0
130.90	150.0
134.90	141.0
136.80	171.0
140.90	843.0
142.00	169.0
142.90	1086.0
144.90	290.0
145.90	148.0
147.90	272.0
155.00	192.0
156.90	216.0
158.70	111.0
160.90	137.0
170.80	191.0
171.90	844.0
173.90	68304.0
174.90	5303.0
175.90	65056.0
176.90	4170.0
177.90	133.0

Instrument :
MSVOA_V
ClientSampleId :
BFB12

m/z	Abundance
35.90	935.0
37.00	4421.0
37.90	4004.0
39.00	1643.0
39.90	225.0
43.90	771.0
44.90	672.0
47.00	1151.0
47.90	439.0
49.00	3806.0
50.00	16315.0
51.00	5366.0
51.90	200.0
52.90	152.0
54.90	240.0
56.00	1199.0
56.90	2394.0
57.80	125.0
58.30	103.0
60.00	833.0
60.90	3854.0
62.00	4148.0
63.00	3239.0
63.90	444.0
64.90	584.0
67.00	284.0
67.90	8454.0
69.00	9047.0
70.00	663.0
71.80	516.0
72.90	3466.0
74.00	15389.0
75.00	44392.0
76.00	3902.0
76.90	415.0
77.90	316.0
78.90	2714.0
79.80	882.0
80.90	2837.0
81.90	637.0
85.90	194.0
86.90	3746.0
88.00	3253.0
91.00	349.0
91.90	2675.0
92.90	4243.0
94.00	10504.0
95.00	85936.0
96.00	5410.0
96.90	112.0
103.90	374.0
104.70	194.0
105.80	423.0
106.70	112.0
109.70	123.0
114.70	156.0
115.70	435.0
116.80	728.0
117.90	395.0
118.90	549.0
121.70	103.0
127.80	400.0
128.80	199.0
129.80	393.0
130.90	119.0
134.90	117.0
136.80	189.0
140.90	901.0
142.00	175.0
142.90	1066.0
144.80	284.0
145.80	190.0
147.90	284.0
152.70	109.0
154.80	174.0
156.80	233.0
158.60	121.0
160.80	141.0
170.80	177.0
171.90	831.0
173.00	1206.0
173.90	72760.0
174.90	5456.0
175.90	69800.0
176.90	4424.0
177.90	123.0

Instrument :
MSVOA_V
ClientSampleId :
BFB12

m/z	Abundance
35.90	926.0
37.00	3859.0
38.00	3663.0
39.00	1521.0
39.90	198.0
44.00	733.0
45.00	634.0
46.10	122.0
47.00	953.0
47.80	429.0
48.90	3544.0
50.00	15553.0
51.00	4962.0
51.90	185.0
52.90	147.0
55.00	227.0
56.00	1048.0
56.90	2068.0
57.90	145.0
60.00	849.0
60.90	3619.0
62.00	4024.0
63.00	2978.0
64.00	396.0
65.00	599.0
66.90	277.0
68.00	7748.0
69.00	8221.0
70.00	528.0
71.80	528.0
72.90	3176.0
74.00	14225.0
75.00	41328.0
76.00	3546.0
76.90	368.0
77.10	380.0
77.80	288.0
78.90	2587.0
79.90	796.0
80.90	2644.0
81.90	693.0
86.00	160.0
86.90	3398.0
88.00	3020.0
91.00	300.0
91.90	2453.0
92.90	4155.0
94.00	9996.0
95.00	80424.0
96.00	5098.0
97.00	143.0
103.90	377.0
104.70	215.0
105.80	402.0
112.80	104.0
114.60	153.0
115.70	377.0
116.80	628.0
117.90	386.0
118.90	552.0
121.80	136.0
127.80	413.0
128.70	169.0
129.80	337.0
135.00	105.0
136.90	167.0
140.90	892.0
141.90	124.0
142.90	1005.0
144.80	239.0
145.80	191.0
146.70	101.0
147.90	271.0
152.70	141.0
154.70	198.0
156.80	208.0
158.50	120.0
159.00	103.0
160.90	140.0
170.80	148.0
171.80	747.0
173.00	1168.0
173.90	69424.0
174.90	5060.0
175.90	67448.0
176.90	4213.0
177.80	113.0

Instrument :
MSVOA_V
ClientSampleId :
BFB12