
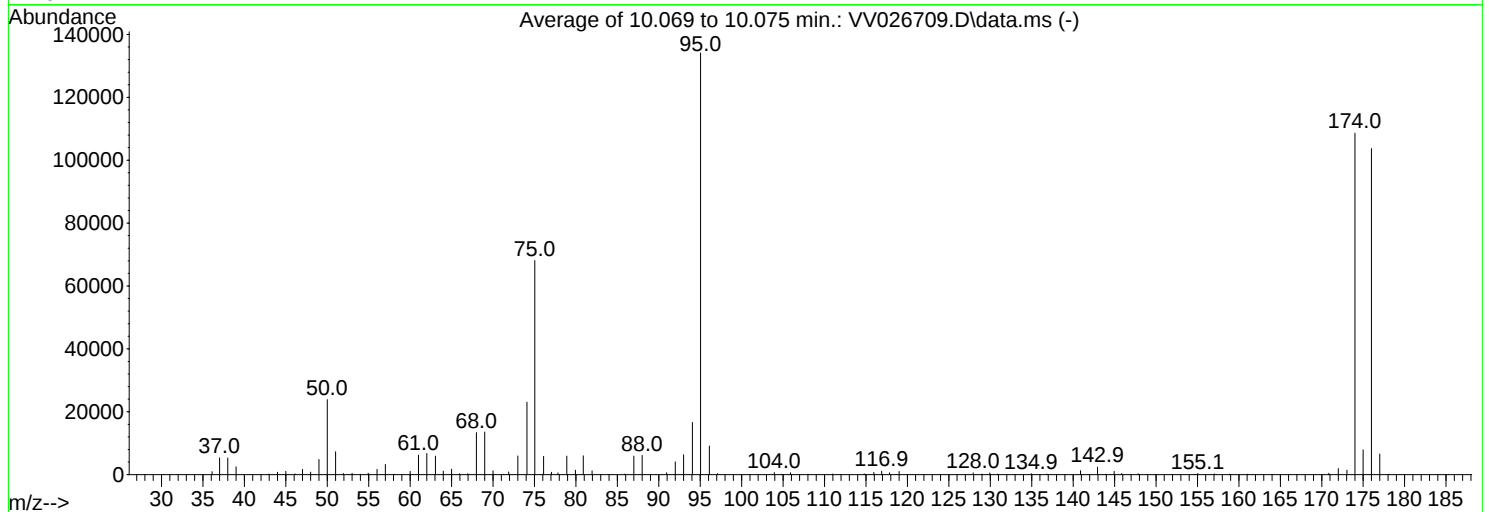


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071122\
 Data File : VV026709.D
 Acq On : 11 Jul 2022 17:51
 Operator : SY/MD
 Sample : BFB342
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB342

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Tue Jul 12 06:00:16 2022

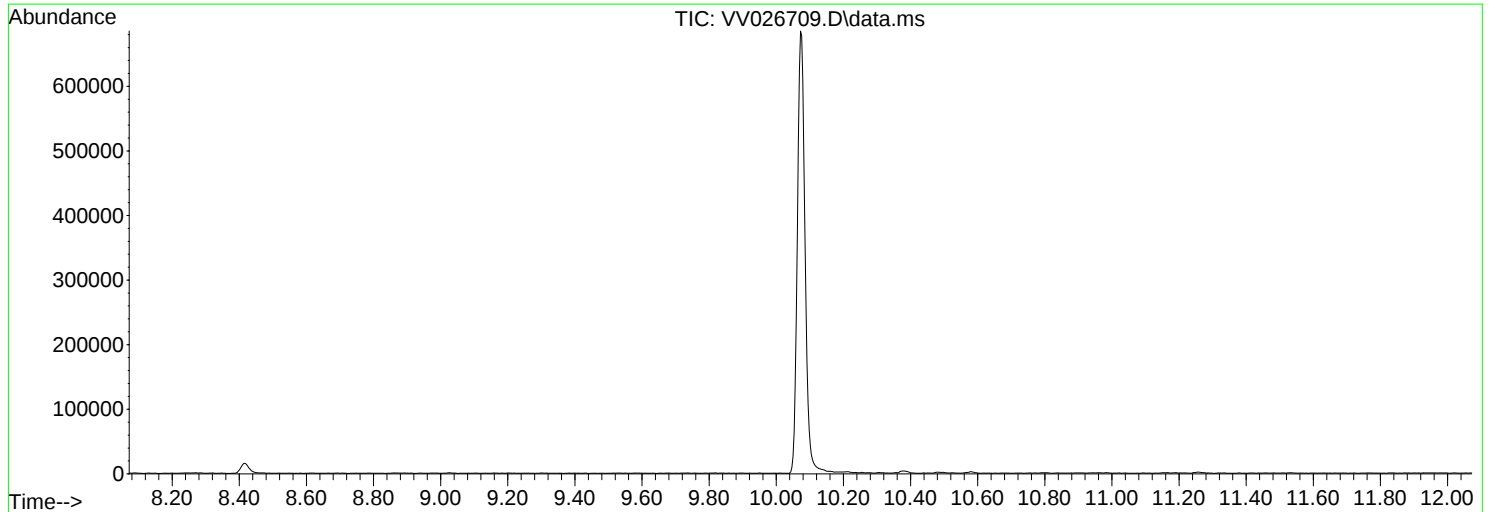

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	23848	PASS
75	95	30	80	50.8	68096	PASS
95	95	100	100	100.0	134147	PASS
96	95	5	9	6.8	9106	PASS
173	174	0.00	2	1.3	1443	PASS
174	95	50	120	80.9	108571	PASS
175	174	5	9	7.3	7910	PASS
176	174	95	105	95.5	103717	PASS
177	176	5	10	6.3	6584	PASS

m/z	Abundance
35.40	115.0
40.00	339.0
44.00	541.0

Instrument :
MSVOA_V
ClientSampleId :
BFB342

m/z	Abundance
36.10	1044.0
37.00	5230.0
38.00	5233.0
39.00	2406.0
39.90	486.0
42.90	171.0
44.00	1312.0
45.00	1030.0
46.10	236.0
47.00	1630.0
48.00	712.0
49.00	4621.0
50.00	22816.0
51.00	6839.0
51.90	334.0
53.00	341.0
54.00	158.0
55.00	412.0
56.00	1702.0
57.00	3049.0
58.00	129.0
60.00	1150.0
61.00	5824.0
62.00	6316.0
63.10	5578.0
64.00	1145.0
65.00	1628.0
66.00	327.0
66.90	272.0
68.00	12495.0
69.00	12975.0
70.00	1187.0
71.30	116.0
71.90	802.0
73.00	5583.0
74.10	21592.0
75.10	65920.0
76.10	5559.0
77.10	712.0
77.80	576.0
78.90	5537.0
80.00	1457.0
80.90	5699.0
82.00	1181.0
83.00	106.0
85.90	365.0
87.00	5596.0
88.00	5657.0
91.00	609.0
92.00	3576.0
93.00	6100.0
94.00	16067.0
95.00	127304.0
96.10	8824.0
97.10	359.0
103.90	583.0
104.80	150.0
105.90	589.0
106.90	135.0
108.00	156.0
110.00	116.0
110.90	193.0
111.80	102.0
114.80	270.0
115.90	682.0
116.90	1153.0
117.90	660.0
119.00	917.0
128.00	579.0
129.00	186.0
129.90	485.0
130.80	165.0
134.90	286.0
136.80	231.0
140.90	1179.0
143.00	2349.0
143.90	192.0
145.00	1009.0
145.90	325.0
146.90	155.0
147.80	283.0
152.90	104.0
154.70	311.0
155.10	293.0
157.00	211.0
158.80	168.0
161.10	166.0
170.90	532.0
172.00	1805.0
173.10	1369.0
174.00	100440.0
175.00	7492.0

Instrument :
MSVOA_V
ClientSampleId :
BFB342

176.0095024.0

177.006202.0

178.10164.0

Instrument :
MSVOA_V
ClientSampleId :
BFB342

m/z	Abundance
36.10	1019.0
37.00	5574.0
38.00	5466.0
39.00	2639.0
40.00	409.0
43.00	187.0
44.00	1369.0
45.00	1122.0
46.10	242.0
47.00	1789.0
48.00	857.0
49.00	5016.0
50.00	24768.0
51.00	7482.0
52.00	337.0
53.00	420.0
54.00	173.0
55.00	551.0
56.00	1725.0
57.00	3354.0
58.00	148.0
60.00	1124.0
61.00	6364.0
62.00	7019.0
63.00	6000.0
64.00	1142.0
65.00	1793.0
66.00	341.0
66.90	328.0
68.00	13924.0
69.00	13855.0
70.00	1260.0
71.30	165.0
71.90	945.0
73.00	6161.0
74.10	23832.0
75.10	70568.0
76.10	6017.0
77.10	781.0
77.90	543.0
78.90	6060.0
79.90	1465.0
80.90	6152.0
81.90	1233.0
85.90	310.0
87.00	5979.0
88.00	6391.0
91.00	670.0
92.00	4188.0
93.00	6530.0
94.10	17256.0
95.00	138816.0
96.10	9461.0
97.10	346.0
103.90	672.0
104.80	160.0
105.90	658.0
106.90	126.0
108.00	164.0
110.00	132.0
110.90	234.0
111.90	113.0
113.00	120.0
114.80	256.0
115.90	721.0
116.90	1159.0
117.80	662.0
119.00	1077.0
128.00	598.0
129.00	204.0
130.00	588.0
130.80	179.0
135.00	293.0
136.80	204.0
140.90	1318.0
143.00	2487.0
143.90	164.0
145.00	1119.0
145.90	365.0
146.90	111.0
147.80	312.0
152.90	128.0
155.00	356.0
157.10	250.0
158.90	190.0
161.10	160.0
170.90	458.0
172.00	1984.0
173.10	1453.0
174.00	112400.0
175.00	8107.0
176.00	107328.0

Instrument :
MSVOA_V
ClientSampleId :
BFB342

177.00	6817.0
178.10	142.0

Instrument :
MSVOA_V
ClientSampleId :
BFB342

m/z	Abundance
36.10	903.0
37.00	5244.0
38.00	5198.0
39.00	2518.0
39.90	404.0
40.80	163.0
43.00	221.0
44.00	1313.0
45.00	1081.0
46.10	228.0
47.00	1665.0
48.00	900.0
49.00	4886.0
50.00	23960.0
51.00	7450.0
52.00	345.0
53.00	403.0
54.00	146.0
54.90	496.0
56.00	1703.0
57.00	3391.0
58.10	188.0
60.00	993.0
61.00	6405.0
62.00	6863.0
63.00	6200.0
64.00	1082.0
65.00	1763.0
65.90	266.0
67.00	383.0
68.00	13688.0
69.00	13706.0
70.00	1251.0
71.90	922.0
73.00	6188.0
74.10	23744.0
75.00	67800.0
76.10	5781.0
77.00	811.0
77.90	517.0
78.90	6098.0
79.90	1324.0
80.90	6121.0
81.90	1188.0
87.00	6219.0
88.00	6236.0
90.90	629.0
92.00	4448.0
93.00	6368.0
94.00	16496.0
95.10	136320.0
96.10	9034.0
97.10	314.0
104.00	693.0
104.80	173.0
105.90	656.0
107.00	110.0
108.00	196.0
110.00	142.0
111.00	237.0
112.00	123.0
112.90	170.0
114.80	224.0
116.00	688.0
116.90	1030.0
117.80	576.0
119.00	1121.0
127.90	559.0
129.00	196.0
129.90	602.0
130.90	213.0
135.00	285.0
136.90	209.0
140.90	1388.0
141.80	164.0
142.90	2402.0
144.00	115.0
144.90	1043.0
145.80	380.0
147.90	370.0
149.90	113.0
152.90	143.0
155.00	377.0
157.10	250.0
158.90	181.0
161.00	202.0
170.80	392.0
172.00	2049.0
173.00	1508.0
174.00	112872.0
175.00	8132.0
176.00	108800.0

Instrument :
MSVOA_V
ClientSampleId :
BFB342

177.006733.0

178.10123.0

Instrument :
MSVOA_V
ClientSampleId :
BFB342