

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071123\
 Data File : VV031675.D
 Acq On : 11 Jul 2023 12:29
 Operator : SY/MD
 Sample : VIBLK224
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK224

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM071123WMA.M
 Title : VOC Analysis

Signal : TIC: VV031675.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	94	rVB	81852	93339	11.37%	1.304%
2	1.532	147	153	167	rVB	91532	115477	14.07%	1.613%
3	2.063	309	318	329	rBV2	136583	200403	24.41%	2.800%
4	2.243	366	374	389	rVB2	16856	26988	3.29%	0.377%
5	2.372	410	414	415	rBV4	799	551	0.07%	0.008%
6	2.449	430	438	451	rVB4	6262	11129	1.36%	0.155%
7	2.516	455	459	466	rVB5	961	973	0.12%	0.014%
8	2.590	468	482	491	rBV5	3233	8041	0.98%	0.112%
9	2.706	510	518	528	rVB6	6658	11997	1.46%	0.168%
10	2.786	539	543	545	rBV3	653	507	0.06%	0.007%
11	3.105	635	642	643	rBV4	1112	1173	0.14%	0.016%
12	3.166	658	661	666	rVB3	698	705	0.09%	0.010%
13	3.288	696	699	701	rVB2	657	413	0.05%	0.006%
14	3.400	730	734	738	rBV3	552	442	0.05%	0.006%
15	3.728	831	836	838	rBV2	581	451	0.05%	0.006%
16	3.796	847	857	892	rBV	99490	290874	35.43%	4.064%
17	4.166	964	972	974	rBV6	1826	2207	0.27%	0.031%
18	4.259	984	1001	1026	rBV	148855	393089	47.88%	5.492%
19	4.577	1094	1100	1101	rBV5	1636	1542	0.19%	0.022%
20	4.748	1143	1153	1158	rVV6	1201	2311	0.28%	0.032%
21	4.777	1158	1162	1165	rVV2	689	602	0.07%	0.008%
22	4.963	1201	1220	1249	rBV2	294947	820925	100.00%	11.469%
23	5.256	1308	1311	1314	rBV4	617	430	0.05%	0.006%
24	5.410	1356	1359	1363	rBV3	683	549	0.07%	0.008%
25	5.474	1372	1379	1384	rBV2	715	819	0.10%	0.011%
26	5.542	1387	1400	1420	rBV	281134	582010	70.90%	8.131%
27	5.831	1479	1490	1510	rVB5	26577	61317	7.47%	0.857%
28	5.995	1527	1541	1569	rBV	214075	457045	55.67%	6.385%
29	6.227	1608	1613	1615	rBV3	677	554	0.07%	0.008%
30	6.249	1617	1620	1623	rVB	676	422	0.05%	0.006%
31	6.272	1623	1627	1632	rVB4	714	621	0.08%	0.009%
32	6.304	1632	1637	1639	rBV4	759	740	0.09%	0.010%
33	6.449	1678	1682	1685	rVV4	613	490	0.06%	0.007%
34	6.516	1697	1703	1707	rBV5	1384	1450	0.18%	0.020%
35	6.571	1714	1720	1722	rBV4	1217	1332	0.16%	0.019%
36	6.735	1765	1771	1775	rBV2	654	744	0.09%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW071123\
 Data File : VW031675.D
 Acq On : 11 Jul 2023 12:29
 Operator : SY/MD
 Sample : VIBLK224
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK224

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM071123WMA.M
 Title : VOC Analysis

37	6.921	1816	1829	1864	rBV	82415	167301	20.38%	2.337%
38	7.185	1902	1911	1920	rBV6	2685	4618	0.56%	0.065%
39	7.249	1920	1931	1953	rBV	223394	407289	49.61%	5.690%
40	7.468	1996	1999	2004	rVB2	1135	820	0.10%	0.011%
41	7.503	2005	2010	2014	rBV3	481	503	0.06%	0.007%
42	7.561	2018	2028	2055	rBV	66538	127171	15.49%	1.777%
43	7.776	2089	2095	2096	rBV3	1922	1375	0.17%	0.019%
44	7.883	2117	2128	2133	rBV2	7283	12234	1.49%	0.171%
45	8.034	2163	2175	2208	rBV	298188	589104	71.76%	8.230%
46	8.487	2311	2316	2317	rBV3	612	405	0.05%	0.006%
47	8.793	2398	2411	2437	rBV	396600	685243	83.47%	9.573%
48	8.960	2455	2463	2475	rBV2	5078	8851	1.08%	0.124%
49	9.005	2475	2477	2482	rVV3	744	564	0.07%	0.008%
50	9.088	2493	2503	2514	rBV4	5324	9196	1.12%	0.128%
51	9.220	2541	2544	2552	rVB4	640	727	0.09%	0.010%
52	9.262	2552	2557	2561	rBV5	832	966	0.12%	0.013%
53	9.413	2598	2604	2607	rVB3	964	983	0.12%	0.014%
54	9.487	2619	2627	2629	rBV5	5299	5656	0.69%	0.079%
55	9.680	2675	2687	2694	rBV7	2573	3893	0.47%	0.054%
56	9.876	2740	2748	2756	rBV4	5190	7857	0.96%	0.110%
57	10.034	2795	2797	2802	rVB3	617	421	0.05%	0.006%
58	10.159	2822	2836	2852	rBV	343222	545608	66.46%	7.622%
59	10.333	2880	2890	2900	rVB	9749	14824	1.81%	0.207%
60	10.442	2921	2924	2927	rVV3	828	635	0.08%	0.009%
61	10.484	2927	2937	2947	rVV4	6260	10521	1.28%	0.147%
62	10.600	2969	2973	2978	rVB4	741	654	0.08%	0.009%
63	10.645	2983	2987	2989	rBV4	802	698	0.09%	0.010%
64	10.680	2993	2998	2999	rBV2	601	409	0.05%	0.006%
65	10.860	3046	3054	3066	rVB3	7173	11267	1.37%	0.157%
66	10.940	3075	3079	3081	rBV3	539	413	0.05%	0.006%
67	10.960	3081	3085	3090	rVB4	526	454	0.06%	0.006%
68	11.075	3118	3121	3122	rBV2	856	432	0.05%	0.006%
69	11.130	3128	3138	3146	rBV3	12633	20538	2.50%	0.287%
70	11.191	3146	3157	3182	rVB	341634	556580	67.80%	7.776%
71	11.448	3234	3237	3240	rBV4	807	703	0.09%	0.010%
72	11.506	3247	3255	3260	rBV8	1855	3163	0.39%	0.044%
73	11.567	3262	3274	3293	rVV	298302	493532	60.12%	6.895%
74	11.718	3319	3321	3324	rBV2	635	419	0.05%	0.006%
75	11.895	3373	3376	3379	rBV5	939	690	0.08%	0.010%
76	12.201	3463	3471	3480	rVV3	4949	7370	0.90%	0.103%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071123\
 Data File : VV031675.D
 Acq On : 11 Jul 2023 12:29
 Operator : SY/MD
 Sample : VIBLK224
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK224

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM071123WMA.M
 Title : VOC Analysis

77	12.297	3495	3501	3503	rBV5	2809	2970	0.36%	0.041%
78	12.371	3516	3524	3534	rBV5	7242	11236	1.37%	0.157%
79	12.474	3552	3556	3558	rBV2	840	633	0.08%	0.009%
80	12.590	3582	3592	3610	rVB3	24446	39919	4.86%	0.558%
81	12.731	3634	3636	3639	rBV2	854	466	0.06%	0.007%
82	12.853	3672	3674	3679	rVV3	706	453	0.06%	0.006%
83	12.879	3680	3682	3685	rVB4	879	415	0.05%	0.006%
84	12.931	3694	3698	3699	rBV3	606	425	0.05%	0.006%
85	12.960	3704	3707	3709	rBV3	634	425	0.05%	0.006%
86	12.988	3709	3716	3718	rBV4	801	783	0.10%	0.011%
87	13.098	3745	3750	3755	rBV4	1002	1300	0.16%	0.018%
88	13.204	3774	3783	3795	rBV2	38584	59936	7.30%	0.837%
89	13.323	3818	3820	3823	rVB2	838	420	0.05%	0.006%
90	13.387	3836	3840	3841	rBV3	691	416	0.05%	0.006%
91	13.445	3848	3858	3878	rVB	91190	147332	17.95%	2.058%
92	13.519	3878	3881	3885	rBV3	772	765	0.09%	0.011%
93	13.615	3908	3911	3917	rVB3	969	964	0.12%	0.013%
94	13.686	3921	3933	3944	rVV2	55202	89104	10.85%	1.245%
95	13.850	3981	3984	3986	rBV3	783	485	0.06%	0.007%
96	13.905	3998	4001	4004	rBV2	737	546	0.07%	0.008%
97	14.207	4093	4095	4098	rBV4	993	526	0.06%	0.007%
98	14.249	4105	4108	4110	rBV3	863	559	0.07%	0.008%
99	14.371	4144	4146	4149	rBV4	864	450	0.05%	0.006%
100	14.390	4149	4152	4155	rBV3	1096	681	0.08%	0.010%




Sum of corrected areas: 7157958

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071123\
Data File : VV031675.D
Acq On : 11 Jul 2023 12:29
Operator : SY/MD
Sample : VIBLK224
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK224

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM071123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

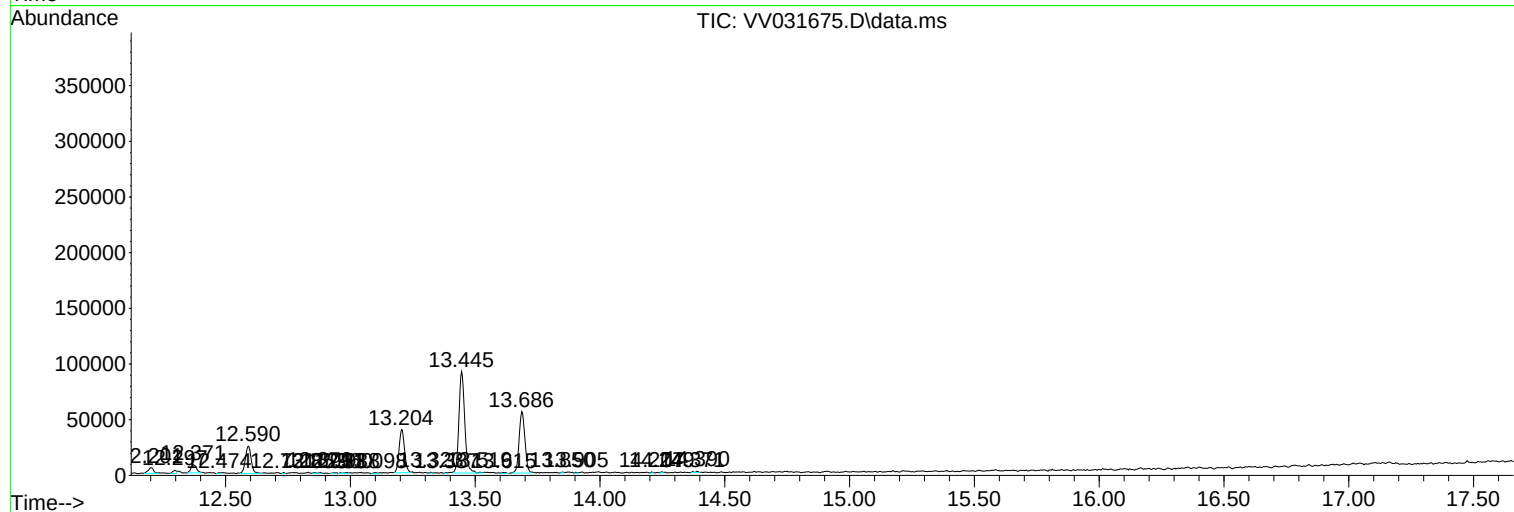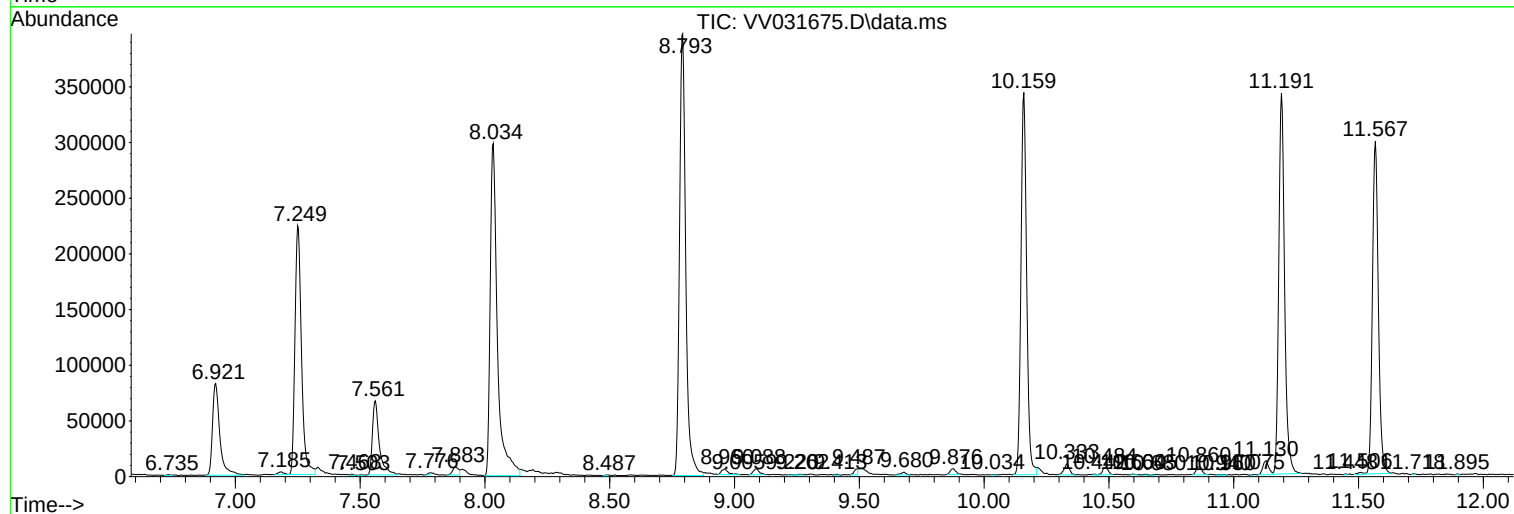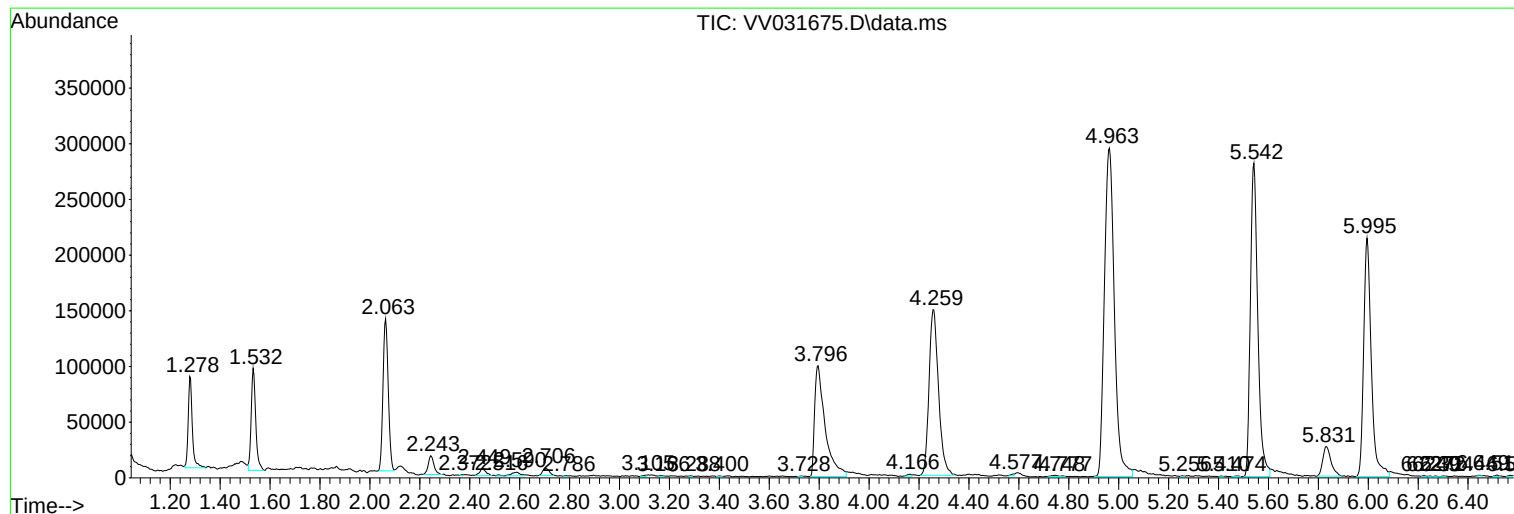

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071123\
Data File : VV031675.D
Acq On : 11 Jul 2023 12:29
Operator : SY/MD
Sample : VIBLK224
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK224

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM071123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071123\
Data File : VV031675.D
Acq On : 11 Jul 2023 12:29
Operator : SY/MD
Sample : VIBLK224
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK224

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM071123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------