

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071123\
 Data File : VV031680.D
 Acq On : 11 Jul 2023 15:43
 Operator : SY/MD
 Sample : VV0711WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK370

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM071123WMA.M
 Title : VOC Analysis

Signal : TIC: VV031680.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	95	rVB	171992	187772	13.93%	1.903%
2	1.532	146	153	168	rVB	161208	191343	14.20%	1.939%
3	2.063	309	318	336	rBV	353228	507962	37.70%	5.149%
4	2.600	483	485	488	rVB3	523	248	0.02%	0.003%
5	2.616	488	490	491	rBV3	214	74	0.01%	0.001%
6	2.664	503	505	509	rBV2	447	350	0.03%	0.004%
7	2.703	511	517	531	rVB6	2824	5662	0.42%	0.057%
8	2.789	541	544	545	rBV3	576	312	0.02%	0.003%
9	2.985	603	605	606	rBV2	308	155	0.01%	0.002%
10	3.008	610	612	618	rVB3	361	310	0.02%	0.003%
11	3.034	618	620	623	rBV2	255	141	0.01%	0.001%
12	3.185	663	667	671	rVB4	279	243	0.02%	0.002%
13	3.207	671	674	679	rBV2	561	388	0.03%	0.004%
14	3.243	681	685	688	rBV	210	196	0.01%	0.002%
15	3.262	688	691	692	rBV2	348	225	0.02%	0.002%
16	3.310	703	706	709	rBV2	542	541	0.04%	0.005%
17	3.339	714	715	717	rBV2	205	67	0.00%	0.001%
18	3.362	720	722	727	rVV2	285	209	0.02%	0.002%
19	3.410	732	737	743	rBV2	384	589	0.04%	0.006%
20	3.432	743	744	747	rVB2	422	206	0.02%	0.002%
21	3.452	747	750	752	rBV2	355	222	0.02%	0.002%
22	3.532	772	775	778	rBV2	419	302	0.02%	0.003%
23	3.571	782	787	788	rBV2	340	300	0.02%	0.003%
24	3.600	793	796	799	rBV3	240	200	0.01%	0.002%
25	3.622	800	803	809	rVB3	637	558	0.04%	0.006%
26	3.651	809	812	814	rBV	389	249	0.02%	0.003%
27	3.680	818	821	824	rBV2	333	163	0.01%	0.002%
28	3.725	830	835	841	rBV2	338	387	0.03%	0.004%
29	3.793	847	856	886	rBV	98499	274007	20.33%	2.777%
30	4.256	985	1000	1030	rBV	224097	571953	42.44%	5.797%
31	4.686	1132	1134	1137	rBV2	761	492	0.04%	0.005%
32	4.805	1168	1171	1174	rBV2	385	233	0.02%	0.002%
33	4.821	1174	1176	1177	rBV	325	162	0.01%	0.002%
34	4.963	1203	1220	1247	rBV2	507117	1347540	100.00%	13.659%
35	5.317	1327	1330	1332	rBV2	759	375	0.03%	0.004%
36	5.387	1350	1352	1356	rVB5	520	330	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071123\
 Data File : VV031680.D
 Acq On : 11 Jul 2023 15:43
 Operator : SY/MD
 Sample : VV0711WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK370

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM071123WMA.M
 Title : VOC Analysis

37	5.413	1356	1360	1361	rBV	367	240	0.02%	0.002%
38	5.448	1367	1371	1373	rBV4	657	428	0.03%	0.004%
39	5.484	1380	1382	1385	rVB2	552	274	0.02%	0.003%
40	5.542	1387	1400	1421	rBV	349160	730279	54.19%	7.402%
41	5.944	1521	1525	1528	rBV3	612	408	0.03%	0.004%
42	5.995	1528	1541	1566	rBV	310308	651148	48.32%	6.600%
43	6.214	1607	1609	1612	rBV2	614	368	0.03%	0.004%
44	6.384	1660	1662	1666	rBV3	705	443	0.03%	0.004%
45	6.432	1672	1677	1680	rBV3	955	848	0.06%	0.009%
46	6.506	1695	1700	1703	rBV2	445	367	0.03%	0.004%
47	6.526	1703	1706	1710	rVB3	506	319	0.02%	0.003%
48	6.561	1715	1717	1720	rBV	628	450	0.03%	0.005%
49	6.651	1742	1745	1749	rBV4	426	270	0.02%	0.003%
50	6.696	1756	1759	1764	rBV2	323	348	0.03%	0.004%
51	6.722	1765	1767	1769	rVB2	566	245	0.02%	0.002%
52	6.731	1769	1770	1771	rBV2	177	68	0.01%	0.001%
53	6.747	1772	1775	1776	rBV	366	191	0.01%	0.002%
54	6.831	1799	1801	1803	rVB	287	116	0.01%	0.001%
55	6.844	1803	1805	1810	rBV2	394	292	0.02%	0.003%
56	6.870	1810	1813	1814	rBV	450	201	0.01%	0.002%
57	6.918	1818	1828	1859	rBV	138152	272291	20.21%	2.760%
58	7.249	1919	1931	1954	rBV	524986	935132	69.40%	9.478%
59	7.558	2017	2027	2057	rBV	105885	200715	14.89%	2.034%
60	7.847	2115	2117	2119	rVB2	393	123	0.01%	0.001%
61	7.857	2119	2120	2122	rBV	484	191	0.01%	0.002%
62	7.918	2132	2139	2147	rVB7	2200	3527	0.26%	0.036%
63	7.947	2147	2148	2150	rBV2	409	137	0.01%	0.001%
64	8.030	2164	2174	2211	rBV	293797	568467	42.19%	5.762%
65	8.683	2375	2377	2379	rBV2	495	244	0.02%	0.002%
66	8.789	2399	2410	2437	rBV	564491	940522	69.80%	9.533%
67	9.156	2521	2524	2526	rBV2	427	203	0.02%	0.002%
68	9.265	2555	2558	2560	rBV3	330	211	0.02%	0.002%
69	9.316	2571	2574	2580	rVB3	632	482	0.04%	0.005%
70	9.397	2595	2599	2602	rBV2	578	443	0.03%	0.004%
71	9.413	2602	2604	2605	rBV	300	112	0.01%	0.001%
72	9.496	2622	2630	2634	rBV5	2028	2990	0.22%	0.030%
73	9.648	2675	2677	2680	rVB2	553	238	0.02%	0.002%
74	9.734	2702	2704	2706	rBV2	443	249	0.02%	0.003%
75	9.805	2724	2726	2730	rVB4	461	271	0.02%	0.003%
76	9.879	2742	2749	2756	rBV6	2463	3176	0.24%	0.032%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071123\
 Data File : VV031680.D
 Acq On : 11 Jul 2023 15:43
 Operator : SY/MD
 Sample : VV0711WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK370

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM071123WMA.M
 Title : VOC Analysis

77	9.956	2770	2773	2775	rBV2	615	335	0.02%	0.003%
78	10.040	2797	2799	2801	rBV	367	147	0.01%	0.001%
79	10.159	2824	2836	2852	rBV	426732	675180	50.10%	6.844%
80	10.384	2902	2906	2909	rBV3	687	530	0.04%	0.005%
81	10.586	2967	2969	2971	rBV	520	311	0.02%	0.003%
82	10.757	3021	3022	3025	rVB2	352	146	0.01%	0.001%
83	10.799	3033	3035	3036	rBV	334	111	0.01%	0.001%
84	10.863	3048	3055	3065	rBV6	2281	3293	0.24%	0.033%
85	11.024	3102	3105	3108	rBV3	474	381	0.03%	0.004%
86	11.123	3132	3136	3137	rBV2	2633	1776	0.13%	0.018%
87	11.191	3146	3157	3180	rBV	556271	868404	64.44%	8.802%
88	11.490	3247	3250	3252	rBV	705	409	0.03%	0.004%
89	11.567	3262	3274	3293	rBV	560581	884492	65.64%	8.965%
90	11.930	3384	3387	3390	rBV2	663	542	0.04%	0.005%
91	12.368	3520	3523	3532	rVB6	1332	1711	0.13%	0.017%
92	13.210	3778	3785	3795	rBV7	3992	6071	0.45%	0.062%
93	13.451	3854	3860	3871	rVB3	6723	10286	0.76%	0.104%
94	13.599	3904	3906	3908	rBV2	557	263	0.02%	0.003%




Sum of corrected areas: 9865881

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071123\
Data File : VV031680.D
Acq On : 11 Jul 2023 15:43
Operator : SY/MD
Sample : VV0711WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK370

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM071123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

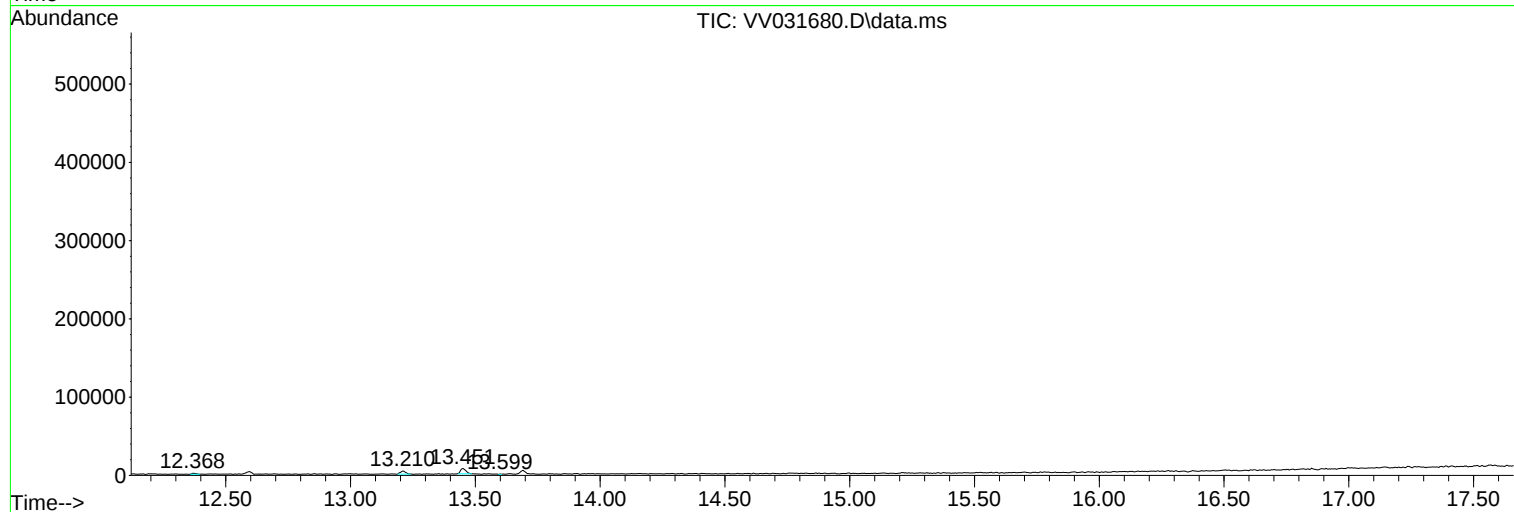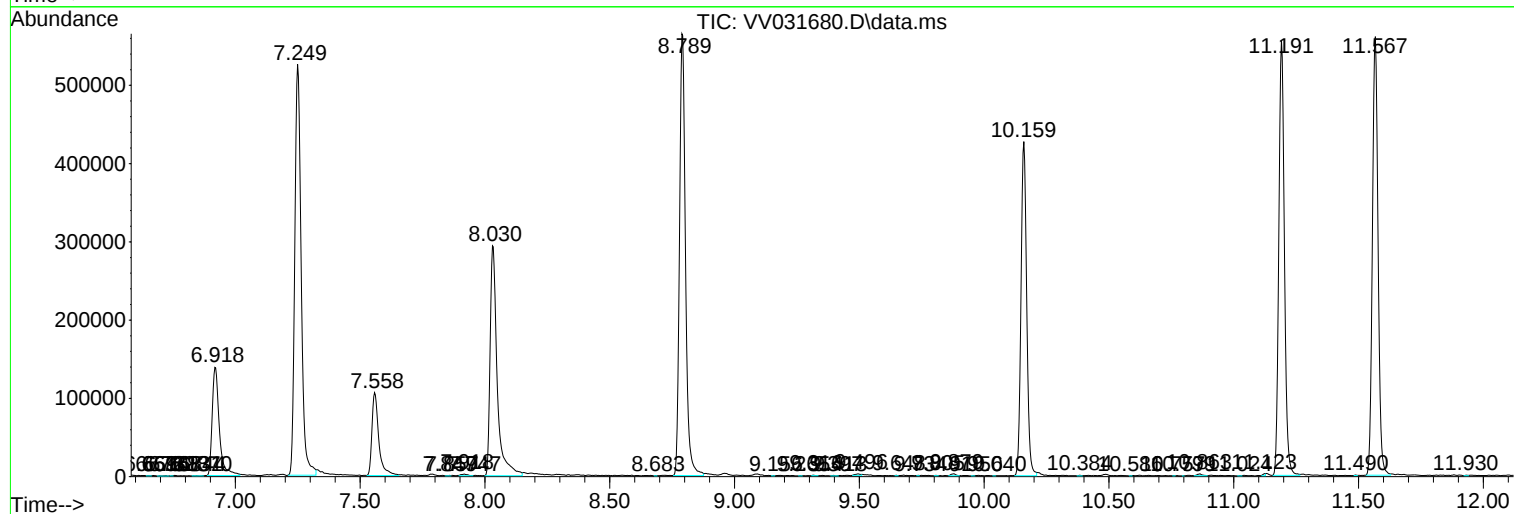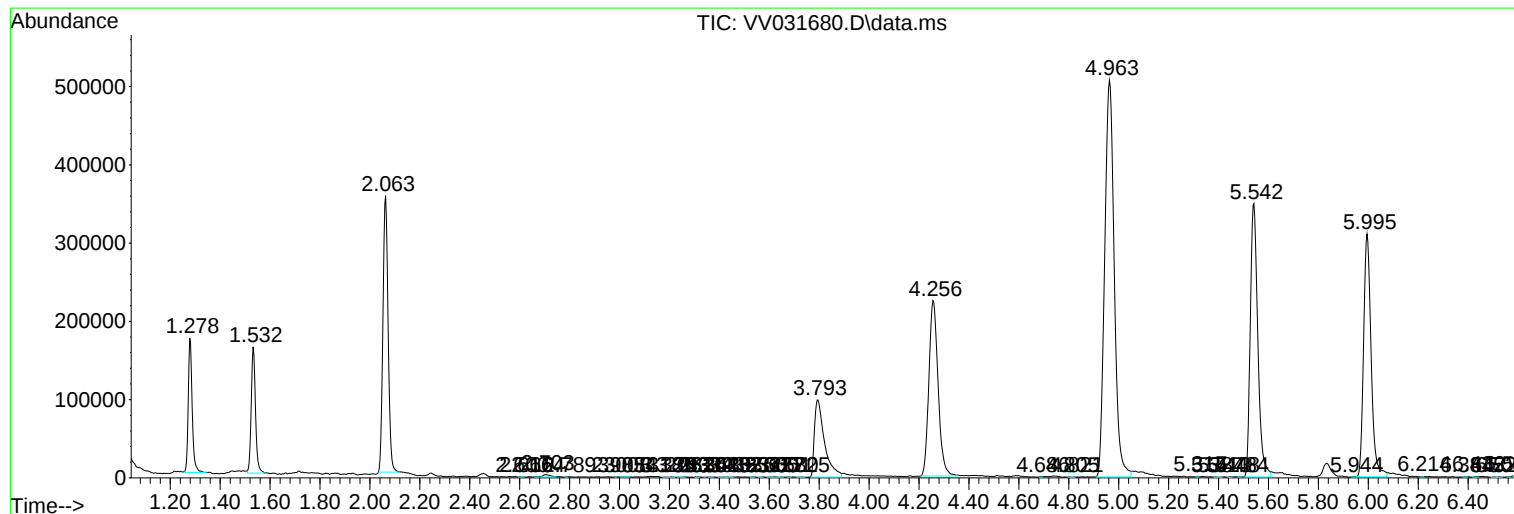

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071123\
Data File : VV031680.D
Acq On : 11 Jul 2023 15:43
Operator : SY/MD
Sample : VV0711WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK370

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM071123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071123\
Data File : VV031680.D
Acq On : 11 Jul 2023 15:43
Operator : SY/MD
Sample : VV0711WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK370

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM071123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------