


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071123\
Data File : VV031669.D
Acq On : 11 Jul 2023 09:22
Operator : SY/MD
Sample : BFB396
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB396

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM071123WMA.M
Title : VOC Analysis
Last Update : Wed Jul 12 07:50:48 2023

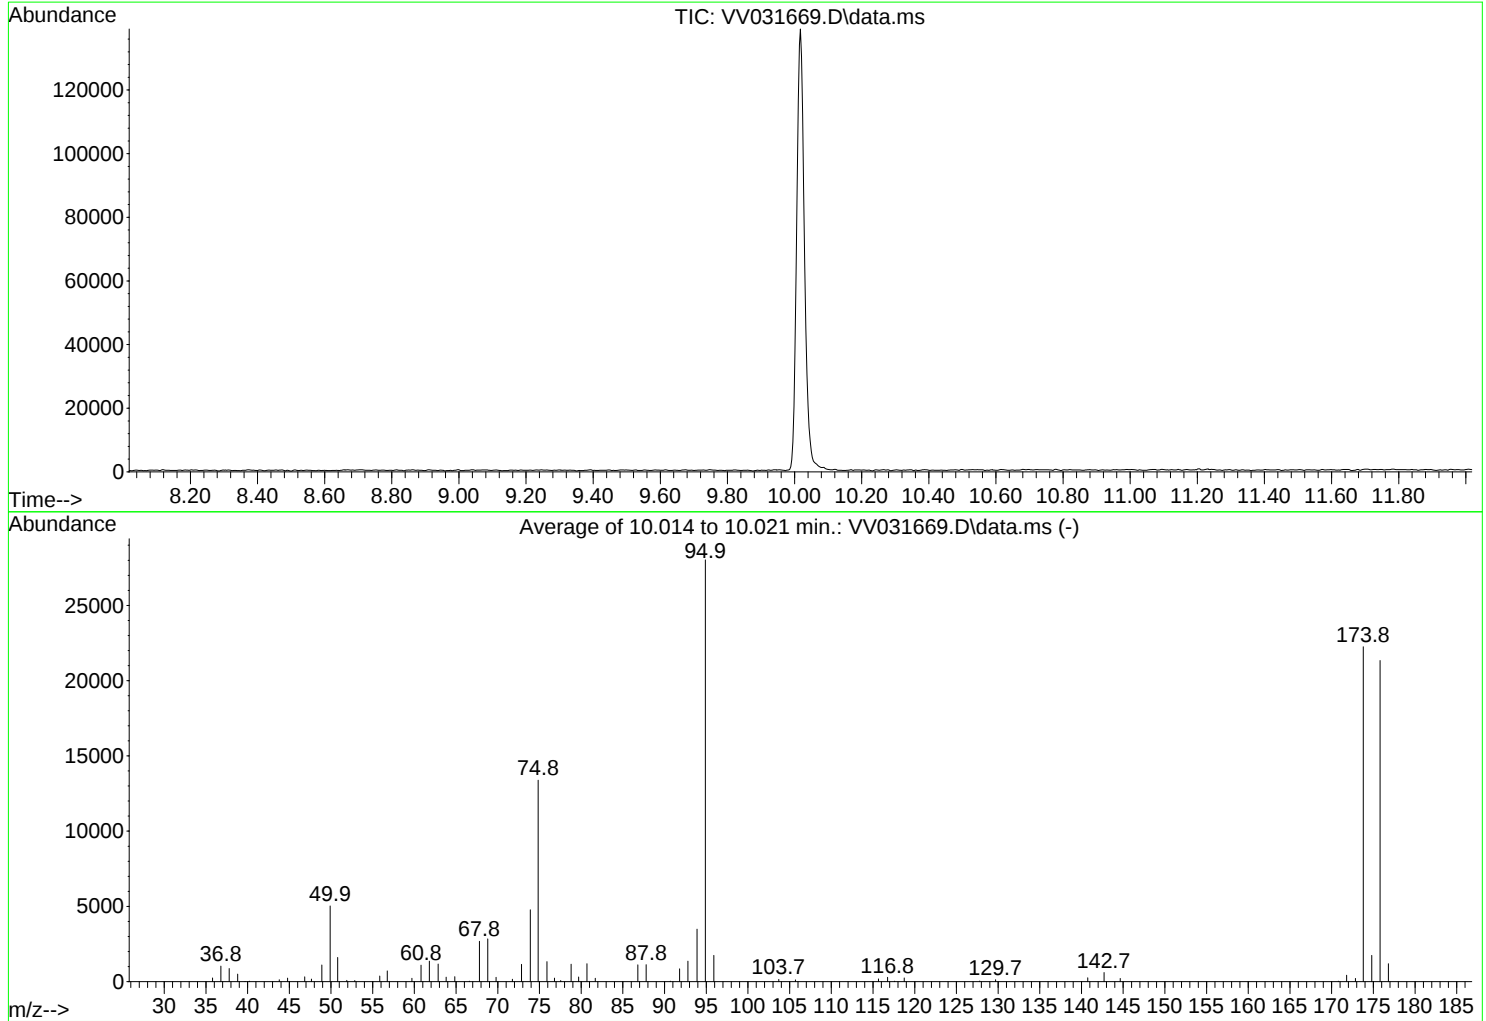

AutoFind: Scans 2791, 2792, 2793; Background Corrected with Scan 2780

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	5030	PASS
75	95	30	80	47.8	13390	PASS
95	95	100	100	100.0	28029	PASS
96	95	5	9	6.2	1740	PASS
173	174	0.00	2	1.0	212	PASS
174	95	50	120	79.4	22251	PASS
175	174	5	9	7.8	1739	PASS
176	174	95	105	95.9	21339	PASS
177	176	5	10	5.6	1192	PASS

m/z	Abundance
39.80	120.0
43.80	440.0

Instrument :
MSVOA_V
ClientSampleId :
BFB396

m/z	Abundance
35.80	260.0
36.80	997.0
37.80	918.0
38.80	532.0
39.60	108.0
43.80	611.0
44.80	244.0
46.90	311.0
47.70	174.0
48.90	1253.0
49.90	5237.0
50.80	1627.0
52.80	107.0
55.90	369.0
56.80	677.0
59.70	234.0
60.80	1184.0
61.80	1408.0
62.80	1254.0
63.80	234.0
64.90	306.0
67.80	2896.0
68.80	2838.0
69.80	277.0
71.80	184.0
72.90	1198.0
73.90	4766.0
74.80	13838.0
75.90	1236.0
76.80	217.0
78.80	1109.0
79.70	271.0
80.70	1136.0
81.70	210.0
86.80	1063.0
87.80	1038.0
91.80	812.0
92.80	1412.0
93.90	3429.0
94.90	28240.0
95.90	1780.0
103.60	159.0
105.70	117.0
115.70	176.0
116.70	273.0
118.80	244.0
129.70	125.0
140.70	262.0
142.70	621.0
144.70	248.0
171.80	387.0
172.80	286.0
173.80	21624.0
174.80	1778.0
175.80	20704.0
176.80	1207.0

Instrument :
MSVOA_V
ClientSampleId :
BFB396

m/z	Abundance
35.80	247.0
36.80	1060.0
37.80	899.0
38.80	486.0
39.60	126.0
40.20	111.0
43.80	564.0
44.80	247.0
46.80	318.0
47.60	180.0
48.90	1137.0
49.90	5227.0
50.80	1646.0
51.90	112.0
52.90	116.0
55.80	382.0
56.80	751.0
59.70	240.0
60.80	1092.0
61.80	1392.0
62.80	1179.0
63.80	292.0
64.80	336.0
66.60	104.0
67.80	2784.0
68.80	2997.0
69.80	309.0
71.70	160.0
72.80	1161.0
73.90	4870.0
74.90	13704.0
75.90	1344.0
76.80	254.0
77.50	115.0
78.80	1181.0
79.70	309.0
80.70	1207.0
81.70	226.0
86.80	1195.0
87.80	1181.0
91.80	886.0
92.80	1443.0
93.90	3627.0
94.90	28984.0
95.90	1800.0
103.70	149.0
105.70	112.0
115.70	186.0
116.70	291.0
117.60	102.0
118.70	238.0
129.70	134.0
140.80	250.0
142.70	631.0
144.70	204.0
171.80	446.0
172.90	350.0
173.80	23072.0
174.80	1799.0
175.80	21992.0
176.80	1220.0

Instrument :
MSVOA_V
ClientSampleId :
BFB396

m/z	Abundance
35.80	232.0
36.80	1030.0
37.80	807.0
38.80	483.0
39.70	167.0
43.80	539.0
44.80	221.0
46.80	328.0
47.60	160.0
48.90	930.0
49.90	4626.0
50.80	1556.0
51.90	138.0
55.80	376.0
56.70	724.0
59.70	208.0
60.80	1016.0
61.80	1271.0
62.90	1080.0
63.80	382.0
64.80	352.0
67.80	2367.0
68.80	2671.0
69.80	275.0
71.70	151.0
72.80	1080.0
73.90	4670.0
74.90	12628.0
75.90	1399.0
76.80	230.0
77.60	106.0
78.80	1185.0
79.70	339.0
80.70	1219.0
81.70	234.0
86.80	1077.0
87.80	1164.0
90.70	101.0
91.80	859.0
92.80	1242.0
93.90	3393.0
94.90	26864.0
95.90	1639.0
103.80	143.0
105.70	115.0
115.60	175.0
116.80	298.0
118.70	242.0
127.80	124.0
129.70	113.0
140.80	268.0
142.70	581.0
144.60	192.0
170.80	104.0
171.80	453.0
173.80	22056.0
174.80	1640.0
175.80	21320.0
176.80	1148.0

Instrument :
MSVOA_V
ClientSampleId :
BFB396