

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV071218\
 Data File : VV006587.D
 Acq On : 12 Jul 2018 15:50
 Operator : SY/MD
 Sample : J3919-13
 Misc : 25 mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AE9

Quant Time: Jul 13 01:47:48 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR070718WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jul 13 01:47:22 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	343887	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	309139	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	137217	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	69122	3.70	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	74.00%
7) Chloroethane-d5	1.58	69	67347	4.13	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	82.60%
11) 1,1-Dichloroethene-d2	2.13	63	97391	2.80	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	56.00%#
20) 2-Butanone-d5	3.95	46	218040	45.91	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	91.82%
24) Chloroform-d	4.41	84	157683	4.29	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.80%
26) 1,2-Dichloroethane-d4	5.09	65	74956	4.39	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.80%
32) Benzene-d6	5.10	84	324366	4.60	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.00%
36) 1,2-Dichloropropane-d6	6.12	67	104871	4.59	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	91.80%
41) Toluene-d8	7.37	98	279325	4.43	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.60%
43) trans-1,3-Dichloropropene-	7.67	79	31918	4.11	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	82.20%
46) 2-Hexanone-d5	8.14	63	202926	51.80	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	103.60%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	78190	4.35	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	87.00%
64) 1,2-Dichlorobenzene-d4	11.68	152	116266	4.93	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.60%

Target Compounds


					Qvalue
13) Acetone	2.19	43	5482	1.825 ug/L	92
21) 2-Butanone	4.03	43	2145	0.435 ug/L	74
22) cis-1,2-Dichloroethene	3.97	96	14288	0.566 ug/L	94
34) Trichloroethene	5.96	95	41346	1.747 ug/L	97
35) Methylcyclohexane	6.12	83	25704	0.674 ug/L #	29
37) 1,2-Dichloropropane	6.12	63	10341	0.458 ug/L #	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV071218\
Data File : VV006587.D
Acq On : 12 Jul 2018 15:50
Operator : SY/MD
Sample : J3919-13
Misc : 25 mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE9

Quant Time: Jul 13 01:47:48 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR070718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jul 13 01:47:22 2018
Response via : Initial Calibration

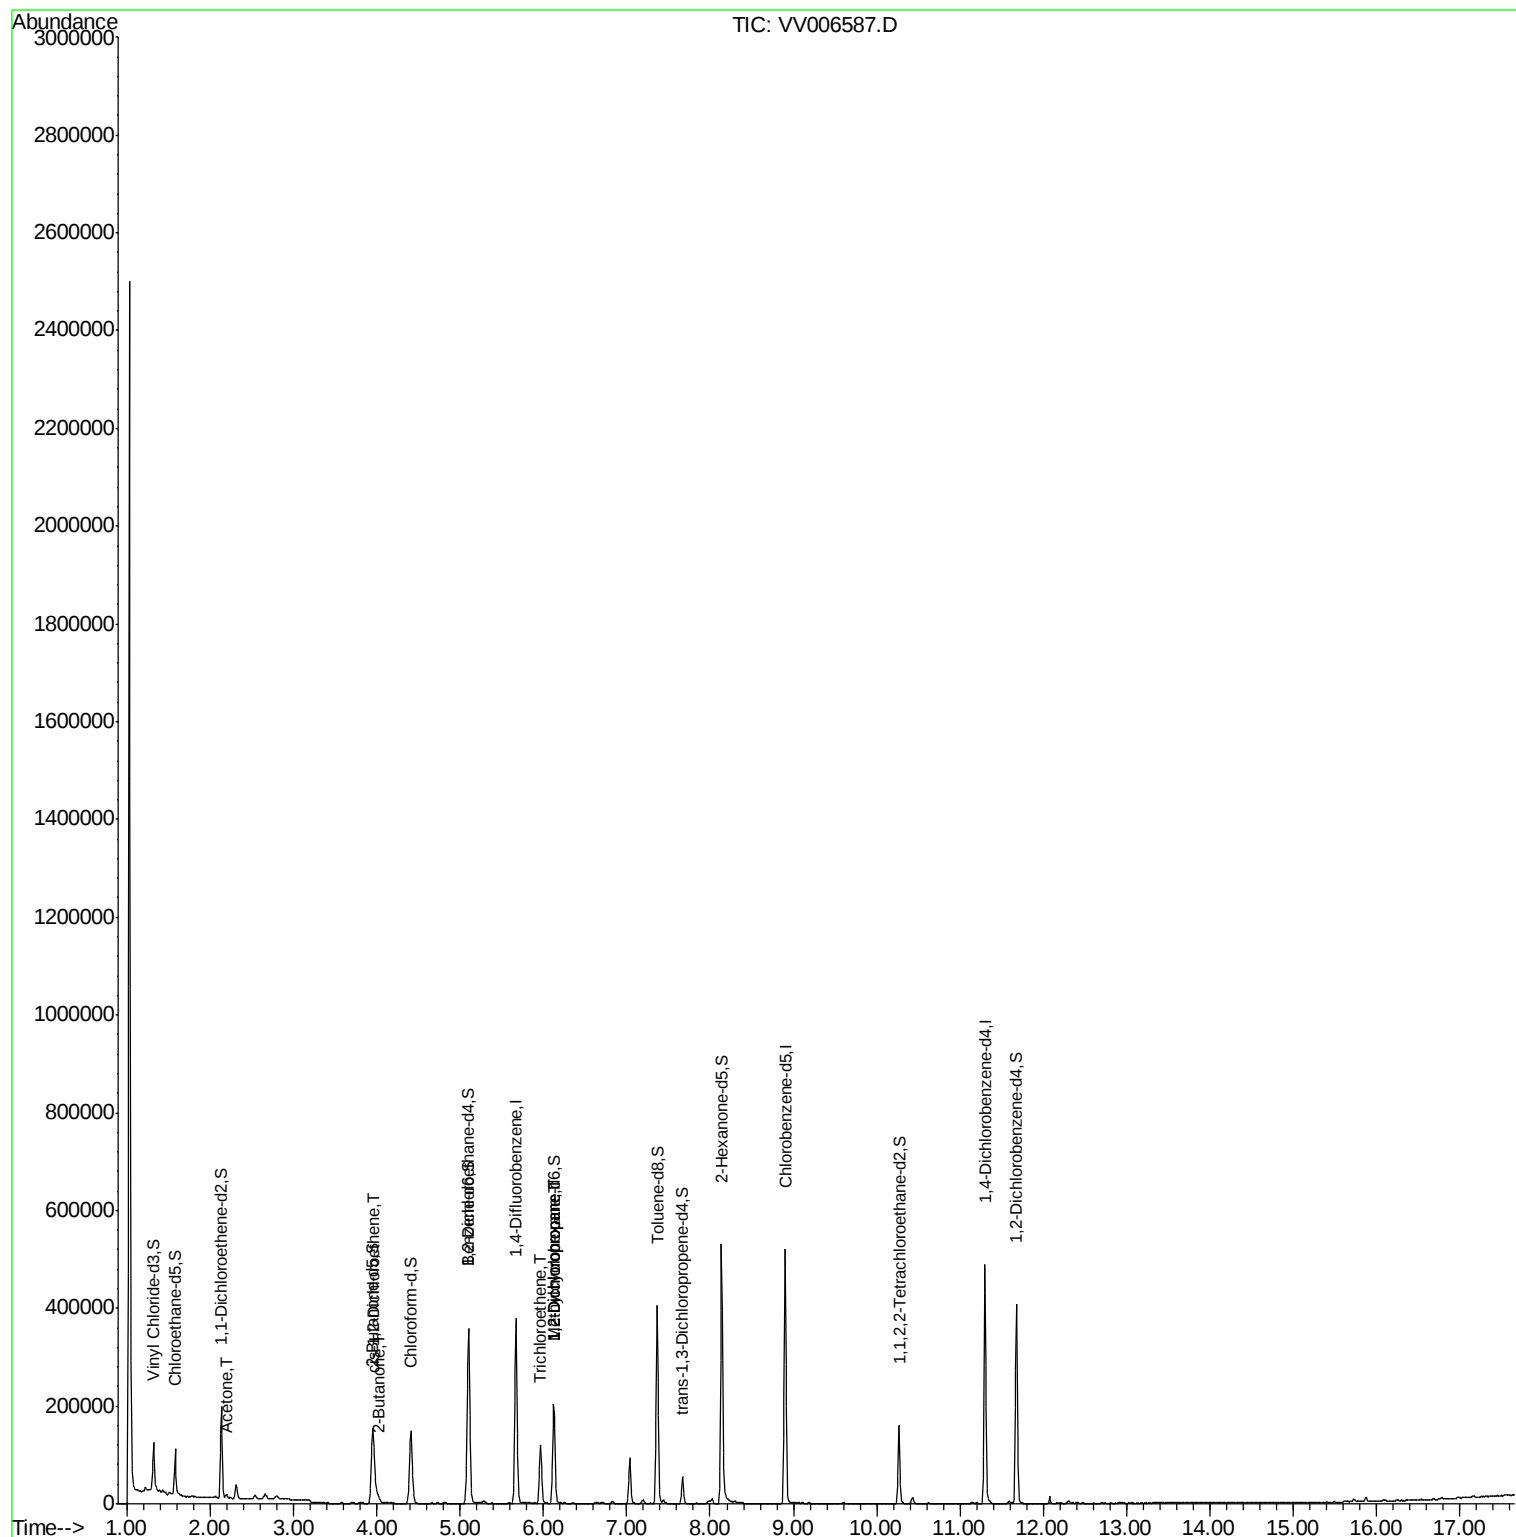

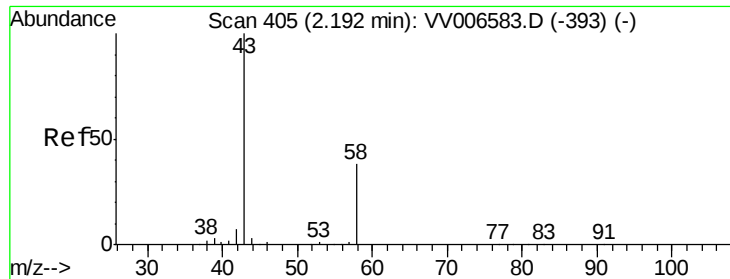

#13

Acetone

Concen: 1.825 ug/L

RT: 2.19 min Scan# 405

Delta R.T. 0.00 min

Lab File: VV006587.D

Acq: 12 Jul 2018 15:50

Instrument :

MSVOA_V

ClientSampled :


C0AE9

Tgt Ion: 43 Resp: 5482

Ion Ratio Lower Upper

43 100

58 42.8 0.0 76.2

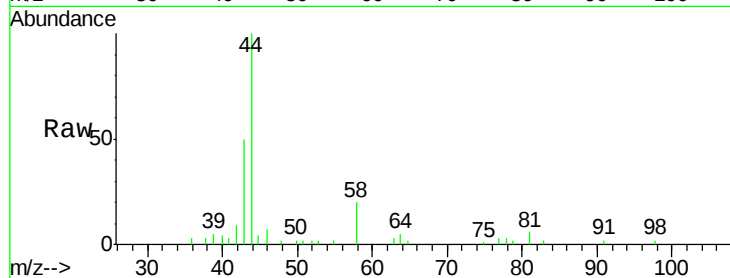

Abundance Ion 43.05 (42.75 to 43.75): VV006587.D (-312) (-)

Ion 58.05 (57.75 to 58.75): VV006587.D (-312) (-)

2.19

4000



3000

2000

1000

0

Time-->

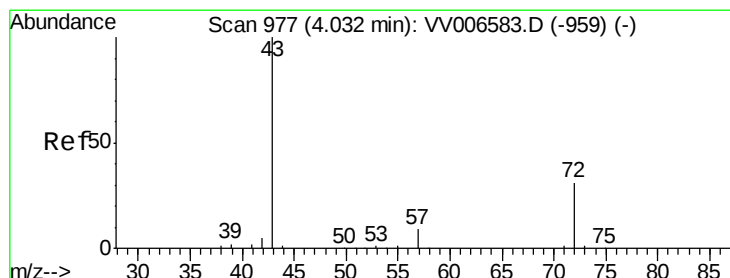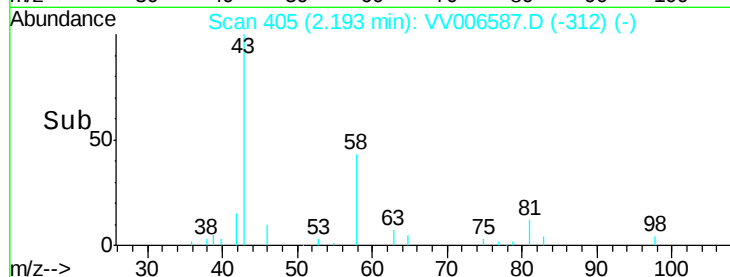

#21

2-Butanone

Concen: 0.435 ug/L

RT: 4.03 min Scan# 976

Delta R.T. -0.00 min

Lab File: VV006587.D


Acq: 12 Jul 2018 15:50

Tgt Ion: 43 Resp: 2145

Ion Ratio Lower Upper

43 100

72 16.3 15.1 45.3

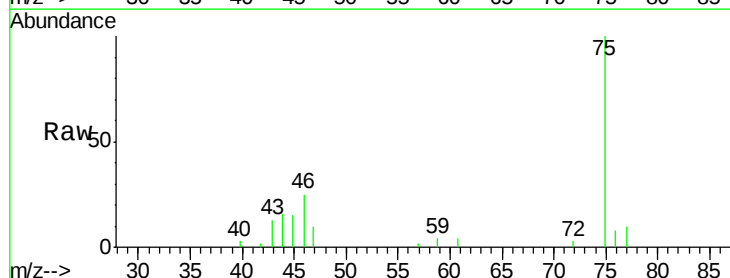

Abundance Ion 43.05 (42.75 to 43.75): VV006587.D (-884) (-)

Ion 72.10 (71.80 to 72.80): VV006587.D (-884) (-)

4.03

800


600


400

200

0

Time-->

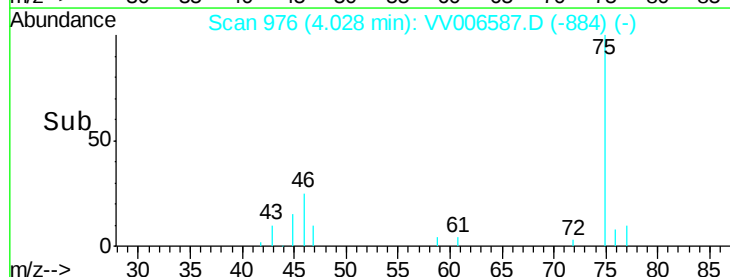

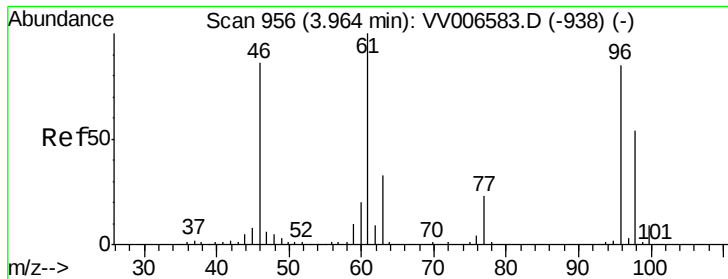


#22




cis-1,2-Dichloroethene
 Concen: 0.566 ug/L
 RT: 3.97 min Scan# 957
 Delta R.T. 0.00 min
 Lab File: VV006587.D
 Acq: 12 Jul 2018 15:50

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AE9

Tgt Ion: 96 Resp: 14288
 Ion Ratio Lower Upper
 96 100
 61 125.8 83.8 155.6
 68 0.0 0.0 0.0

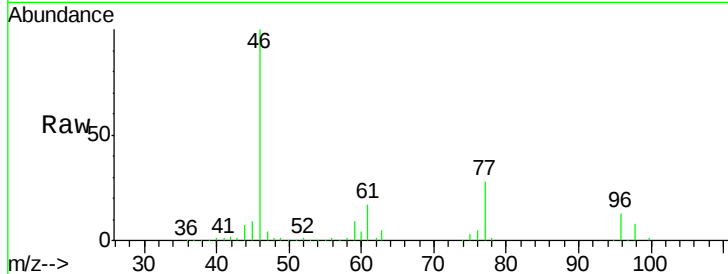


Abundance Ion 96.00 (95.70 to 96.70): VV0
 Ion 61.05 (60.75 to 61.75): VV0
 Ion 68.15 (67.85 to 68.85): VV0

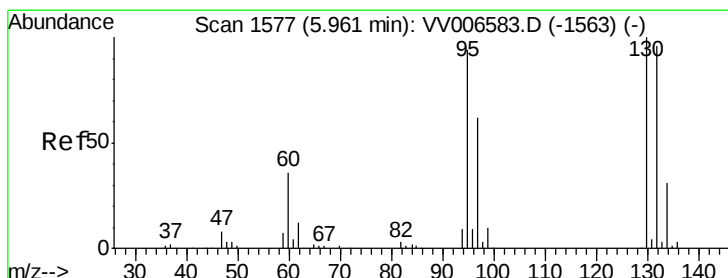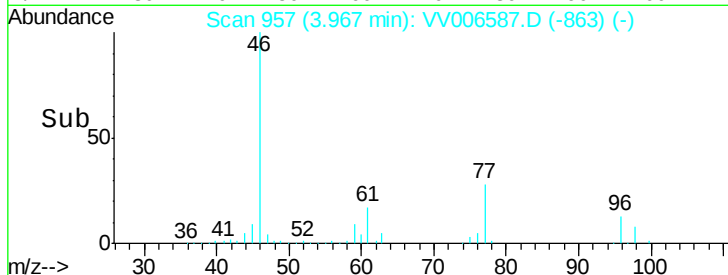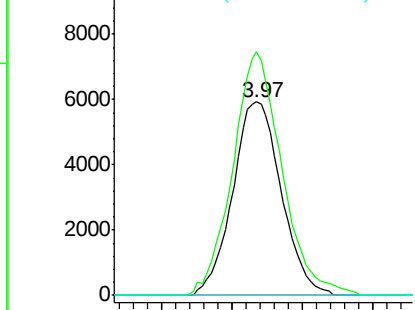



#34


Trichloroethene
 Concen: 1.747 ug/L
 RT: 5.96 min Scan# 1578
 Delta R.T. 0.00 min
 Lab File: VV006587.D
 Acq: 12 Jul 2018 15:50

Tgt Ion: 95 Resp: 41346
 Ion Ratio Lower Upper
 95 100
 97 66.0 44.3 82.3
 132 103.3 70.0 130.0
 130 107.2 72.7 134.9

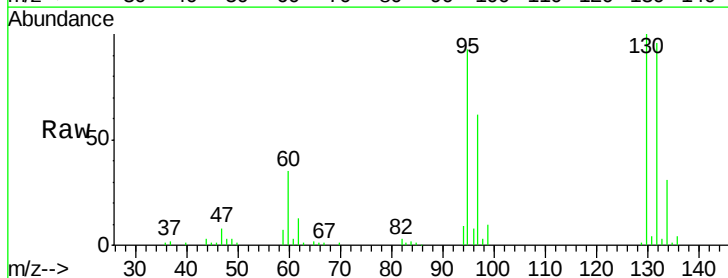

Abundance Ion 95.00 (94.70 to 95.70): VV0
 Ion 96.95 (96.65 to 97.65): VV0
 Ion 131.95 (131.65 to 132.65): VV0
 Ion 129.95 (129.65 to 130.65): VV0

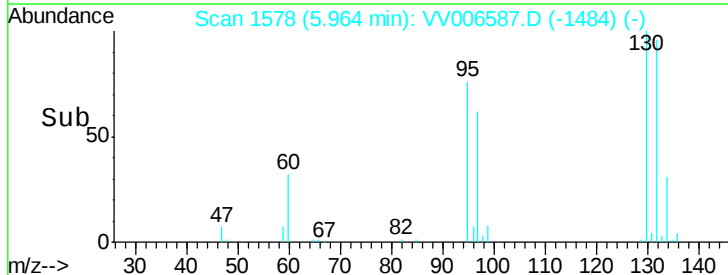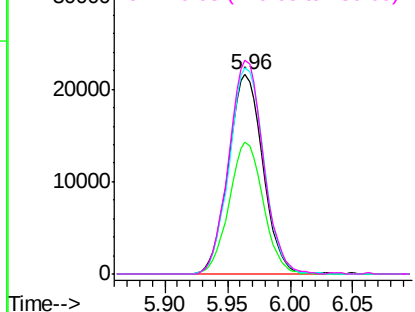


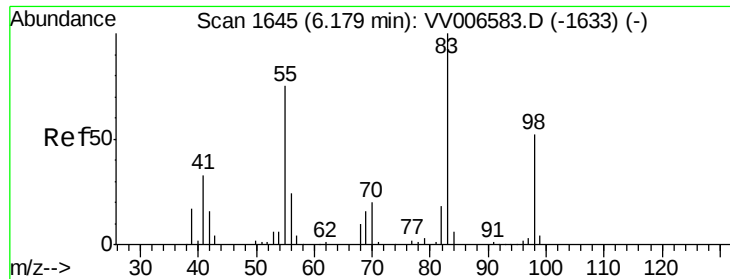




#35
Methylcyclohexane
Concen: 0.674 ug/L
RT: 6.12 min Scan# 1628
Delta R.T. -0.05 min
Lab File: VV006587.D
Acq: 12 Jul 2018 15:50

Instrument :
MSVOA_V
ClientSampleId :
C0AE9

Tgt Ion: 83 Resp: 25704
Ion Ratio Lower Upper
83 100
55 0.3 58.3 87.5#
98 16.9 39.3 58.9#

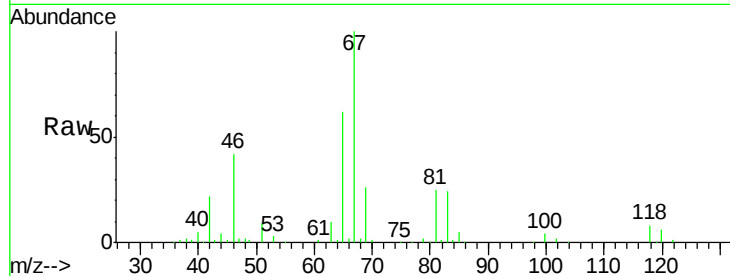


Abundance Ion 83.15 (82.85 to 83.85): VV0
Ion 55.10 (54.80 to 55.80): VV0
Ion 98.15 (97.85 to 98.85): VV0

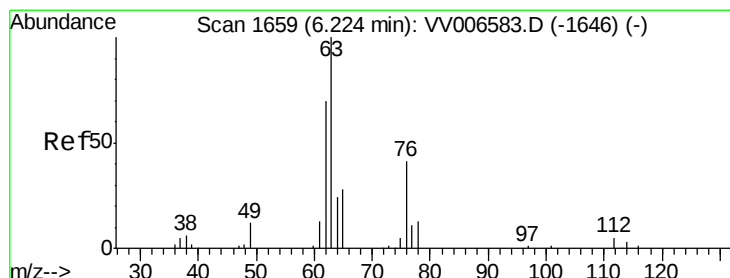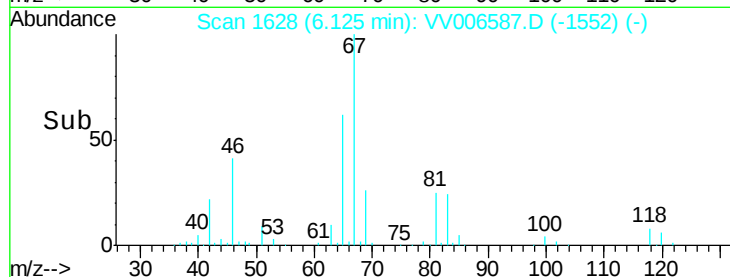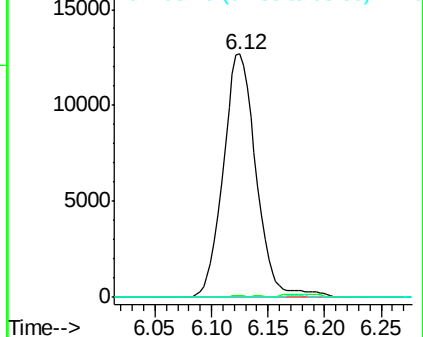

#37
1,2-Dichloropropane
Concen: 0.458 ug/L
RT: 6.12 min Scan# 1628
Delta R.T. -0.10 min
Lab File: VV006587.D
Acq: 12 Jul 2018 15:50

Tgt Ion: 63 Resp: 10341
Ion Ratio Lower Upper
63 100
112 0.0 3.8 5.6#

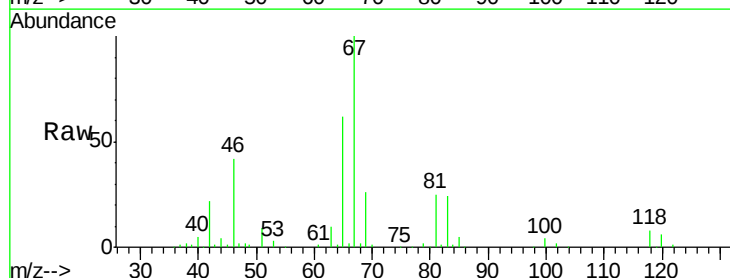

Abundance Ion 63.10 (62.80 to 63.80): VV0
Ion 112.10 (111.80 to 112.80): V

