


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV071218\
 Data File : VV006582.D
 Acq On : 12 Jul 2018 09:16
 Operator : SY/MD
 Sample : BFB64
 Misc : 25 mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB64

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR070718WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Mon Jul 16 08:05:56 2018

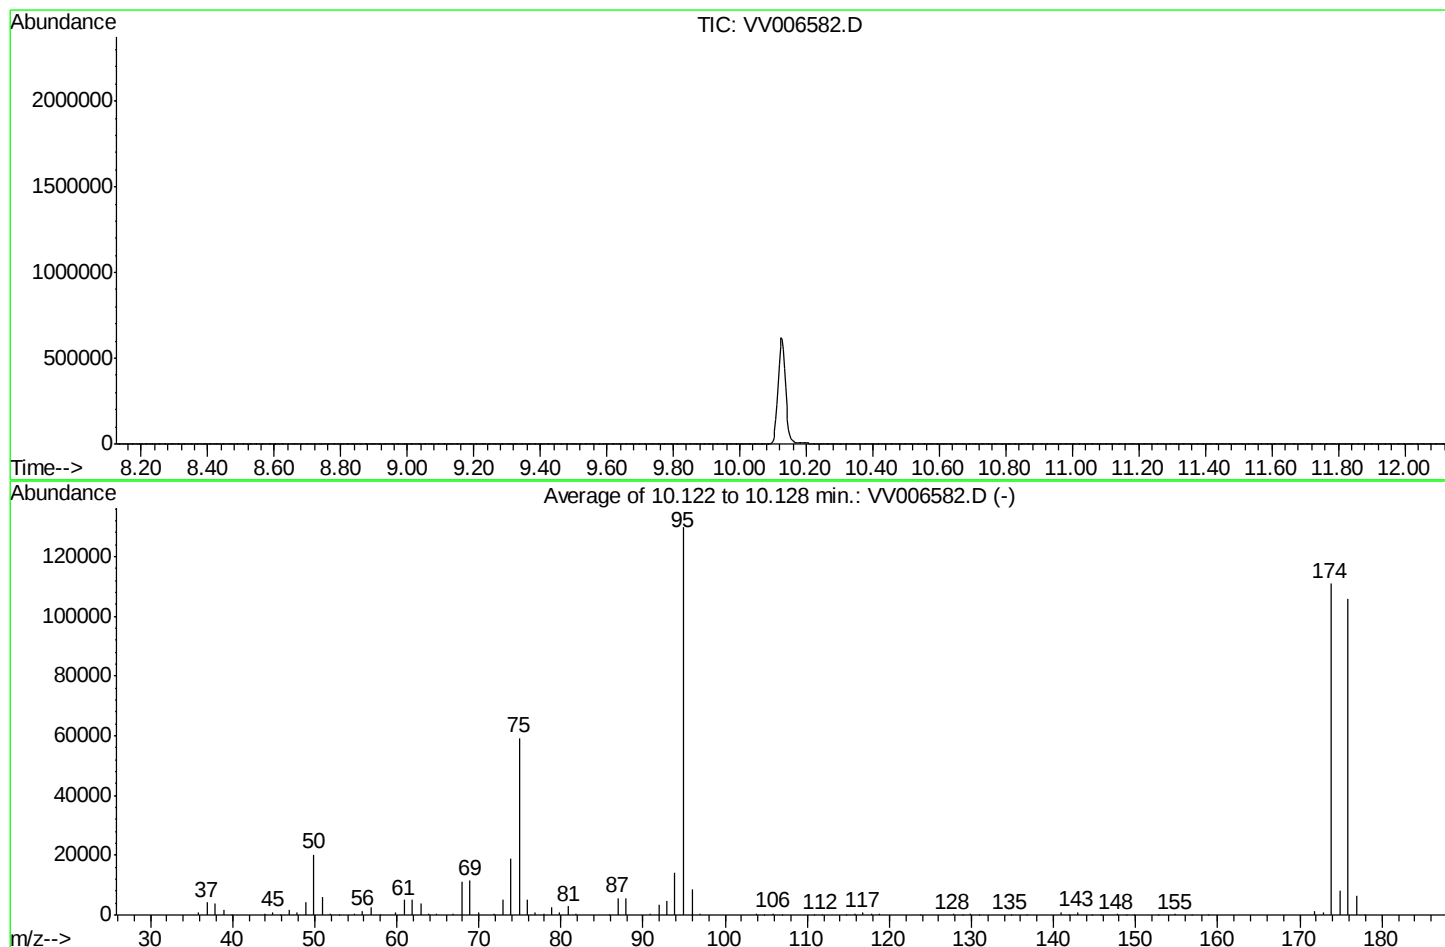

AutoFind: Scans 2871, 2872, 2873; Background Corrected with Scan 2858

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.7	20338	PASS
75	95	30	80	45.7	59336	PASS
95	95	100	100	100.0	129738	PASS
96	95	5	9	6.5	8478	PASS
173	174	0.00	2	0.8	841	PASS
174	95	50	120	85.5	110920	PASS
175	174	5	9	7.3	8078	PASS
176	174	95	101	95.3	105669	PASS
177	176	5	9	6.3	6637	PASS

m/z	Abundance
39.80	187.0
43.90	657.0

Instrument :
MSVOA_V
ClientSampleId :
BFB64

m/z	Abundance
35.90	824.0
36.90	3998.0
37.90	3845.0
38.90	1645.0
39.80	258.0
43.90	1187.0
44.90	843.0
47.00	1503.0
47.80	693.0
48.90	3944.0
49.90	19664.0
50.90	5973.0
51.90	281.0
52.90	112.0
54.90	207.0
55.80	1395.0
56.90	2753.0
57.90	139.0
59.90	838.0
60.90	4796.0
61.90	4666.0
62.90	3767.0
63.90	408.0
64.90	570.0
66.80	266.0
67.90	10587.0
68.90	11019.0
69.90	856.0
71.90	614.0
72.90	4924.0
73.90	17896.0
74.90	56832.0
75.90	5021.0
76.90	746.0
77.90	605.0
78.80	2472.0
79.80	763.0
80.90	2714.0
81.80	622.0
85.80	162.0
86.90	5300.0
87.90	5472.0
90.80	336.0
91.90	3215.0
92.90	4618.0
93.90	13386.0
94.90	123424.0
96.00	8244.0
97.00	252.0
103.80	386.0
104.70	149.0
105.90	464.0
106.90	123.0
115.80	390.0
116.80	647.0
117.90	355.0
118.80	614.0
127.70	353.0
128.80	177.0
129.80	385.0
130.90	169.0
134.80	234.0
136.70	124.0
140.80	884.0
141.80	114.0
142.90	996.0
144.70	131.0
145.80	184.0
147.80	245.0
148.80	104.0
152.70	105.0
154.80	289.0
156.80	217.0
158.90	140.0
171.80	1017.0
172.80	803.0
173.80	102136.0
174.90	7467.0
175.80	97592.0
176.90	6153.0
177.80	185.0

Instrument :
MSVOA_V
ClientSampleId :
BFB64

m/z	Abundance
35.90	868.0
36.90	4349.0
37.90	4144.0
38.90	1687.0
39.80	225.0
43.90	1292.0
44.90	902.0
46.90	1581.0
47.80	753.0
48.90	4348.0
49.90	21080.0
50.90	6332.0
51.90	300.0
52.90	110.0
54.80	247.0
55.90	1441.0
56.90	2860.0
57.90	138.0
59.80	936.0
60.90	5157.0
61.90	5118.0
62.90	3932.0
63.90	462.0
64.90	669.0
66.80	293.0
67.90	11504.0
68.90	11867.0
69.90	958.0
71.90	623.0
72.90	5209.0
73.90	19400.0
74.90	61280.0
75.90	5197.0
76.90	838.0
77.80	607.0
78.80	2661.0
79.80	945.0
80.90	2984.0
81.80	662.0
85.80	199.0
86.90	5806.0
87.90	5776.0
90.80	382.0
91.90	3490.0
92.90	5059.0
93.90	14560.0
94.90	134272.0
96.00	8743.0
97.00	288.0
103.80	439.0
104.70	161.0
105.90	507.0
106.90	129.0
111.70	102.0
114.70	114.0
115.80	412.0
116.80	732.0
117.80	410.0
118.80	622.0
123.80	102.0
127.70	405.0
128.90	194.0
129.80	407.0
130.90	174.0
134.80	233.0
136.80	158.0
140.80	944.0
141.80	116.0
142.90	1094.0
144.70	147.0
145.80	183.0
147.80	268.0
152.70	114.0
154.80	317.0
156.80	214.0
158.90	135.0
171.80	1152.0
172.80	876.0
173.80	114792.0
174.90	8397.0
175.80	109184.0
176.90	6812.0
177.90	199.0

Instrument :
MSVOA_V
ClientSampleId :
BFB64

m/z	Abundance
35.90	755.0
36.90	4164.0
37.90	3960.0
38.90	1582.0
39.80	173.0
43.90	1358.0
44.90	857.0
45.80	104.0
46.90	1484.0
47.90	713.0
48.90	4188.0
49.90	20272.0
50.90	6084.0
51.90	289.0
54.80	262.0
55.90	1386.0
56.90	2668.0
57.90	124.0
59.80	973.0
60.90	4989.0
61.90	5068.0
62.90	3874.0
63.90	487.0
64.90	704.0
66.80	300.0
67.90	11301.0
68.90	11529.0
69.90	988.0
71.90	592.0
72.90	4993.0
73.90	19152.0
74.90	59896.0
75.90	4977.0
76.90	779.0
77.80	510.0
78.80	2582.0
79.80	986.0
80.90	2914.0
81.80	666.0
85.80	180.0
86.90	5754.0
87.90	5515.0
90.80	368.0
91.90	3460.0
92.90	5063.0
93.90	14396.0
94.90	131520.0
96.00	8448.0
97.00	275.0
103.90	462.0
104.80	142.0
105.80	461.0
106.90	119.0
110.80	106.0
111.80	105.0
114.80	116.0
115.80	414.0
116.80	751.0
117.80	433.0
118.80	584.0
123.80	111.0
127.80	422.0
128.90	179.0
129.80	382.0
130.90	146.0
134.80	195.0
136.80	168.0
140.90	938.0
141.80	112.0
142.90	1097.0
144.70	145.0
145.80	174.0
147.70	270.0
149.80	116.0
152.70	112.0
154.80	324.0
156.90	205.0
158.90	106.0
171.80	1160.0
172.80	844.0
173.80	115832.0
174.90	8372.0
175.80	110232.0
176.90	6947.0
177.90	169.0

Instrument :
MSVOA_V
ClientSampleId :
BFB64