

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV071219\
 Data File : VV011874.D
 Acq On : 12 Jul 2019 18:42
 Operator : SY/MD
 Sample : K3785-04
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0XL2

Quant Time: Jul 13 04:54:06 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR071219WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Jul 13 04:20:11 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	152880	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	148617	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	66053	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	60178	5.24	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	104.80%
7) Chloroethane-d5	1.58	69	48503	5.34	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	106.80%
11) 1,1-Dichloroethene-d2	2.13	63	72921	4.03	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	80.60%
20) 2-Butanone-d5	3.95	46	159536	66.17	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	132.34%#
24) Chloroform-d	4.40	84	110985	5.33	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.60%
26) 1,2-Dichloroethane-d4	5.08	65	63938	6.16	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	123.20%
32) Benzene-d6	5.10	84	225827	5.52	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	110.40%
36) 1,2-Dichloropropane-d6	6.12	67	69614	5.52	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	110.40%
41) Toluene-d8	7.36	98	191998	5.13	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.60%
43) trans-1,3-Dichloropropene-	7.66	79	22927	4.97	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	99.40%
46) 2-Hexanone-d5	8.14	63	108560	59.81	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	119.62%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	38336	4.91	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.20%
64) 1,2-Dichlorobenzene-d4	11.67	152	70438	5.77	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	115.40%


Target Compounds					Ovalue
13) Acetone	2.20	43	2953	1.997 ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV071219\
Data File : VV011874.D
Acq On : 12 Jul 2019 18:42
Operator : SY/MD
Sample : K3785-04
Misc : 25ML/MSVOA V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0XL2

Quant Time: Jul 13 04:54:06 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR071219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Jul 13 04:20:11 2019
Response via : Initial Calibration

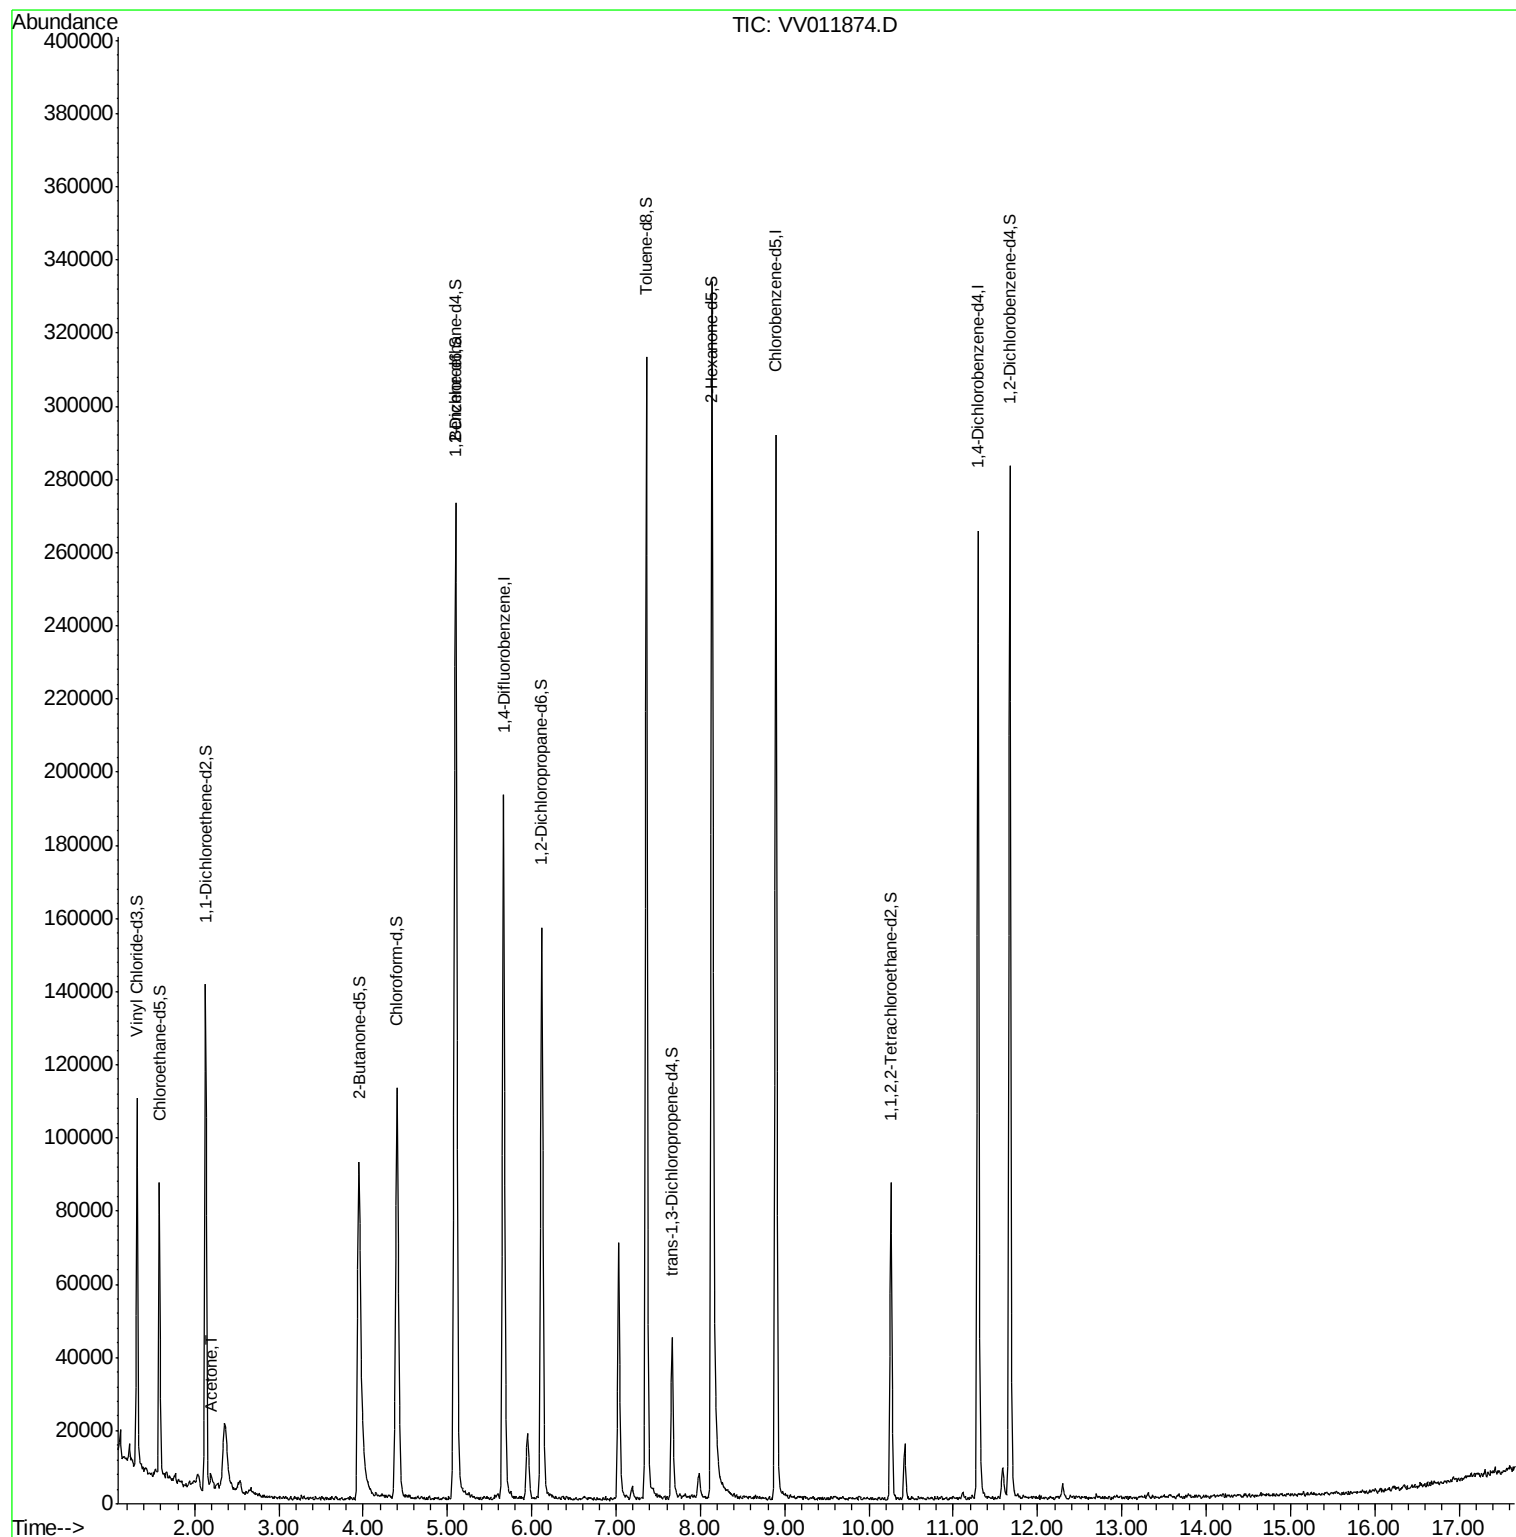

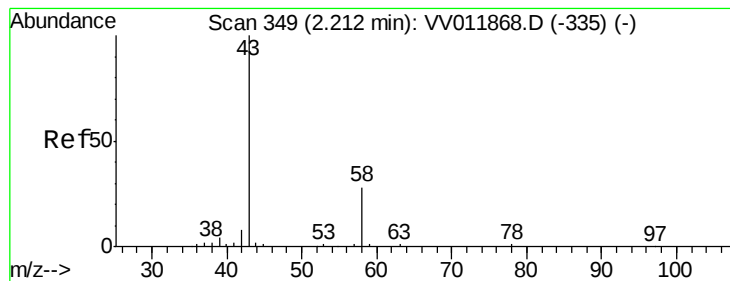

#13

Acetone

Concen: 1.997 ug/L

RT: 2.20 min Scan# 345

Delta R.T. -0.01 min

Lab File: VV011874.D

Acq: 12 Jul 2019 18:42

Instrument :
MSVOA_V
ClientSampleId :
C0XL2

Tot Ion: 43 Resp: 2953

Ion Ratio Lower Upper

43 100

58 29.2 0.0 58.4

