

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV071219\
 Data File : VV011875.D
 Acq On : 12 Jul 2019 19:07
 Operator : SY/MD
 Sample : K3785-06
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0XL4

Quant Time: Jul 13 04:59:45 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR071219WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Jul 13 04:20:11 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	161187	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	158256	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	70297	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	59154	4.88	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	97.60%
7) Chloroethane-d5	1.58	69	49298	5.15	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	103.00%
11) 1,1-Dichloroethene-d2	2.13	63	62809	3.29	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	65.80%
20) 2-Butanone-d5	3.96	46	161443	63.51	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	127.02%
24) Chloroform-d	4.40	84	110573	5.03	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.60%
26) 1,2-Dichloroethane-d4	5.08	65	61645	5.63	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	112.60%
32) Benzene-d6	5.10	84	221137	5.07	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.40%
36) 1,2-Dichloropropane-d6	6.12	67	69290	5.16	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	103.20%
41) Toluene-d8	7.36	98	193193	4.85	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.00%
43) trans-1,3-Dichloropropene-	7.67	79	22629	4.60	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	92.00%
46) 2-Hexanone-d5	8.14	63	107576	55.66	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	111.32%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	37705	4.53	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	90.60%
64) 1,2-Dichlorobenzene-d4	11.67	152	71091	5.47	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	109.40%


Target Compounds					Ovalue
3) Chloromethane	1.25	50	5561	0.356 ug/L	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV071219\
Data File : VV011875.D
Acq On : 12 Jul 2019 19:07
Operator : SY/MD
Sample : K3785-06
Misc : 25ML/MSVOA V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0XL4

Quant Time: Jul 13 04:59:45 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR071219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Jul 13 04:20:11 2019
Response via : Initial Calibration

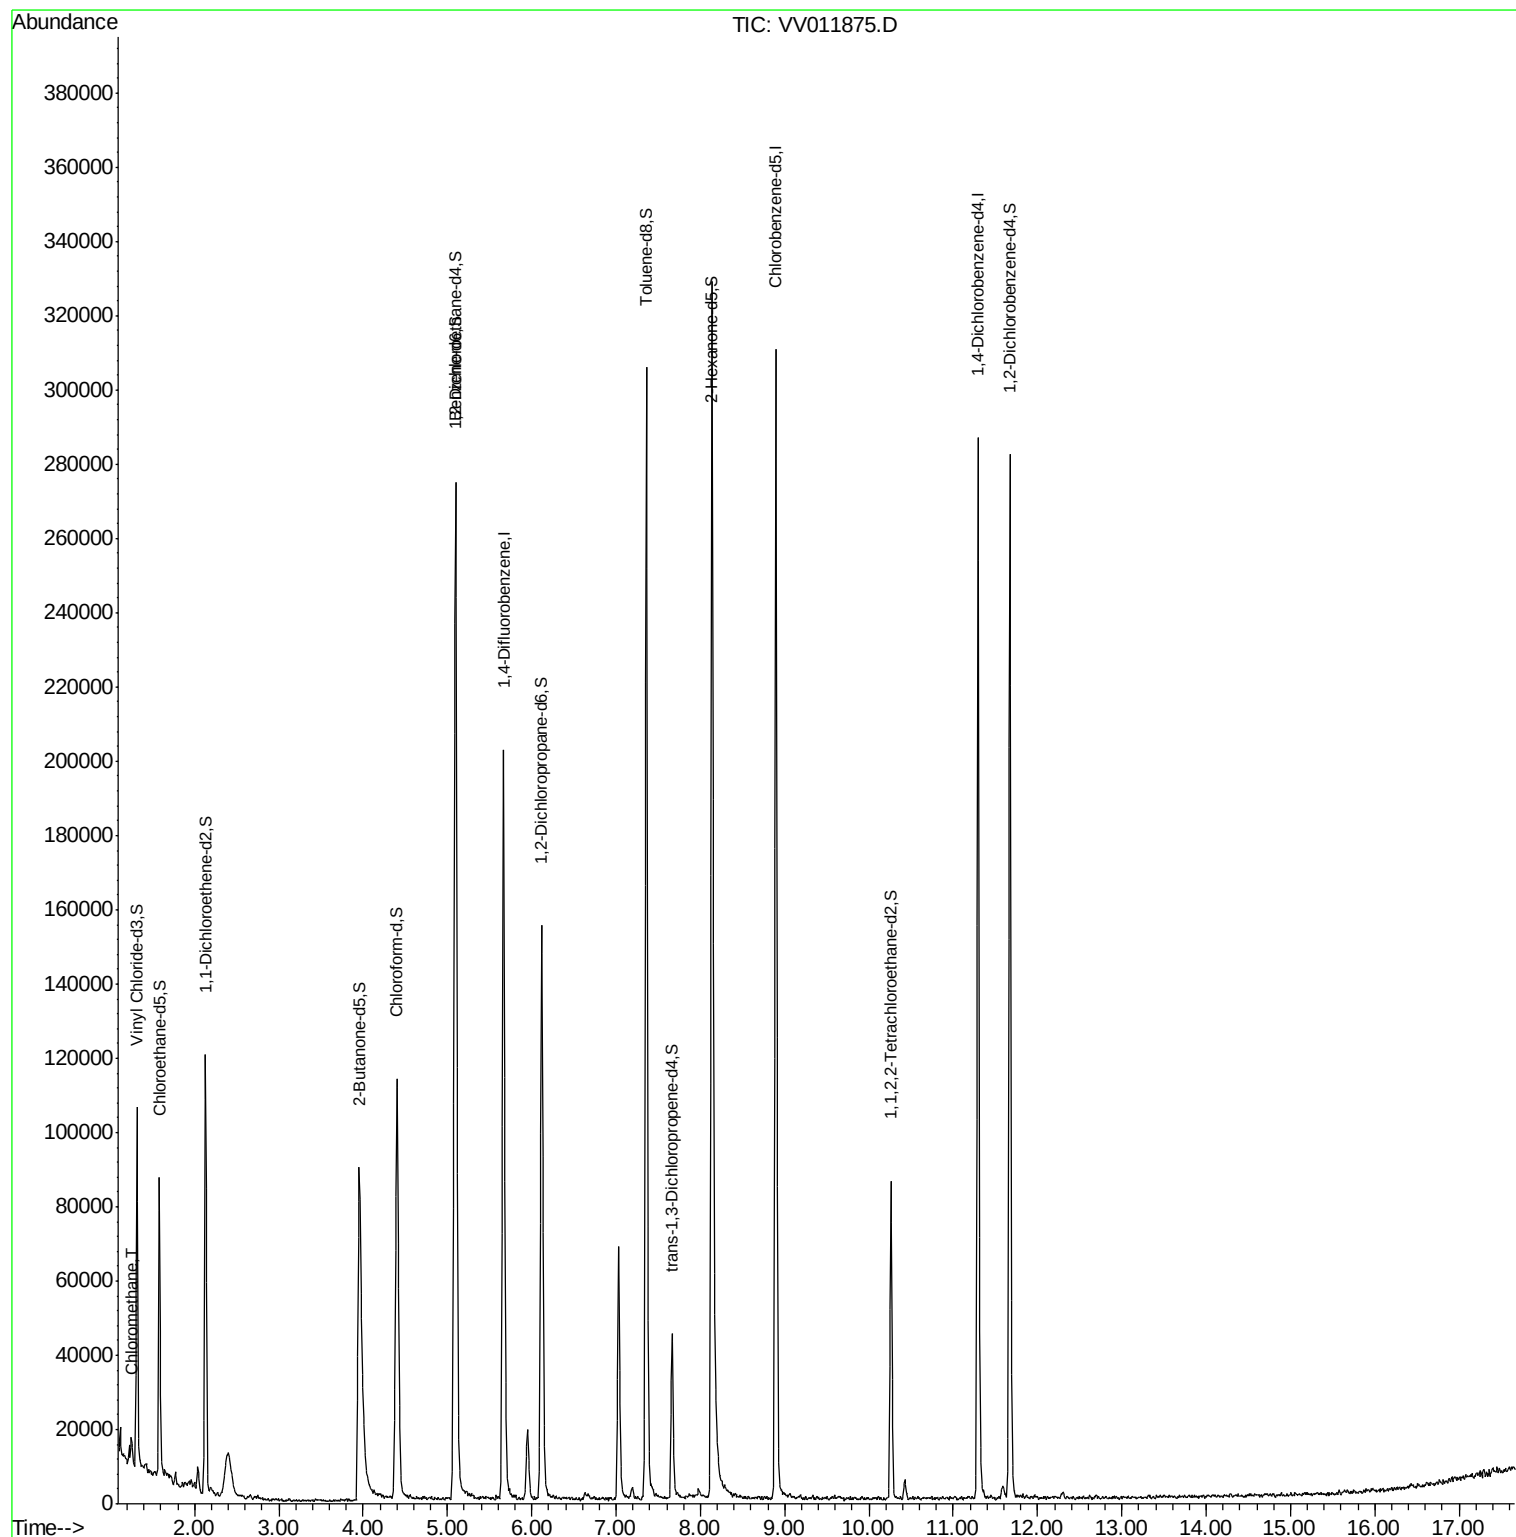

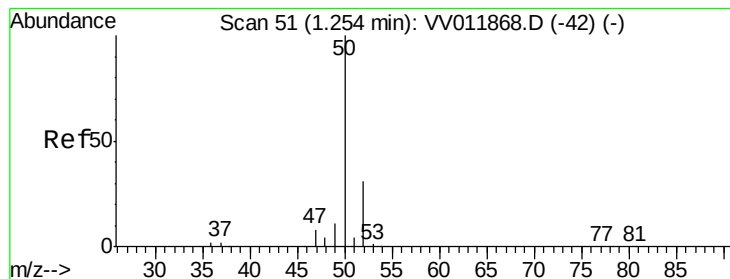

#3

Chloromethane

Concen: 0.356 ug/L

RT: 1.25 min Scan# 50

Delta R.T. -0.00 min

Lab File: VV011875.D

Acq: 12 Jul 2019 19:07

Instrument :
MSVOA_V
ClientSampleId :
C0XL4

Tot Ion: 50 Resp: 5561

Ion Ratio Lower Upper

50 100

52 40.7 22.0 41.0

