


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV071219\
Data File : VV011861.D
Acq On : 12 Jul 2019 09:53
Operator : SY/MD
Sample : BFB31
Misc : 25ML/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB31

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR071219WMA.M
Title : TRACE VOA SOM01.0
Last Update : Tue Jul 16 03:56:26 2019

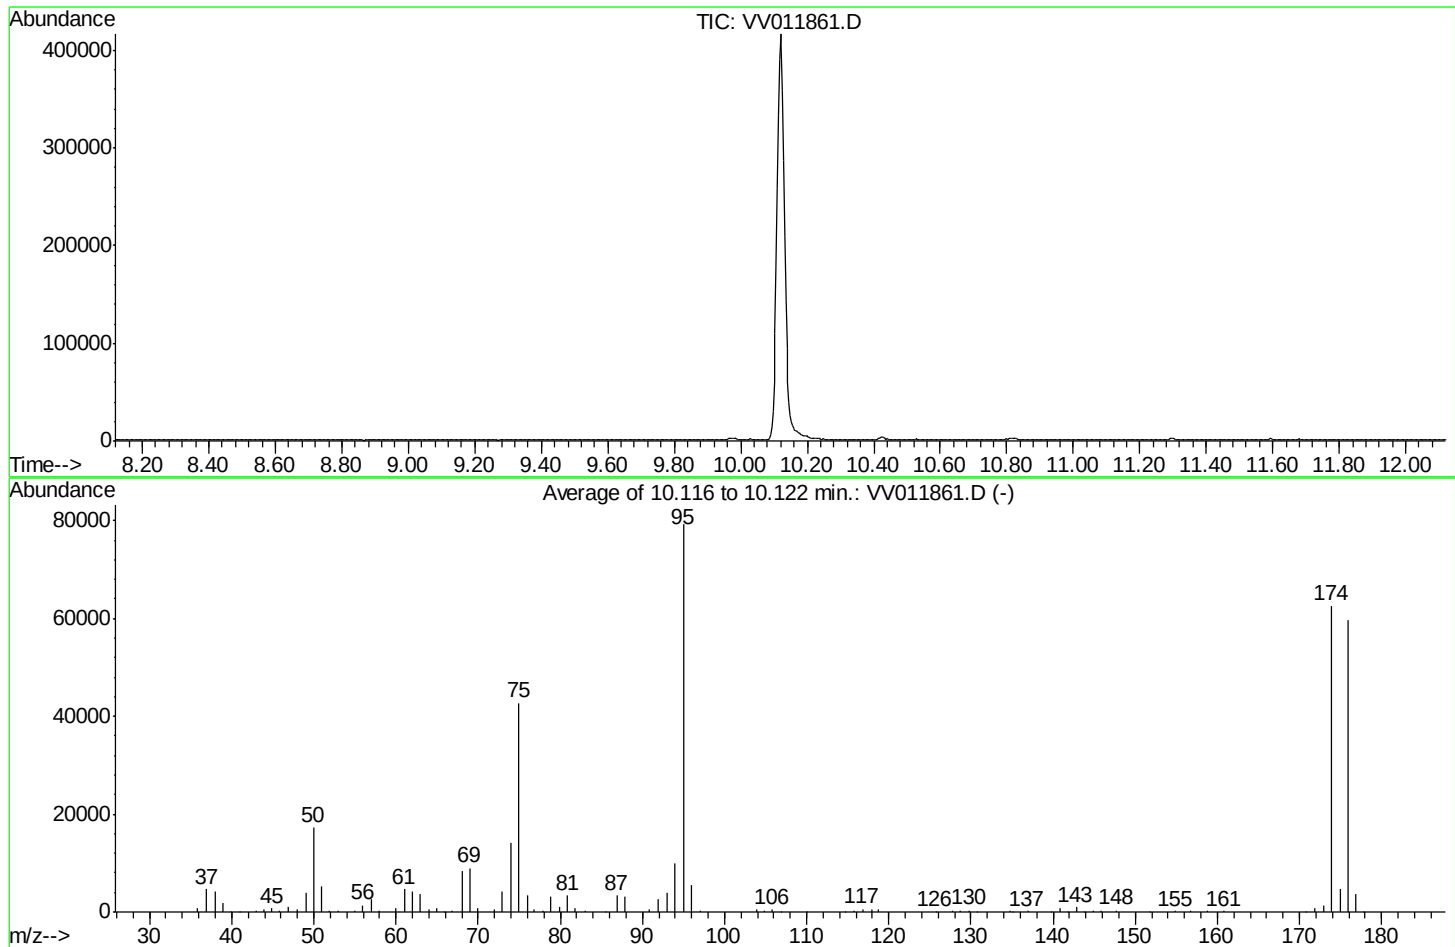

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2793

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.8	17250	PASS
75	95	30	80	53.8	42658	PASS
95	95	100	100	100.0	79234	PASS
96	95	5	9	6.9	5440	PASS
173	174	0.00	2	1.9	1193	PASS
174	95	50	120	79.0	62610	PASS
175	174	5	9	7.6	4777	PASS
176	174	95	101	95.5	59786	PASS
177	176	5	9	6.4	3801	PASS

Scan 2793 (10.071 min): VV011861.D
BFB31

m/z	Abundance
35.70	113.0
38.50	114.0
38.90	110.0
40.00	442.0
43.90	494.0
46.60	103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB31

m/z	Abundance
35.90	853.0
37.00	4604.0
38.00	4164.0
39.00	1866.0
39.90	517.0
41.10	103.0
43.00	147.0
43.90	892.0
44.90	785.0
45.90	167.0
46.90	1275.0
47.90	630.0
49.00	3750.0
50.00	16968.0
51.00	5207.0
51.90	255.0
52.90	185.0
55.00	304.0
55.90	1468.0
57.00	2470.0
58.00	142.0
59.90	702.0
61.00	4438.0
62.00	4277.0
63.00	3593.0
63.90	679.0
64.90	681.0
66.00	132.0
66.90	293.0
68.00	8177.0
69.00	8627.0
70.00	676.0
71.90	557.0
72.90	4051.0
74.00	14097.0
75.00	41464.0
76.00	3431.0
76.90	500.0
77.90	256.0
78.80	3050.0
79.90	956.0
80.90	3238.0
81.90	670.0
83.00	151.0
85.60	134.0
86.90	3317.0
87.90	3169.0
90.80	402.0
92.00	2474.0
93.00	3852.0
94.00	9755.0
95.00	75968.0
96.00	5457.0
97.00	186.0
103.90	428.0
104.90	149.0
105.80	442.0
106.80	111.0
114.70	128.0
115.70	390.0
116.80	616.0
117.90	418.0
118.70	450.0
127.80	369.0
128.80	175.0
129.80	366.0
130.70	118.0
134.70	157.0
136.90	166.0
140.80	757.0
141.90	136.0
142.80	997.0
143.80	107.0
144.90	372.0
145.80	136.0
147.80	275.0
151.70	106.0
155.00	247.0
156.80	221.0
158.70	148.0
160.80	183.0
170.80	118.0
171.90	892.0
173.00	1084.0
173.90	59184.0
174.90	4414.0
175.90	56544.0
176.90	3779.0
177.80	131.0

Instrument :
MSVOA_V
ClientSampleId :
BFB31

m/z	Abundance
35.90	927.0
36.90	4786.0
38.00	4306.0
39.00	2046.0
39.90	516.0
41.10	106.0
43.00	148.0
43.90	936.0
44.90	750.0
45.90	185.0
46.90	1137.0
47.90	581.0
49.00	4003.0
50.00	17736.0
51.00	5244.0
51.90	262.0
53.00	178.0
55.00	345.0
55.90	1495.0
57.00	2623.0
58.00	178.0
60.00	768.0
61.00	4748.0
62.00	4313.0
63.00	3656.0
63.90	617.0
64.90	775.0
65.90	113.0
66.90	268.0
68.00	8752.0
69.00	9157.0
70.00	689.0
71.90	516.0
73.00	4188.0
74.00	14657.0
75.00	43896.0
76.00	3631.0
76.90	506.0
77.90	312.0
78.80	3189.0
79.90	1053.0
80.90	3435.0
81.80	731.0
83.00	158.0
85.60	141.0
86.90	3447.0
87.90	3285.0
90.90	422.0
91.90	2777.0
93.00	4049.0
94.00	10256.0
95.00	81824.0
96.00	5614.0
97.00	197.0
103.80	408.0
104.90	165.0
105.80	457.0
109.90	113.0
114.70	130.0
115.80	386.0
116.80	655.0
117.90	450.0
118.80	527.0
127.80	371.0
128.70	161.0
129.80	381.0
130.80	132.0
134.80	145.0
136.90	189.0
140.80	871.0
141.80	125.0
142.80	1052.0
143.70	107.0
144.90	399.0
145.80	157.0
147.70	292.0
154.90	259.0
156.80	178.0
158.70	191.0
160.80	211.0
170.80	135.0
171.90	954.0
173.00	1250.0
173.90	64584.0
174.90	4908.0
175.90	61920.0
176.90	3908.0
177.80	134.0

Instrument :
MSVOA_V
ClientSampleId :
BFB31

m/z	Abundance
35.90	921.0
36.90	4454.0
38.00	4044.0
39.00	1913.0
39.80	465.0
40.90	135.0
43.00	129.0
43.90	959.0
44.90	680.0
45.80	211.0
47.00	962.0
47.90	530.0
49.00	3843.0
50.00	17048.0
51.00	5053.0
51.90	258.0
53.00	187.0
55.00	333.0
56.00	1293.0
57.00	2462.0
57.90	192.0
60.00	768.0
61.00	4582.0
62.00	4004.0
63.00	3530.0
64.00	503.0
64.90	790.0
66.80	240.0
68.00	8484.0
69.00	8996.0
70.00	650.0
72.00	458.0
73.00	3995.0
74.00	14005.0
75.00	42616.0
76.00	3551.0
76.80	465.0
77.90	413.0
78.90	3147.0
79.90	980.0
80.90	3250.0
81.80	791.0
83.00	137.0
85.60	126.0
86.90	3376.0
87.90	3027.0
90.90	402.0
91.90	2642.0
93.00	3936.0
94.00	10049.0
95.00	79912.0
96.00	5249.0
97.00	220.0
103.80	419.0
104.90	164.0
105.80	388.0
110.00	130.0
114.70	120.0
115.80	388.0
116.80	671.0
117.90	414.0
118.80	551.0
125.70	108.0
127.70	354.0
128.80	167.0
129.80	352.0
130.80	156.0
134.60	118.0
135.10	102.0
136.90	172.0
139.80	102.0
140.80	912.0
141.70	128.0
142.90	1055.0
143.70	111.0
144.80	351.0
145.80	201.0
147.70	240.0
154.80	256.0
156.80	126.0
158.70	185.0
160.80	192.0
170.80	131.0
171.90	905.0
173.00	1245.0
173.90	64064.0
174.90	5010.0
175.90	60896.0
176.90	3717.0
177.70	151.0

Instrument :
MSVOA_V
ClientSampleId :
BFB31