

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071221\
 Data File : VV021620.D
 Acq On : 12 Jul 2021 12:49
 Operator : SY/MD
 Sample : M2959-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7H4

Quant Time: Jul 13 01:16:07 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jul 13 01:14:23 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	405647	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	376501	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	186026	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	171576	66.852	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	133.700%	
7) Chloroethane-d5	1.561	69	129331	61.656	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	123.320%	
11) 1,1-Dichloroethene-d2	2.105	63	218256	46.479	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	92.960%	
21) 2-Butanone-d5	3.870	46	262474	119.745	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	119.750%	
24) Chloroform-d	4.349	84	314400	58.566	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	117.140%	
26) 1,2-Dichloroethane-d4	5.034	65	196949	62.262	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	124.520%	
32) Benzene-d6	5.050	84	663373	62.753	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	125.500%#	
36) 1,2-Dichloropropane-d6	6.069	67	209889	62.950	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	125.900%#	
41) Toluene-d8	7.317	98	612532	62.653	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	125.300%#	
43) trans-1,3-Dichloroprop...	7.622	79	101896	61.436	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	122.880%	
47) 2-Hexanone-d5	8.088	63	176838	114.340	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	114.340%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	273762	60.941	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	121.880%#	
66) 1,2-Dichlorobenzene-d4	11.625	152	230689	62.202	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	124.400%#	
Target Compounds						
13) Acetone	2.159	43	21049	11.616	ug/L	Qvalue # 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071221\
Data File : VV021620.D
Acq On : 12 Jul 2021 12:49
Operator : SY/MD
Sample : M2959-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7H4

Quant Time: Jul 13 01:16:07 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jul 13 01:14:23 2021
Response via : Initial Calibration

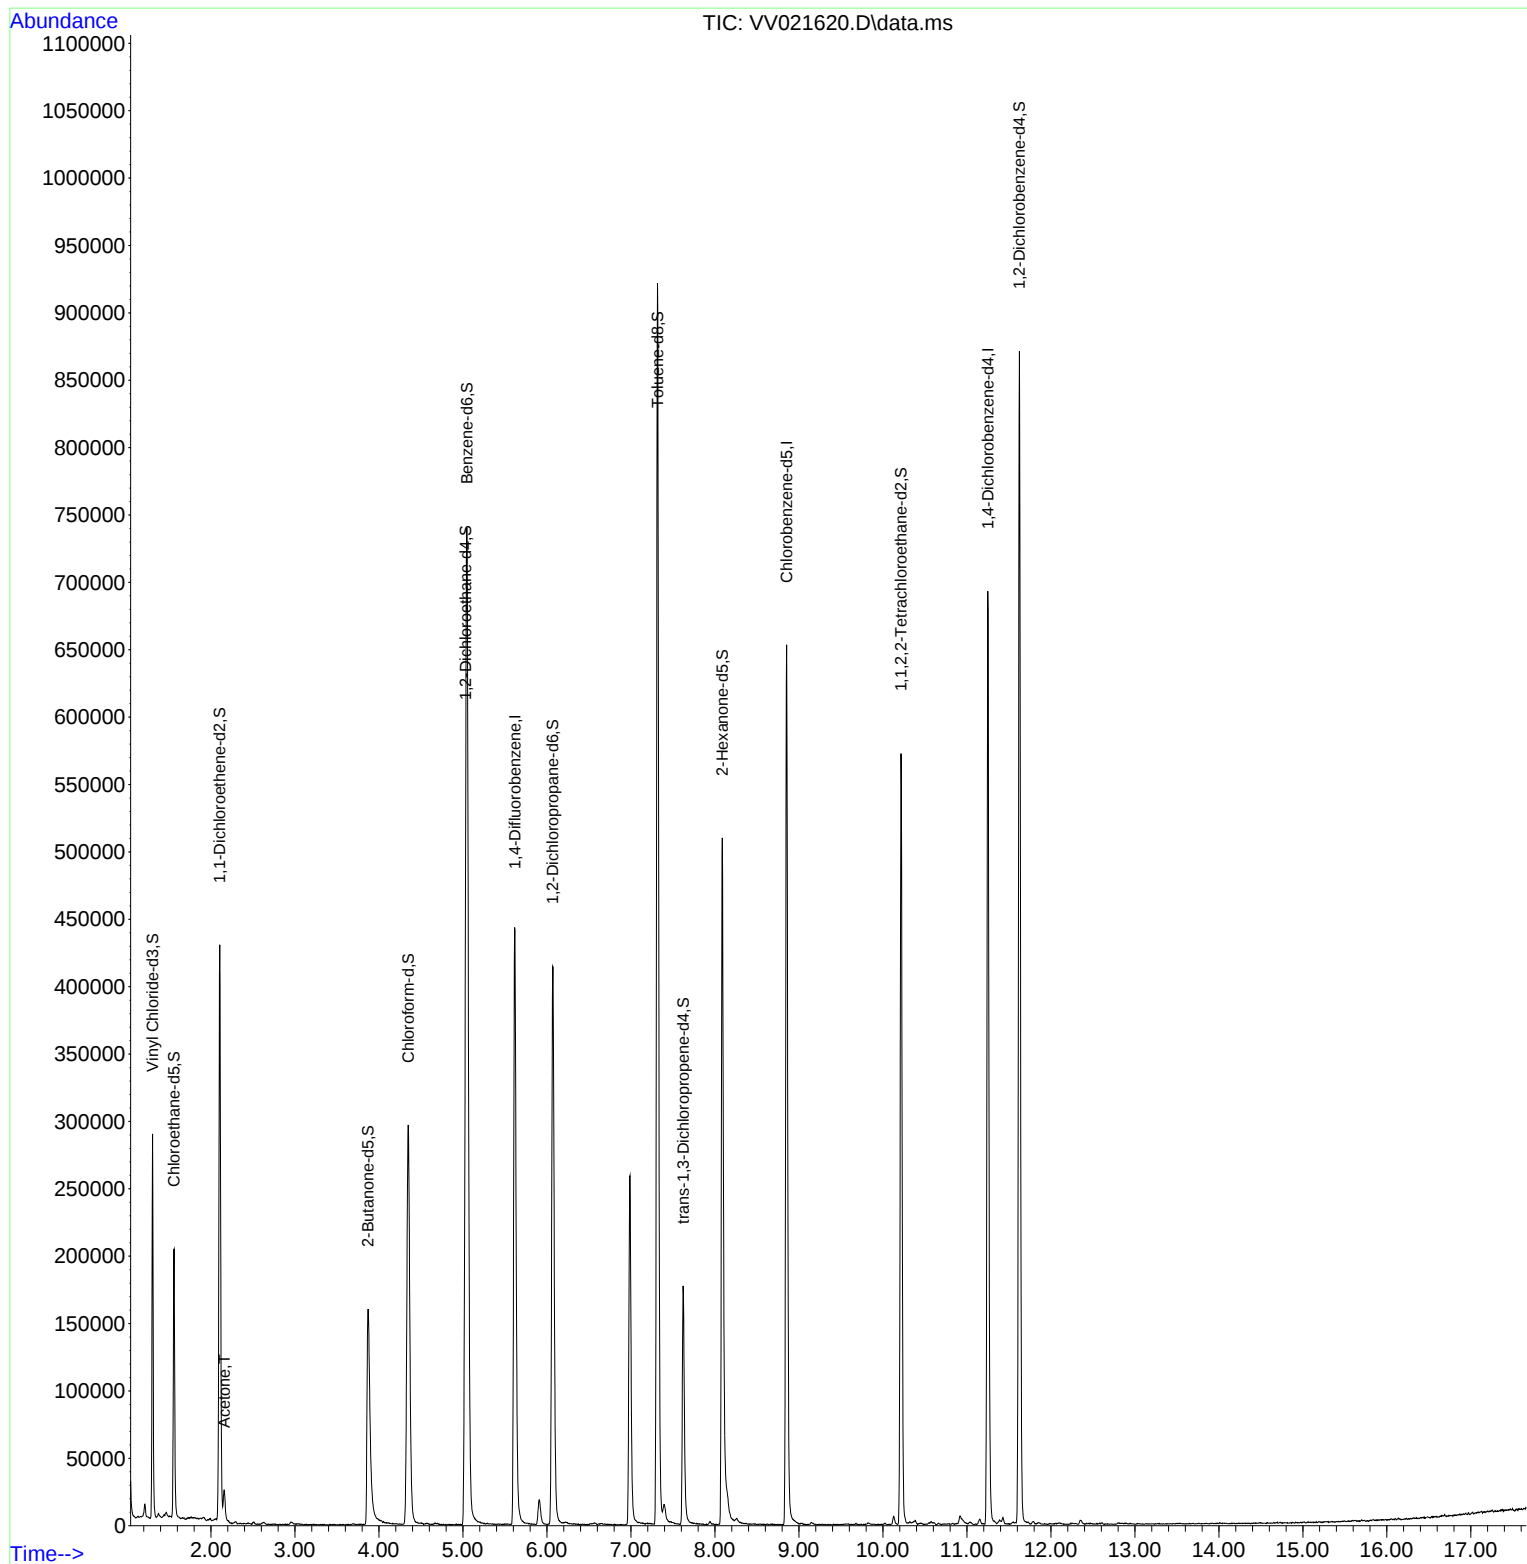

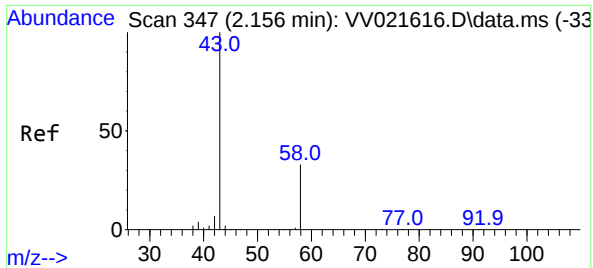

#13
 Acetone
 Concen: 11.616 ug/L
 RT: 2.159 min Scan# 348
 Delta R.T. 0.003 min
 Lab File: VV021620.D
 Acq: 12 Jul 2021 12:49

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7H4

Tgt Ion: 43 Resp: 21049
 Ion Ratio Lower Upper
 43 100
 58 35.1 0.0 0.0#

