

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071221\
 Data File : VV021622.D
 Acq On : 12 Jul 2021 13:37
 Operator : SY/MD
 Sample : M2978-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7H5

Quant Time: Jul 13 01:16:33 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jul 13 01:14:23 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	490808	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	457677	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	223665	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	157166	50.612	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	101.220%	
7) Chloroethane-d5	1.561	69	119094	46.924	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	93.840%	
11) 1,1-Dichloroethene-d2	2.105	63	202472	35.636	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	71.280%	
21) 2-Butanone-d5	3.873	46	234965	88.595	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	88.600%	
24) Chloroform-d	4.349	84	287002	44.186	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	88.380%	
26) 1,2-Dichloroethane-d4	5.034	65	182180	47.600	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	95.200%	
32) Benzene-d6	5.050	84	612217	47.642	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	95.280%	
36) 1,2-Dichloropropane-d6	6.072	67	191547	47.260	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	94.520%	
41) Toluene-d8	7.317	98	564261	47.479	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	94.960%	
43) trans-1,3-Dichloroprop...	7.622	79	94947	47.092	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	94.180%	
47) 2-Hexanone-d5	8.088	63	160625	85.436	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	85.440%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	250413	45.857	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	91.720%	
66) 1,2-Dichlorobenzene-d4	11.625	152	212807	47.724	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	95.440%	
Target Compounds					Qvalue	
13) Acetone	2.159	43	19429	8.861	ug/L	# 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071221\
Data File : VV021622.D
Acq On : 12 Jul 2021 13:37
Operator : SY/MD
Sample : M2978-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7H5

Quant Time: Jul 13 01:16:33 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jul 13 01:14:23 2021
Response via : Initial Calibration

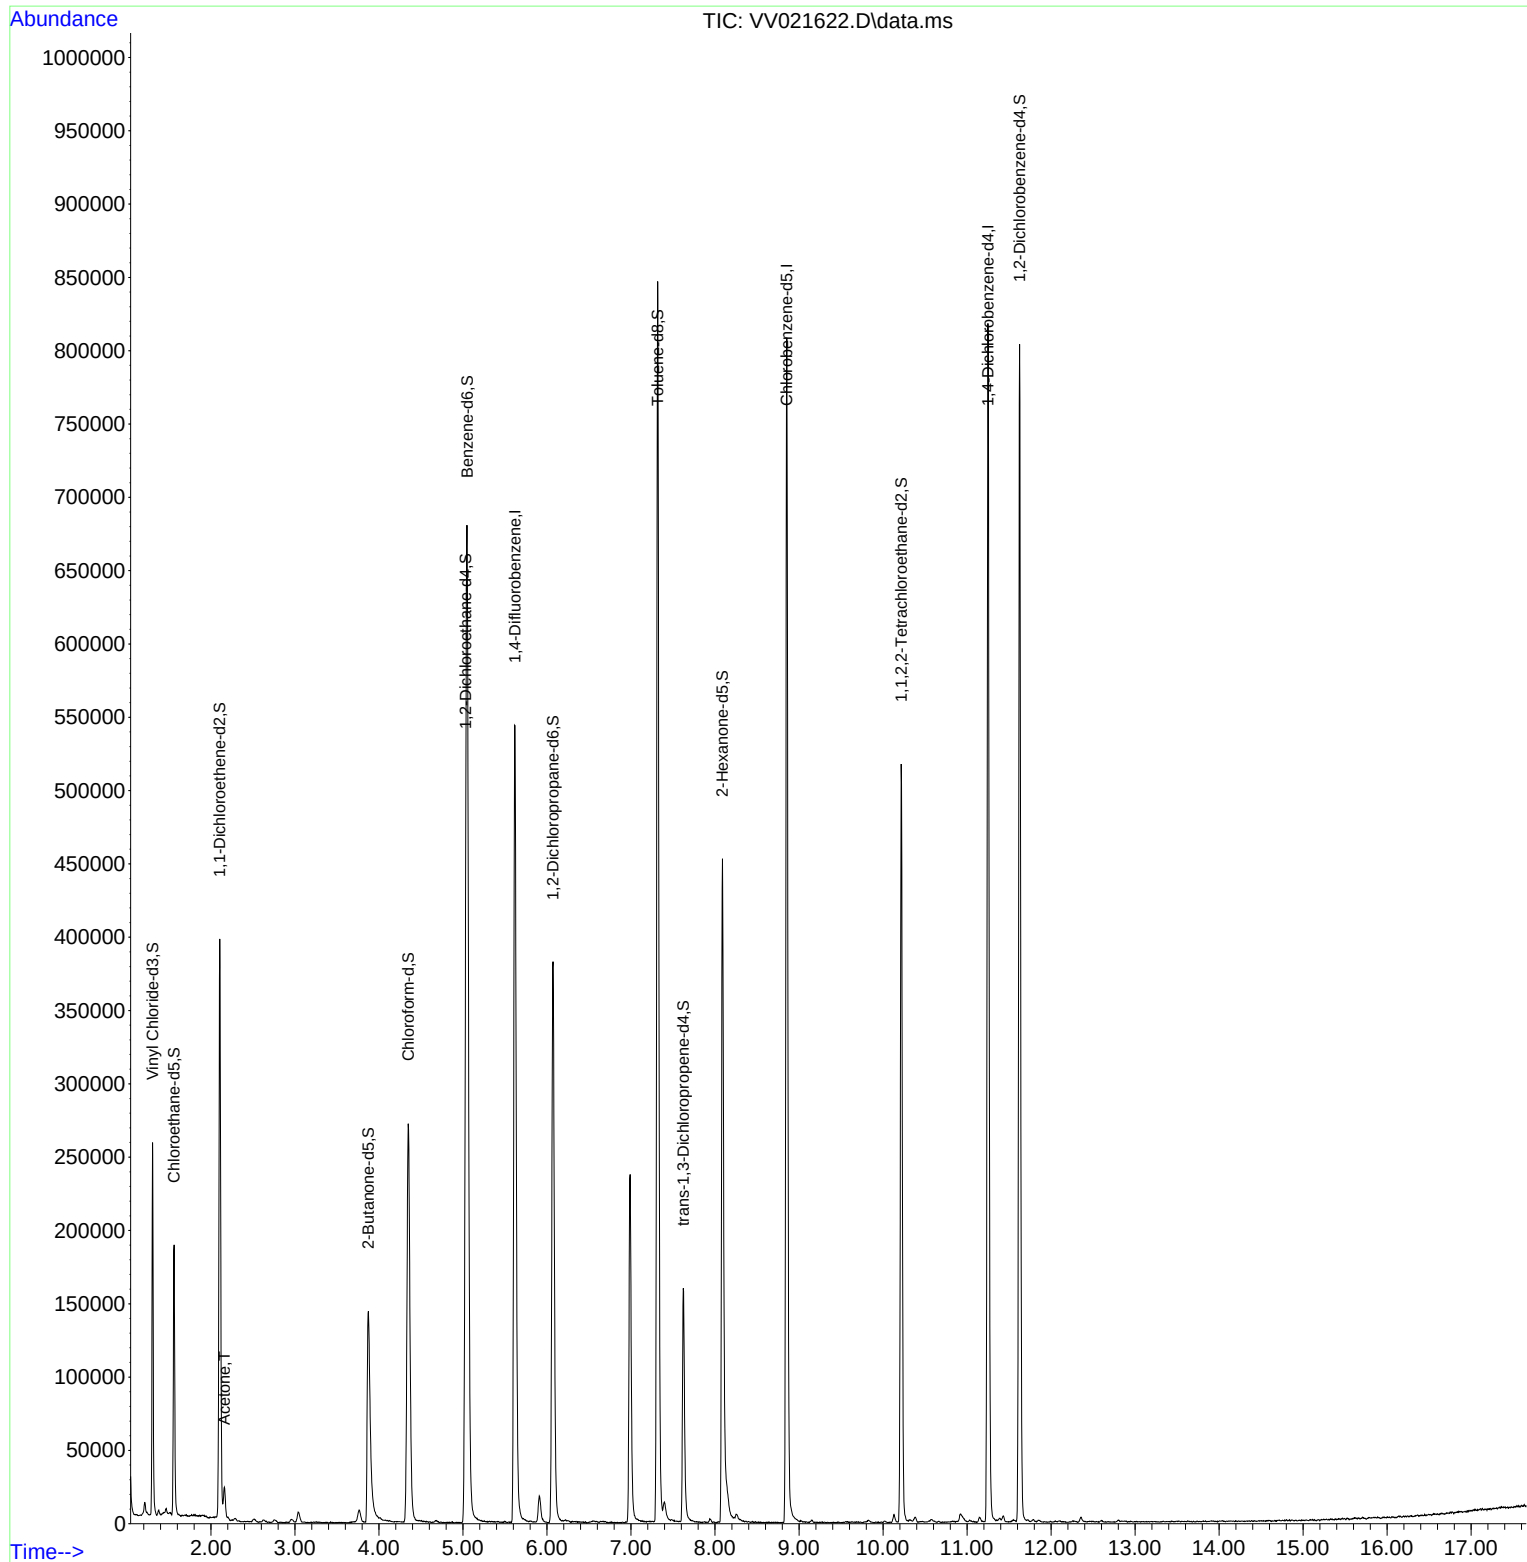

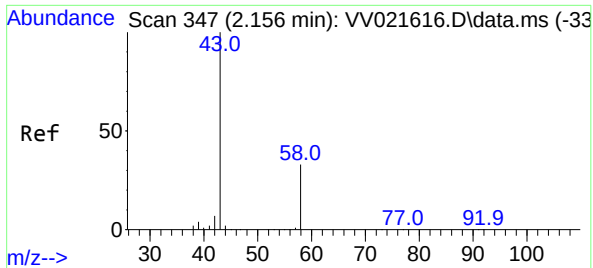

#13

Acetone

Concen: 8.861 ug/L


RT: 2.159 min Scan# 348

Delta R.T. 0.003 min

Lab File: VV021622.D

Acq: 12 Jul 2021 13:37

Instrument :
MSVOA_V
ClientSampleId :
BG7H5

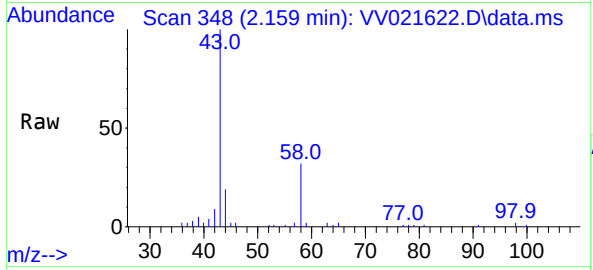

Tgt Ion: 43 Resp: 19429

Ion	Ratio	Lower	Upper
43	100		
58	34.0	0.0	0.0#

