

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071221\
 Data File : VV021618.D
 Acq On : 12 Jul 2021 11:48
 Operator : SY/MD
 Sample : VV0712WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK212

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
 Title : VOC Analysis

Signal : TIC: VV021618.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	102	rVB	263126	270236	14.85%	1.940%
2	1.558	154	161	180	rVB	189214	223205	12.27%	1.602%
3	2.105	321	331	348	rVB	409935	596453	32.78%	4.281%
4	2.506	449	456	470	rVB2	9490	15319	0.84%	0.110%
5	2.619	487	491	492	rBV2	527	383	0.02%	0.003%
6	2.699	512	516	519	rBV2	649	479	0.03%	0.003%
7	2.741	527	529	530	rBV	279	127	0.01%	0.001%
8	2.886	572	574	577	rVB3	449	262	0.01%	0.002%
9	2.902	577	579	580	rBV	377	205	0.01%	0.001%
10	2.934	585	589	593	rVB2	479	298	0.02%	0.002%
11	3.014	612	614	616	rBV2	246	150	0.01%	0.001%
12	3.027	616	618	623	rBV3	460	320	0.02%	0.002%
13	3.079	632	634	638	rBV3	507	401	0.02%	0.003%
14	3.098	638	640	643	rVV3	385	242	0.01%	0.002%
15	3.149	652	656	657	rBV	224	138	0.01%	0.001%
16	3.191	664	669	670	rVB2	183	134	0.01%	0.001%
17	3.201	670	672	676	rBV2	223	162	0.01%	0.001%
18	3.246	684	686	687	rBV2	224	109	0.01%	0.001%
19	3.256	687	689	692	rVB	395	197	0.01%	0.001%
20	3.268	692	693	696	rBV2	211	108	0.01%	0.001%
21	3.288	696	699	700	rBV	371	170	0.01%	0.001%
22	3.378	724	727	728	rBV2	242	164	0.01%	0.001%
23	3.403	733	735	738	rVB3	336	185	0.01%	0.001%
24	3.477	756	758	760	rBV2	256	113	0.01%	0.001%
25	3.516	768	770	773	rVB2	364	170	0.01%	0.001%
26	3.539	773	777	780	rBV2	359	278	0.02%	0.002%
27	3.612	796	800	805	rBV3	350	411	0.02%	0.003%
28	3.693	822	825	827	rBV2	292	179	0.01%	0.001%
29	3.722	831	834	837	rBV2	193	123	0.01%	0.001%
30	3.744	837	841	845	rBV3	420	379	0.02%	0.003%
31	3.770	845	849	853	rBV3	173	133	0.01%	0.001%
32	3.786	853	854	858	rBV2	308	216	0.01%	0.002%
33	3.866	869	879	916	rBV	154140	403473	22.18%	2.896%
34	4.346	1011	1028	1051	rBV	284944	704338	38.71%	5.056%
35	4.850	1179	1185	1186	rBV2	413	283	0.02%	0.002%
36	4.876	1191	1193	1195	rVV2	365	199	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071221\
 Data File : VV021618.D
 Acq On : 12 Jul 2021 11:48
 Operator : SY/MD
 Sample : VV0712WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK212

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
 Title : VOC Analysis

37	4.902	1199	1201	1208	rVV3	438	393	0.02%	0.003%
38	4.979	1221	1225	1227	rBV3	330	232	0.01%	0.002%
39	5.043	1227	1245	1277	rBV2	716762	1819319	100.00%	13.059%
40	5.567	1404	1408	1410	rBV2	492	326	0.02%	0.002%
41	5.616	1410	1423	1459	rVV	531763	1069015	58.76%	7.673%
42	5.905	1503	1513	1528	rBV4	11059	23590	1.30%	0.169%
43	5.982	1535	1537	1538	rBV	335	152	0.01%	0.001%
44	6.069	1549	1564	1593	rBV	395558	811723	44.62%	5.826%
45	6.291	1630	1633	1634	rBV2	272	146	0.01%	0.001%
46	6.333	1644	1646	1650	rBV4	517	356	0.02%	0.003%
47	6.423	1670	1674	1676	rVB2	260	177	0.01%	0.001%
48	6.442	1678	1680	1685	rVB	430	229	0.01%	0.002%
49	6.493	1693	1696	1699	rBV2	578	427	0.02%	0.003%
50	6.606	1728	1731	1734	rVB2	377	227	0.01%	0.002%
51	6.645	1736	1743	1746	rBV3	811	1165	0.06%	0.008%
52	6.725	1764	1768	1770	rBV2	419	286	0.02%	0.002%
53	6.754	1775	1777	1779	rVB	197	96	0.01%	0.001%
54	6.780	1783	1785	1788	rBV2	474	302	0.02%	0.002%
55	6.818	1793	1797	1798	rBV	350	200	0.01%	0.001%
56	6.850	1804	1807	1812	rVB2	379	234	0.01%	0.002%
57	6.889	1812	1819	1825	rBV3	385	560	0.03%	0.004%
58	6.915	1825	1827	1829	rBV2	280	134	0.01%	0.001%
59	6.985	1835	1849	1871	rBV	253948	456462	25.09%	3.276%
60	7.317	1939	1952	1970	rBV	890179	1527767	83.97%	10.966%
61	7.622	2036	2047	2071	rBV	168488	299151	16.44%	2.147%
62	7.895	2128	2132	2135	rBV2	202	189	0.01%	0.001%
63	7.927	2139	2142	2146	rBV3	461	411	0.02%	0.003%
64	8.050	2177	2180	2181	rBV2	338	192	0.01%	0.001%
65	8.085	2181	2191	2227	rBV	491901	889107	48.87%	6.382%
66	8.464	2305	2309	2310	rBV2	270	184	0.01%	0.001%
67	8.513	2322	2324	2326	rVB3	454	198	0.01%	0.001%
68	8.525	2326	2328	2329	rBV3	346	159	0.01%	0.001%
69	8.596	2348	2350	2355	rBV3	497	359	0.02%	0.003%
70	8.673	2372	2374	2377	rVB2	454	235	0.01%	0.002%
71	8.696	2377	2381	2383	rBV2	471	283	0.02%	0.002%
72	8.712	2383	2386	2389	rVB	429	292	0.02%	0.002%
73	8.747	2394	2397	2400	rVB2	443	223	0.01%	0.002%
74	8.776	2404	2406	2410	rBV3	366	241	0.01%	0.002%
75	8.799	2410	2413	2415	rBV	302	160	0.01%	0.001%
76	8.853	2417	2430	2459	rBV	773911	1265289	69.55%	9.082%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071221\
 Data File : VV021618.D
 Acq On : 12 Jul 2021 11:48
 Operator : SY/MD
 Sample : VV0712WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK212

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
 Title : VOC Analysis

77	9.095	2503	2505	2511	rVB3	527	315	0.02%	0.002%
78	9.133	2515	2517	2519	rBV3	668	300	0.02%	0.002%
79	9.242	2547	2551	2554	rBV	199	182	0.01%	0.001%
80	9.262	2554	2557	2560	rVV2	489	323	0.02%	0.002%
81	9.287	2563	2565	2568	rBV	297	225	0.01%	0.002%
82	9.329	2575	2578	2580	rBV	306	166	0.01%	0.001%
83	9.368	2588	2590	2593	rBV2	247	164	0.01%	0.001%
84	9.464	2616	2620	2624	rBV2	178	178	0.01%	0.001%
85	9.487	2624	2627	2628	rBV	363	240	0.01%	0.002%
86	9.619	2666	2668	2672	rBV2	539	447	0.02%	0.003%
87	9.760	2710	2712	2715	rBV2	253	130	0.01%	0.001%
88	9.786	2717	2720	2724	rBV	215	197	0.01%	0.001%
89	9.940	2765	2768	2773	rVB	703	425	0.02%	0.003%
90	10.017	2790	2792	2793	rBV	363	123	0.01%	0.001%
91	10.095	2814	2816	2817	rBV	292	129	0.01%	0.001%
92	10.127	2818	2826	2838	rVB2	7644	11586	0.64%	0.083%
93	10.217	2842	2854	2875	rBV	557034	872596	47.96%	6.263%
94	10.445	2923	2925	2926	rBV	472	174	0.01%	0.001%
95	10.541	2952	2955	2958	rBV3	852	656	0.04%	0.005%
96	11.027	3102	3106	3107	rBV3	1233	847	0.05%	0.006%
97	11.146	3136	3143	3153	rVB4	4414	6327	0.35%	0.045%
98	11.249	3164	3175	3195	rBV	807094	1286806	70.73%	9.236%
99	11.625	3280	3292	3314	rBV	858213	1358925	74.69%	9.754%
100	12.500	3561	3564	3568	rVB5	733	385	0.02%	0.003%




Sum of corrected areas: 13931779

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071221\
Data File : VV021618.D
Acq On : 12 Jul 2021 11:48
Operator : SY/MD
Sample : VV0712WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
VBLK212

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

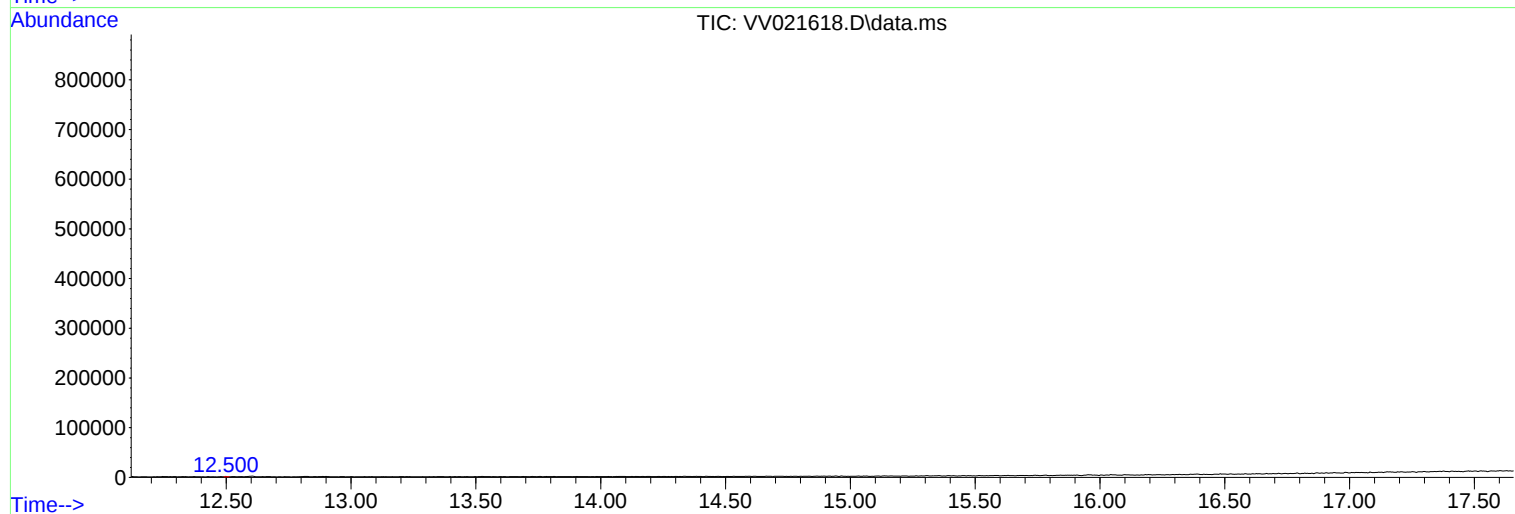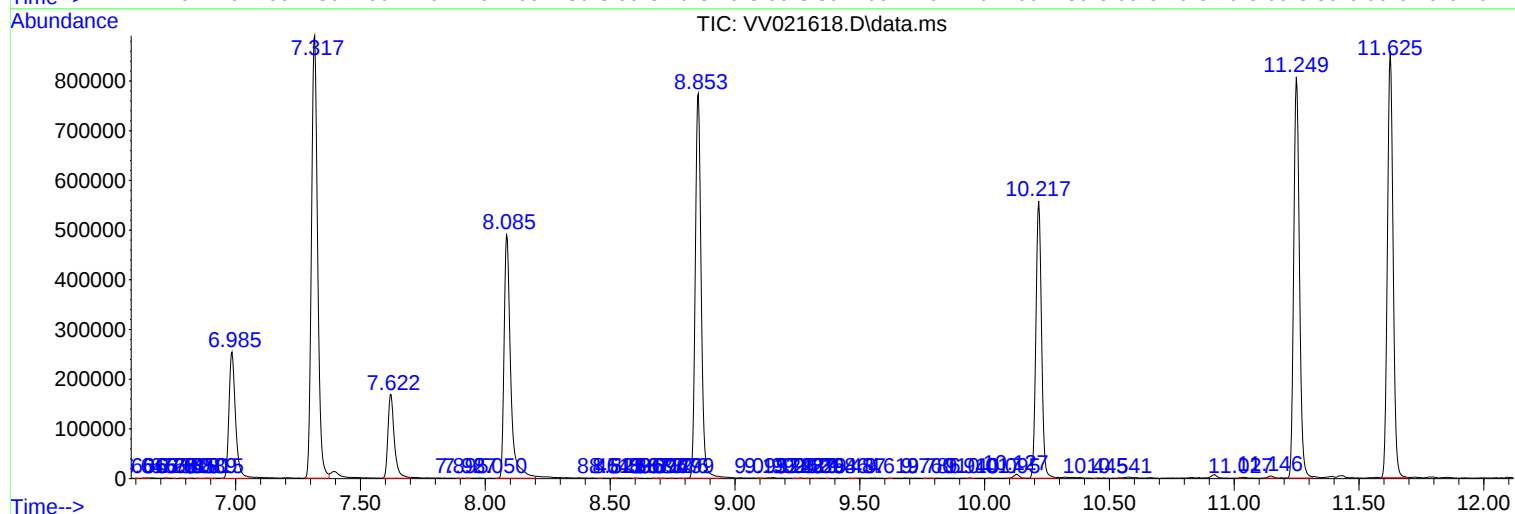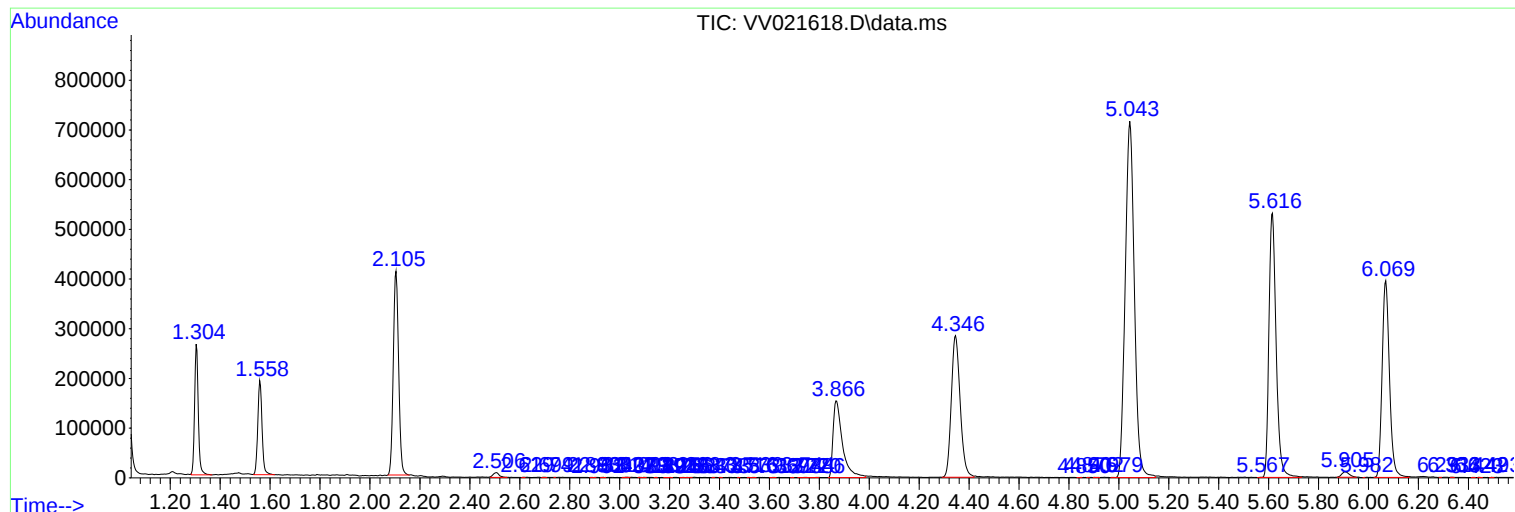

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071221\
Data File : VV021618.D
Acq On : 12 Jul 2021 11:48
Operator : SY/MD
Sample : VV0712WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK212

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071221\
Data File : VV021618.D
Acq On : 12 Jul 2021 11:48
Operator : SY/MD
Sample : VV0712WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK212

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
