

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071221\
 Data File : VV021619.D
 Acq On : 12 Jul 2021 12:25
 Operator : SY/MD
 Sample : M2970-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGEB0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M

Title : VOC Analysis

Signal : TIC: VV021619.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	99	rVB	285008	282241	14.70%	2.004%
2	1.558	154	161	179	rVB	203988	239816	12.49%	1.703%
3	2.101	321	330	345	rBV	433724	635675	33.10%	4.514%
4	2.506	449	456	462	rVB7	1434	2282	0.12%	0.016%
5	2.937	587	590	593	rBV2	358	303	0.02%	0.002%
6	2.969	593	600	604	rVV3	485	562	0.03%	0.004%
7	3.014	612	614	617	rBV2	289	149	0.01%	0.001%
8	3.076	631	633	635	rBV	280	161	0.01%	0.001%
9	3.117	642	646	648	rBV2	374	228	0.01%	0.002%
10	3.133	648	651	652	rVB	557	229	0.01%	0.002%
11	3.153	652	657	660	rVB3	359	323	0.02%	0.002%
12	3.178	661	665	666	rBV	366	206	0.01%	0.001%
13	3.346	714	717	719	rBV	274	179	0.01%	0.001%
14	3.413	735	738	741	rVB2	318	189	0.01%	0.001%
15	3.432	741	744	747	rBV	152	121	0.01%	0.001%
16	3.474	751	757	759	rBV4	386	394	0.02%	0.003%
17	3.522	769	772	776	rVV3	304	261	0.01%	0.002%
18	3.561	781	784	787	rVB2	241	121	0.01%	0.001%
19	3.580	787	790	794	rBV	377	284	0.01%	0.002%
20	3.600	794	796	799	rVB2	514	274	0.01%	0.002%
21	3.622	799	803	805	rBV2	302	193	0.01%	0.001%
22	3.667	812	817	820	rBV3	449	482	0.03%	0.003%
23	3.728	834	836	838	rBV	395	121	0.01%	0.001%
24	3.796	856	857	859	rBV	320	131	0.01%	0.001%
25	3.867	869	879	910	rBV	149435	386457	20.12%	2.744%
26	4.143	963	965	967	rBV	676	292	0.02%	0.002%
27	4.342	1012	1027	1053	rBV	299773	743199	38.70%	5.278%
28	4.635	1117	1118	1120	rBV	376	181	0.01%	0.001%
29	4.696	1134	1137	1140	rBV2	631	409	0.02%	0.003%
30	4.738	1147	1150	1153	rBV3	381	292	0.02%	0.002%
31	4.834	1177	1180	1181	rBV2	288	124	0.01%	0.001%
32	4.844	1181	1183	1187	rVB3	282	163	0.01%	0.001%
33	4.860	1187	1188	1190	rBV2	267	121	0.01%	0.001%
34	4.899	1198	1200	1202	rBV2	318	171	0.01%	0.001%
35	4.960	1217	1219	1222	rVB	402	190	0.01%	0.001%
36	4.979	1222	1225	1227	rBV	267	163	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW071221\
 Data File : VW021619.D
 Acq On : 12 Jul 2021 12:25
 Operator : SY/MD
 Sample : M2970-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGEB0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
 Title : VOC Analysis

37	5.043	1227	1245	1272	rBV2	745932	1920654	100.00%	13.640%
38	5.326	1329	1333	1335	rBV3	621	502	0.03%	0.004%
39	5.493	1383	1385	1388	rVB2	600	252	0.01%	0.002%
40	5.510	1388	1390	1393	rVB2	542	336	0.02%	0.002%
41	5.542	1397	1400	1403	rBV2	699	543	0.03%	0.004%
42	5.612	1410	1422	1445	rBV	488208	984415	51.25%	6.991%
43	5.902	1502	1512	1526	rBV4	16683	35751	1.86%	0.254%
44	6.066	1546	1563	1592	rBV	421076	862241	44.89%	6.123%
45	6.291	1631	1633	1636	rBV2	368	258	0.01%	0.002%
46	6.323	1640	1643	1644	rBV	277	151	0.01%	0.001%
47	6.368	1655	1657	1661	rBV	619	369	0.02%	0.003%
48	6.423	1672	1674	1677	rBV	372	174	0.01%	0.001%
49	6.461	1681	1686	1689	rBV3	648	552	0.03%	0.004%
50	6.712	1762	1764	1765	rBV2	434	184	0.01%	0.001%
51	6.802	1789	1792	1793	rBV	380	143	0.01%	0.001%
52	6.847	1803	1806	1809	rBV3	391	274	0.01%	0.002%
53	6.921	1828	1829	1832	rVB	349	123	0.01%	0.001%
54	6.937	1832	1834	1835	rBV	330	136	0.01%	0.001%
55	6.982	1836	1848	1880	rBV	261793	481481	25.07%	3.419%
56	7.313	1939	1951	1968	rBV	930575	1608550	83.75%	11.423%
57	7.619	2036	2046	2076	rBV	183100	313201	16.31%	2.224%
58	7.831	2110	2112	2114	rVB2	686	255	0.01%	0.002%
59	7.915	2134	2138	2139	rBV3	336	212	0.01%	0.002%
60	7.927	2139	2142	2144	rBV2	1083	749	0.04%	0.005%
61	7.982	2157	2159	2164	rBV4	483	290	0.02%	0.002%
62	8.008	2165	2167	2169	rVB2	398	135	0.01%	0.001%
63	8.030	2173	2174	2178	rBV	236	165	0.01%	0.001%
64	8.085	2178	2191	2229	rBV	471387	869090	45.25%	6.172%
65	8.397	2285	2288	2289	rBV2	610	355	0.02%	0.003%
66	8.551	2333	2336	2338	rVB2	413	230	0.01%	0.002%
67	8.567	2338	2341	2342	rBV	501	328	0.02%	0.002%
68	8.590	2346	2348	2352	rVV3	398	228	0.01%	0.002%
69	8.619	2355	2357	2359	rBV2	311	172	0.01%	0.001%
70	8.654	2363	2368	2371	rVB3	424	315	0.02%	0.002%
71	8.673	2372	2374	2376	rBV2	324	151	0.01%	0.001%
72	8.738	2391	2394	2395	rBV	248	122	0.01%	0.001%
73	8.796	2410	2412	2414	rBV2	537	310	0.02%	0.002%
74	8.850	2418	2429	2464	rBV	712697	1185752	61.74%	8.421%
75	9.146	2516	2521	2531	rVB5	2483	3705	0.19%	0.026%
76	9.226	2544	2546	2549	rBV2	485	314	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071221\
 Data File : VV021619.D
 Acq On : 12 Jul 2021 12:25
 Operator : SY/MD
 Sample : M2970-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGEB0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
 Title : VOC Analysis

77	9.265	2555	2558	2562	rVB2	424	309	0.02%	0.002%
78	9.284	2562	2564	2565	rBV	309	155	0.01%	0.001%
79	9.397	2595	2599	2601	rVV3	421	287	0.01%	0.002%
80	9.503	2628	2632	2633	rBV	519	388	0.02%	0.003%
81	9.558	2641	2649	2660	rBV	3083	7273	0.38%	0.052%
82	9.670	2679	2684	2688	rBV3	832	810	0.04%	0.006%
83	9.789	2717	2721	2723	rBV	485	337	0.02%	0.002%
84	9.870	2743	2746	2750	rBV2	552	317	0.02%	0.002%
85	9.905	2755	2757	2759	rBV	321	145	0.01%	0.001%
86	9.918	2759	2761	2763	rVB	312	147	0.01%	0.001%
87	9.940	2763	2768	2771	rBV2	333	393	0.02%	0.003%
88	10.056	2802	2804	2806	rBV3	349	193	0.01%	0.001%
89	10.127	2815	2826	2835	rBV3	6862	11903	0.62%	0.085%
90	10.217	2842	2854	2878	rBV	563101	880848	45.86%	6.255%
91	10.545	2953	2956	2957	rBV2	617	345	0.02%	0.002%
92	10.751	3014	3020	3023	rBV3	792	703	0.04%	0.005%
93	10.776	3023	3028	3031	rBV3	778	733	0.04%	0.005%
94	10.828	3040	3044	3047	rBV4	747	722	0.04%	0.005%
95	11.037	3097	3109	3120	rBV5	1786	4555	0.24%	0.032%
96	11.149	3137	3144	3153	rBV6	3906	6289	0.33%	0.045%
97	11.249	3164	3175	3195	rBV	763690	1189672	61.94%	8.449%
98	11.625	3280	3292	3320	rBV	895522	1403732	73.09%	9.969%
99	11.985	3401	3404	3408	rBV3	856	733	0.04%	0.005%
100	13.004	3719	3721	3724	rBV	749	502	0.03%	0.004%




Sum of corrected areas: 14081346

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071221\
Data File : VV021619.D
Acq On : 12 Jul 2021 12:25
Operator : SY/MD
Sample : M2970-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
BGBE0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

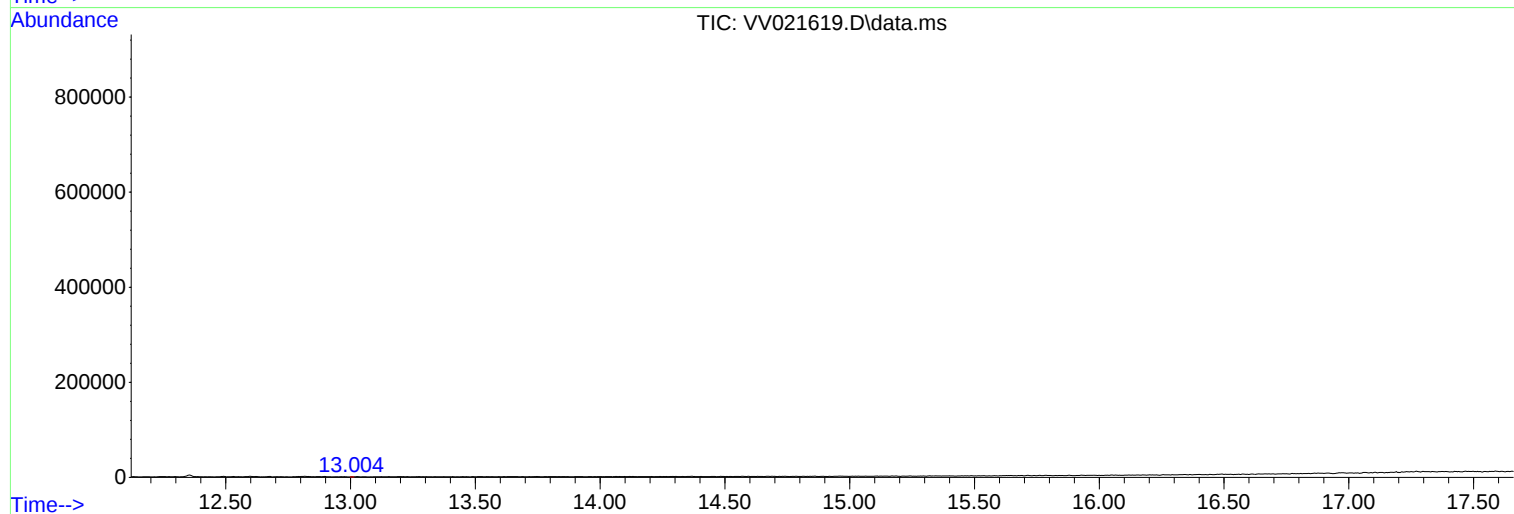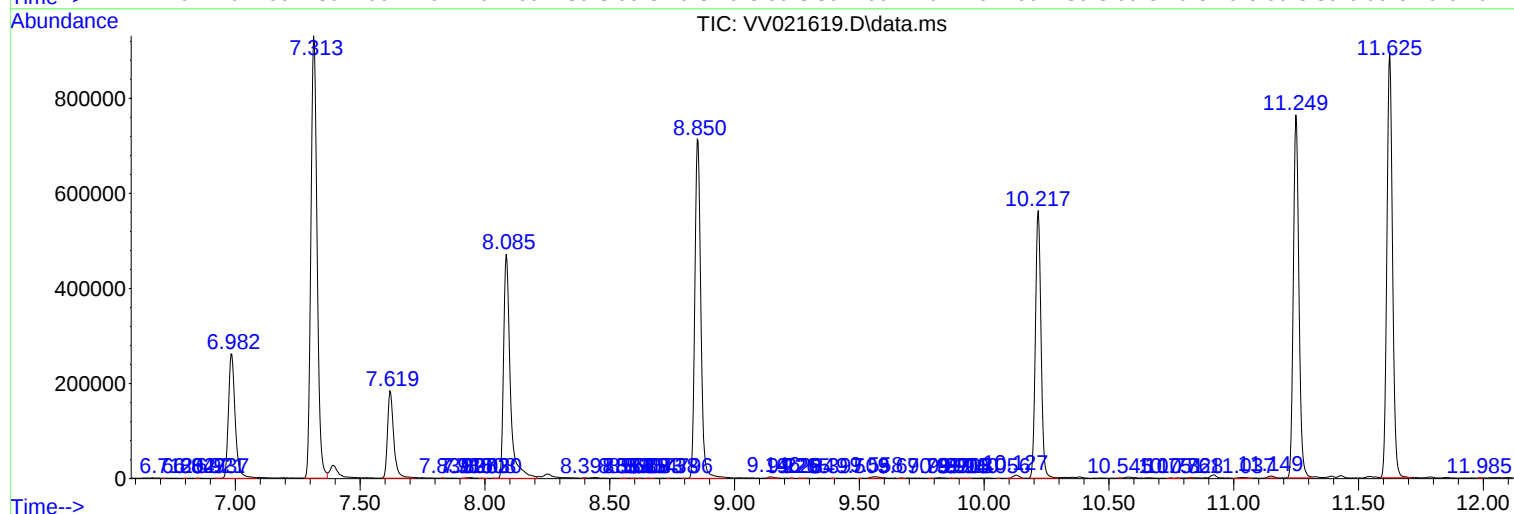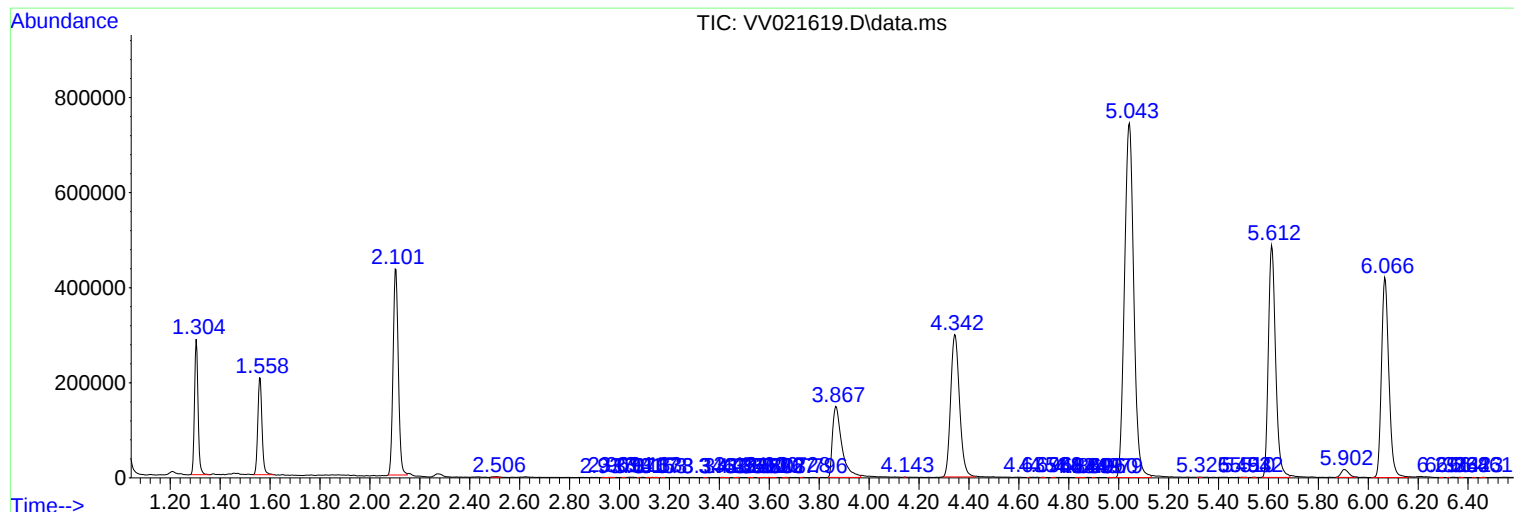

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071221\
Data File : VV021619.D
Acq On : 12 Jul 2021 12:25
Operator : SY/MD
Sample : M2970-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGEBO

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071221\
Data File : VV021619.D
Acq On : 12 Jul 2021 12:25
Operator : SY/MD
Sample : M2970-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGEBO

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
