

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071221\
 Data File : VV021620.D
 Acq On : 12 Jul 2021 12:49
 Operator : SY/MD
 Sample : M2959-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7H4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M

Title : VOC Analysis

Signal : TIC: VV021620.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	96	rVB	284627	275316	14.47%	2.010%
2	1.561	154	162	181	rVB	199360	236017	12.40%	1.723%
3	2.105	322	331	342	rBV	423627	603671	31.72%	4.408%
4	2.500	450	454	455	rBV2	1620	1142	0.06%	0.008%
5	2.558	469	472	476	rBV5	506	348	0.02%	0.003%
6	2.818	549	553	557	rBV3	308	293	0.02%	0.002%
7	2.889	573	575	579	rVB2	635	343	0.02%	0.003%
8	2.912	579	582	584	rBV	485	333	0.02%	0.002%
9	2.950	587	594	598	rBV3	1912	2627	0.14%	0.019%
10	3.114	642	645	647	rBV	282	179	0.01%	0.001%
11	3.150	654	656	658	rBV	192	76	0.00%	0.001%
12	3.159	658	659	661	rBV	139	37	0.00%	0.000%
13	3.169	661	662	664	rBV2	231	105	0.01%	0.001%
14	3.217	670	677	679	rBV4	508	528	0.03%	0.004%
15	3.249	685	687	690	rBV	293	159	0.01%	0.001%
16	3.285	694	698	701	rVB	310	256	0.01%	0.002%
17	3.307	701	705	707	rBV2	493	321	0.02%	0.002%
18	3.378	723	727	729	rVB2	264	199	0.01%	0.001%
19	3.394	729	732	734	rBV2	167	115	0.01%	0.001%
20	3.407	734	736	739	rBV2	196	156	0.01%	0.001%
21	3.420	739	740	741	rVB	245	47	0.00%	0.000%
22	3.432	741	744	745	rBV	219	106	0.01%	0.001%
23	3.481	757	759	762	rBV	189	99	0.01%	0.001%
24	3.529	771	774	776	rBV	333	141	0.01%	0.001%
25	3.609	797	799	801	rVB	250	77	0.00%	0.001%
26	3.622	801	803	805	rBV	323	180	0.01%	0.001%
27	3.690	817	824	827	rBV2	901	1069	0.06%	0.008%
28	3.780	850	852	853	rBV2	383	180	0.01%	0.001%
29	3.870	870	880	915	rBV	159421	417102	21.91%	3.045%
30	4.349	1012	1029	1055	rBV	296242	733511	38.54%	5.356%
31	4.674	1124	1130	1132	rBV5	778	810	0.04%	0.006%
32	4.770	1157	1160	1164	rVB2	593	376	0.02%	0.003%
33	4.799	1164	1169	1171	rBV2	328	194	0.01%	0.001%
34	4.815	1172	1174	1176	rBV	189	110	0.01%	0.001%
35	4.857	1186	1187	1190	rVB2	349	143	0.01%	0.001%
36	4.879	1190	1194	1197	rBV3	303	277	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071221\
 Data File : VV021620.D
 Acq On : 12 Jul 2021 12:49
 Operator : SY/MD
 Sample : M2959-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7H4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
 Title : VOC Analysis

37	4.921	1204	1207	1212	rVB4	614	472	0.02%	0.003%
38	4.950	1212	1216	1221	rBV3	396	428	0.02%	0.003%
39	5.047	1228	1246	1286	rBV2	739830	1903319	100.00%	13.897%
40	5.477	1378	1380	1381	rBV2	300	88	0.00%	0.001%
41	5.616	1410	1423	1457	rBV	442968	900958	47.34%	6.578%
42	5.908	1503	1514	1532	rBV2	18373	40795	2.14%	0.298%
43	6.014	1544	1547	1548	rBV	525	283	0.01%	0.002%
44	6.069	1551	1564	1588	rBV	413985	847775	44.54%	6.190%
45	6.471	1686	1689	1691	rBV2	364	268	0.01%	0.002%
46	6.513	1698	1702	1705	rBV3	727	712	0.04%	0.005%
47	6.776	1783	1784	1785	rBV3	41	9	0.00%	0.000%
48	6.786	1785	1787	1788	rBV	143	64	0.00%	0.000%
49	6.802	1788	1792	1795	rVV2	511	319	0.02%	0.002%
50	6.815	1795	1796	1799	rVB2	277	100	0.01%	0.001%
51	6.831	1799	1801	1802	rBV	261	126	0.01%	0.001%
52	6.873	1812	1814	1816	rBV	309	124	0.01%	0.001%
53	6.928	1829	1831	1832	rBV	233	61	0.00%	0.000%
54	6.989	1833	1850	1880	rBV	259094	471713	24.78%	3.444%
55	7.182	1906	1910	1911	rBV4	828	547	0.03%	0.004%
56	7.317	1940	1952	1970	rBV	920773	1577312	82.87%	11.516%
57	7.622	2035	2047	2071	rBV	177178	307108	16.14%	2.242%
58	7.882	2125	2128	2131	rBV	347	270	0.01%	0.002%
59	7.899	2131	2133	2135	rVB	633	276	0.01%	0.002%
60	7.940	2138	2146	2154	rVV6	2270	3342	0.18%	0.024%
61	8.017	2164	2170	2174	rBV3	563	552	0.03%	0.004%
62	8.046	2174	2179	2181	rBV3	521	503	0.03%	0.004%
63	8.088	2181	2192	2227	rBV	509389	930415	48.88%	6.793%
64	8.587	2346	2347	2349	rBV3	262	122	0.01%	0.001%
65	8.664	2369	2371	2375	rVB3	423	251	0.01%	0.002%
66	8.718	2386	2388	2389	rBV	299	142	0.01%	0.001%
67	8.751	2395	2398	2400	rBV2	300	153	0.01%	0.001%
68	8.786	2405	2409	2412	rVB2	261	221	0.01%	0.002%
69	8.805	2412	2415	2417	rVB3	306	139	0.01%	0.001%
70	8.853	2418	2430	2475	rBV	652964	1077493	56.61%	7.867%
71	9.069	2495	2497	2503	rVB2	474	267	0.01%	0.002%
72	9.333	2576	2579	2581	rBV	138	87	0.00%	0.001%
73	9.410	2598	2603	2604	rBV2	479	313	0.02%	0.002%
74	9.452	2614	2616	2619	rBV2	334	147	0.01%	0.001%
75	9.625	2668	2670	2672	rVB	241	77	0.00%	0.001%
76	9.696	2691	2692	2694	rVB	433	110	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071221\
 Data File : VV021620.D
 Acq On : 12 Jul 2021 12:49
 Operator : SY/MD
 Sample : M2959-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7H4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M

Title : VOC Analysis

77	9.741	2704	2706	2711	rVB2	559	319	0.02%	0.002%
78	9.773	2713	2716	2720	rBV	481	413	0.02%	0.003%
79	9.943	2766	2769	2775	rVB3	456	381	0.02%	0.003%
80	10.021	2787	2793	2799	rBV6	981	1401	0.07%	0.010%
81	10.056	2803	2804	2806	rBV	202	95	0.00%	0.001%
82	10.127	2819	2826	2835	rBV2	5786	8726	0.46%	0.064%
83	10.217	2842	2854	2876	rBV	571860	890410	46.78%	6.501%
84	10.664	2986	2993	2999	rBV4	1042	1504	0.08%	0.011%
85	10.709	3003	3007	3012	rBV3	638	774	0.04%	0.006%
86	10.918	3065	3072	3077	rBV4	5526	8650	0.45%	0.063%
87	11.249	3164	3175	3198	rBV	692453	1067819	56.10%	7.796%
88	11.625	3280	3292	3314	rBV	869414	1371322	72.05%	10.012%
89	11.818	3351	3352	3355	rBV	517	269	0.01%	0.002%
90	12.220	3475	3477	3478	rBV	418	168	0.01%	0.001%




Sum of corrected areas: 13696355

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071221\
Data File : VV021620.D
Acq On : 12 Jul 2021 12:49
Operator : SY/MD
Sample : M2959-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
BG7H4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

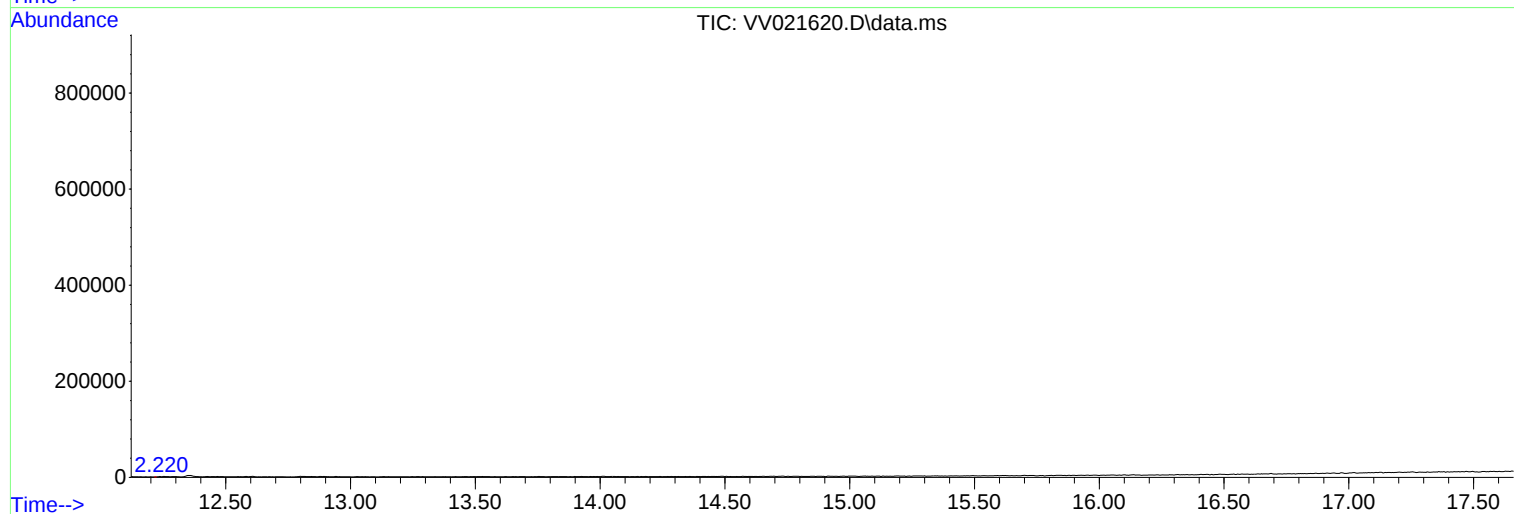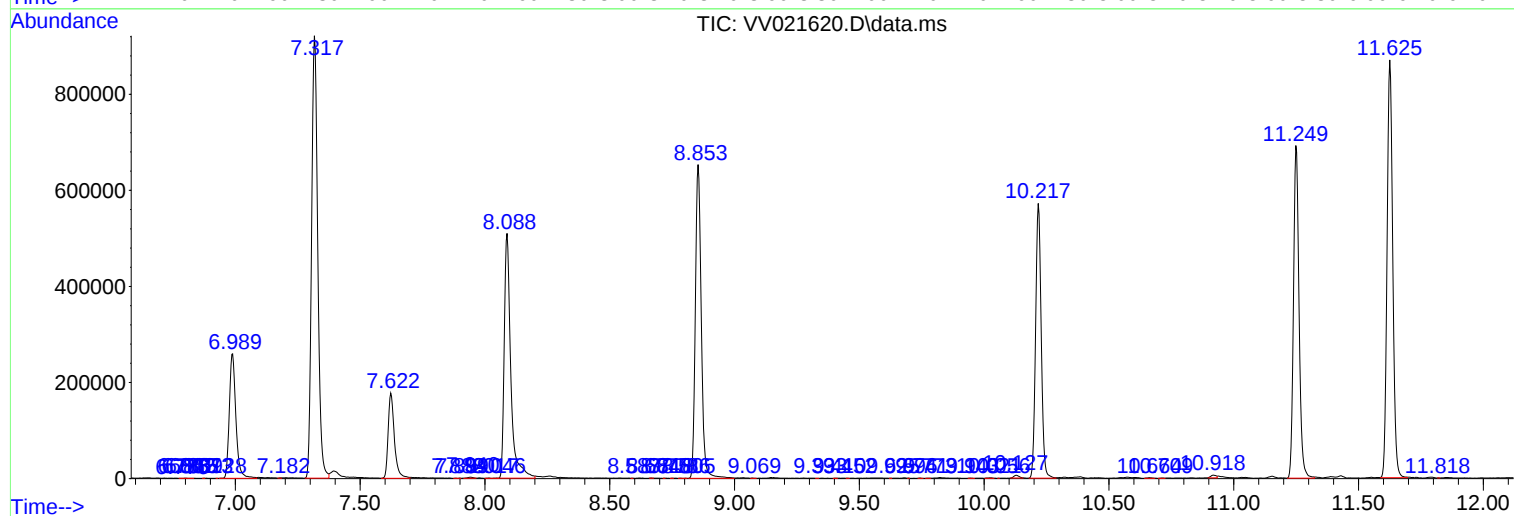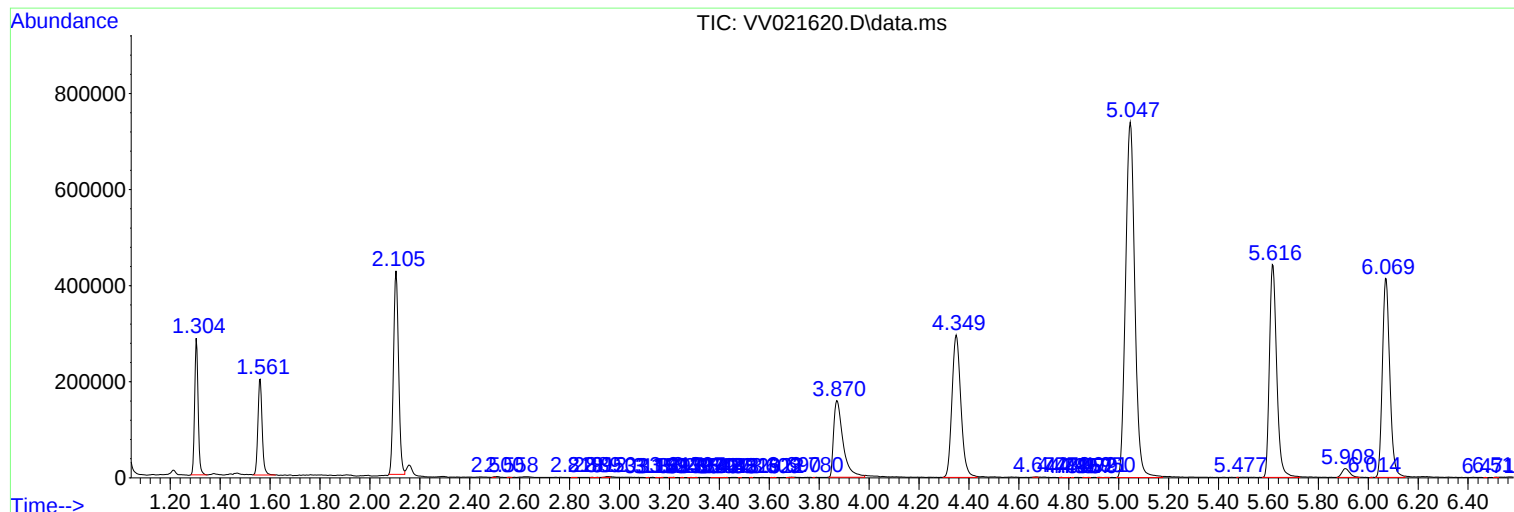

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071221\
Data File : VV021620.D
Acq On : 12 Jul 2021 12:49
Operator : SY/MD
Sample : M2959-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7H4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071221\
Data File : VV021620.D
Acq On : 12 Jul 2021 12:49
Operator : SY/MD
Sample : M2959-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7H4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
