

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071221\
 Data File : VV021622.D
 Acq On : 12 Jul 2021 13:37
 Operator : SY/MD
 Sample : M2978-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7H5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M

Title : VOC Analysis

Signal : TIC: VV021622.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	98	rVB	254199	254922	14.62%	1.882%
2	1.561	154	162	177	rVB	184054	217539	12.48%	1.606%
3	2.105	321	331	342	rBV	393132	565882	32.46%	4.178%
4	2.510	449	457	458	rBV4	1905	2282	0.13%	0.017%
5	2.622	487	492	495	rBV2	1220	1497	0.09%	0.011%
6	2.751	523	532	540	rBV4	1616	3279	0.19%	0.024%
7	2.950	587	594	595	rBV3	1998	1805	0.10%	0.013%
8	3.037	612	621	636	rVB4	6920	14212	0.82%	0.105%
9	3.188	663	668	670	rBV3	376	285	0.02%	0.002%
10	3.220	675	678	683	rVV4	352	301	0.02%	0.002%
11	3.423	734	741	743	rBV3	656	575	0.03%	0.004%
12	3.436	743	745	749	rVV2	405	307	0.02%	0.002%
13	3.764	834	847	860	rBV4	8012	18311	1.05%	0.135%
14	3.873	871	881	913	rBV	143897	377460	21.65%	2.787%
15	4.349	1013	1029	1057	rBV	271571	673180	38.62%	4.971%
16	4.532	1083	1086	1088	rBV3	500	277	0.02%	0.002%
17	4.600	1105	1107	1111	rBV3	400	306	0.02%	0.002%
18	4.674	1122	1130	1132	rBV4	1268	1320	0.08%	0.010%
19	4.735	1146	1149	1156	rBV4	609	595	0.03%	0.004%
20	4.870	1187	1191	1195	rVB3	610	608	0.03%	0.004%
21	5.047	1226	1246	1282	rBV2	680340	1743173	100.00%	12.871%
22	5.313	1324	1329	1335	rBV5	613	631	0.04%	0.005%
23	5.497	1384	1386	1391	rVB4	591	343	0.02%	0.003%
24	5.545	1397	1401	1405	rVB5	479	446	0.03%	0.003%
25	5.616	1411	1423	1453	rBV	543700	1098092	62.99%	8.108%
26	5.908	1500	1514	1526	rBV2	17891	37970	2.18%	0.280%
27	6.072	1550	1565	1591	rBV	382509	778894	44.68%	5.751%
28	6.201	1602	1605	1606	rBV2	500	320	0.02%	0.002%
29	6.304	1633	1637	1638	rBV2	589	404	0.02%	0.003%
30	6.346	1647	1650	1653	rVB3	545	321	0.02%	0.002%
31	6.378	1656	1660	1661	rBV3	475	277	0.02%	0.002%
32	6.458	1681	1685	1688	rVB2	796	602	0.03%	0.004%
33	6.535	1705	1709	1710	rBV3	469	315	0.02%	0.002%
34	6.635	1736	1740	1743	rBV4	700	610	0.03%	0.005%
35	6.744	1769	1774	1776	rBV3	410	354	0.02%	0.003%
36	6.764	1776	1780	1782	rVV2	517	277	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071221\
 Data File : VV021622.D
 Acq On : 12 Jul 2021 13:37
 Operator : SY/MD
 Sample : M2978-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7H5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
 Title : VOC Analysis

37	6.895	1818	1821	1824	rBV3	476	424	0.02%	0.003%
38	6.937	1829	1834	1837	rBV2	557	505	0.03%	0.004%
39	6.989	1838	1850	1873	rBV	237145	427513	24.52%	3.157%
40	7.188	1910	1912	1914	rBV2	618	366	0.02%	0.003%
41	7.227	1922	1924	1927	rVB3	629	295	0.02%	0.002%
42	7.317	1940	1952	1970	rBV	845864	1452634	83.33%	10.726%
43	7.622	2037	2047	2074	rBV	159133	277768	15.93%	2.051%
44	7.776	2092	2095	2097	rVB2	486	284	0.02%	0.002%
45	7.873	2123	2125	2130	rVV4	498	327	0.02%	0.002%
46	7.937	2139	2145	2155	rVB5	2482	3658	0.21%	0.027%
47	8.043	2172	2178	2181	rVV3	504	506	0.03%	0.004%
48	8.088	2181	2192	2228	rBV	452493	840888	48.24%	6.209%
49	8.400	2284	2289	2295	rVB5	499	476	0.03%	0.004%
50	8.442	2298	2302	2305	rBV4	587	407	0.02%	0.003%
51	8.484	2313	2315	2318	rVB	647	346	0.02%	0.003%
52	8.513	2318	2324	2326	rBV3	457	342	0.02%	0.003%
53	8.538	2329	2332	2334	rBV2	485	283	0.02%	0.002%
54	8.632	2359	2361	2365	rBV4	541	370	0.02%	0.003%
55	8.673	2372	2374	2377	rBV	433	278	0.02%	0.002%
56	8.853	2418	2430	2462	rBV	808098	1310664	75.19%	9.678%
57	9.017	2479	2481	2482	rBV3	841	324	0.02%	0.002%
58	9.091	2500	2504	2510	rVB3	479	449	0.03%	0.003%
59	9.146	2514	2521	2531	rVB7	1664	2767	0.16%	0.020%
60	9.558	2644	2649	2650	rVV3	640	546	0.03%	0.004%
61	9.580	2653	2656	2658	rVB2	528	315	0.02%	0.002%
62	9.773	2712	2716	2719	rBV2	617	598	0.03%	0.004%
63	9.911	2755	2759	2764	rBV3	475	520	0.03%	0.004%
64	9.979	2775	2780	2784	rBV3	504	492	0.03%	0.004%
65	10.021	2787	2793	2798	rBV6	835	1136	0.07%	0.008%
66	10.085	2809	2813	2817	rBV3	463	397	0.02%	0.003%
67	10.130	2817	2827	2838	rBV4	5604	9501	0.55%	0.070%
68	10.217	2842	2854	2876	rVV	517076	810002	46.47%	5.981%
69	10.320	2880	2886	2894	rVV5	1505	2966	0.17%	0.022%
70	10.381	2898	2905	2916	rVB5	3545	6855	0.39%	0.051%
71	10.426	2916	2919	2922	rBV3	396	372	0.02%	0.003%
72	10.570	2960	2964	2976	rBV7	1166	2032	0.12%	0.015%
73	10.657	2986	2991	3001	rVB4	844	1328	0.08%	0.010%
74	10.706	3003	3006	3009	rBV2	494	277	0.02%	0.002%
75	10.869	3054	3057	3060	rBV4	579	552	0.03%	0.004%
76	10.924	3065	3074	3093	rVB9	5213	14767	0.85%	0.109%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071221\
 Data File : VV021622.D
 Acq On : 12 Jul 2021 13:37
 Operator : SY/MD
 Sample : M2978-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7H5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
 Title : VOC Analysis

77	11.030	3103	3107	3111	rBV6	920	755	0.04%	0.006%
78	11.078	3120	3122	3126	rVB2	655	385	0.02%	0.003%
79	11.146	3133	3143	3144	rBV2	3475	3309	0.19%	0.024%
80	11.249	3164	3175	3204	rBV	817157	1283580	73.63%	9.478%
81	11.548	3264	3268	3270	rBV3	756	515	0.03%	0.004%
82	11.625	3279	3292	3317	rBV	803028	1265426	72.59%	9.344%
83	11.921	3381	3384	3390	rVB2	430	385	0.02%	0.003%
84	11.988	3402	3405	3407	rBV2	551	321	0.02%	0.002%
85	12.104	3432	3441	3443	rBV5	632	950	0.05%	0.007%
86	12.258	3485	3489	3492	rBV3	777	670	0.04%	0.005%
87	12.355	3509	3519	3532	rBV7	3414	6506	0.37%	0.048%
88	12.599	3587	3595	3600	rBV5	1333	2049	0.12%	0.015%
89	12.676	3617	3619	3623	rVB3	484	302	0.02%	0.002%
90	12.795	3649	3656	3657	rBV4	1107	1008	0.06%	0.007%
91	12.921	3692	3695	3698	rBV3	483	367	0.02%	0.003%
92	13.078	3741	3744	3748	rBV3	374	395	0.02%	0.003%
93	13.156	3765	3768	3772	rVB3	477	389	0.02%	0.003%
94	13.181	3772	3776	3778	rBV2	350	310	0.02%	0.002%
95	13.484	3868	3870	3873	rBV2	357	302	0.02%	0.002%
96	13.625	3911	3914	3921	rBV6	693	622	0.04%	0.005%
97	13.738	3945	3949	3953	rVV3	666	562	0.03%	0.004%
98	14.088	4054	4058	4063	rBV2	483	643	0.04%	0.005%
99	14.564	4204	4206	4208	rBV2	597	297	0.02%	0.002%
100	14.856	4295	4297	4299	rBV	649	379	0.02%	0.003%




Sum of corrected areas: 13542929

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071221\
Data File : VV021622.D
Acq On : 12 Jul 2021 13:37
Operator : SY/MD
Sample : M2978-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7H5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

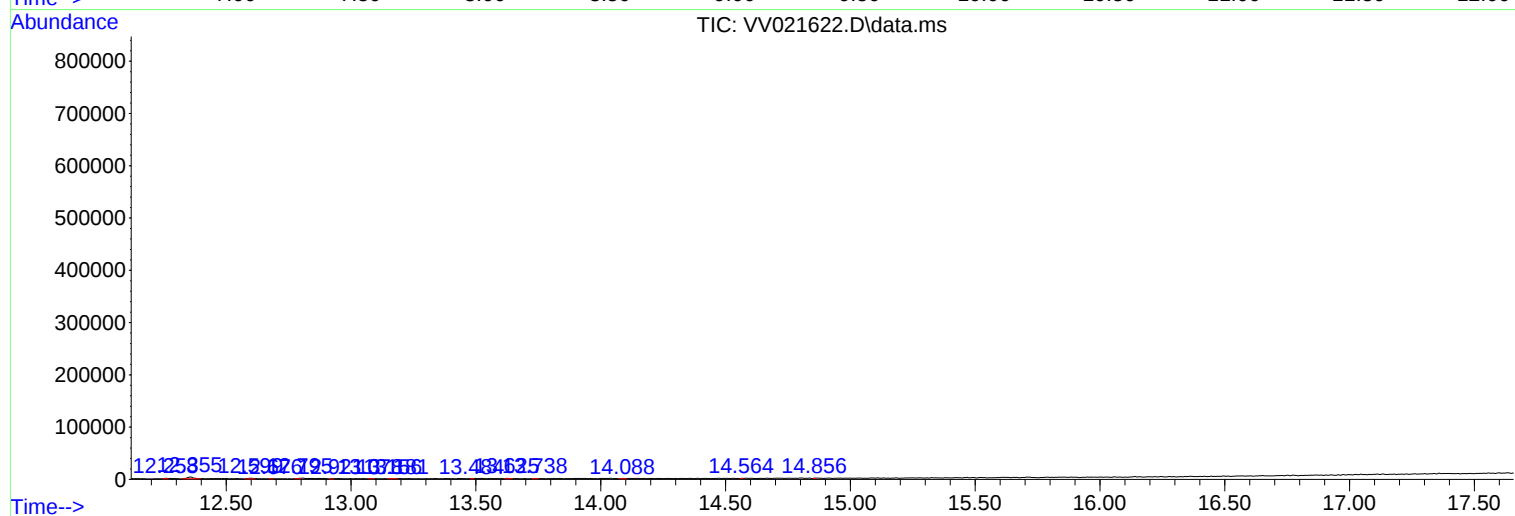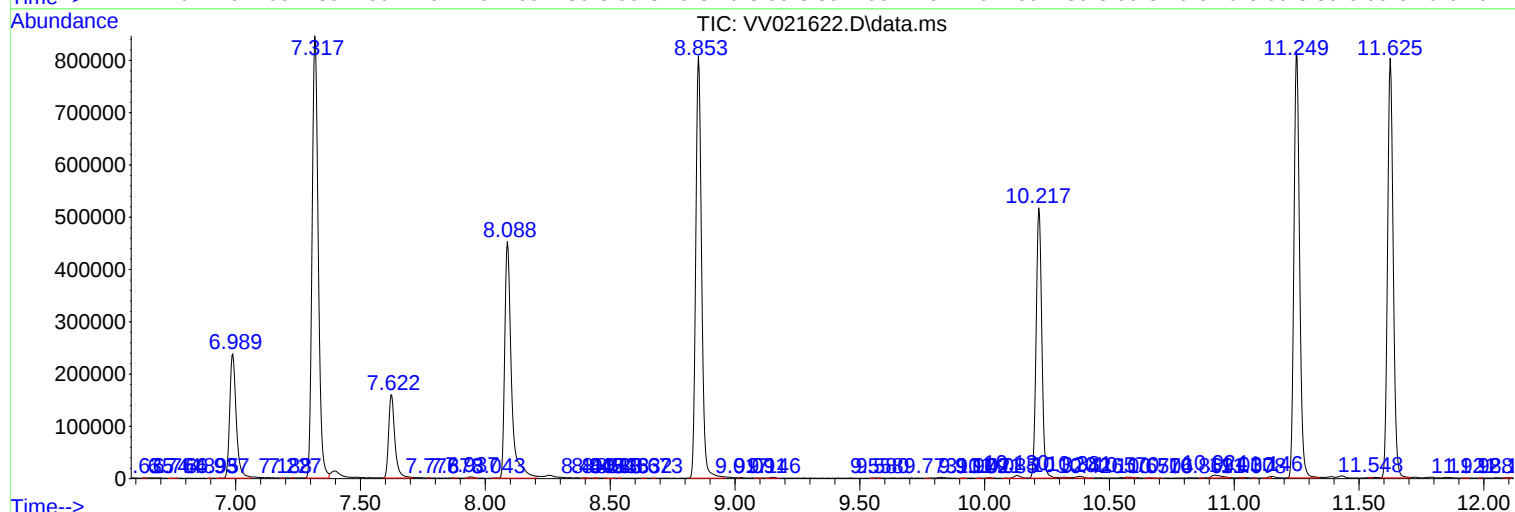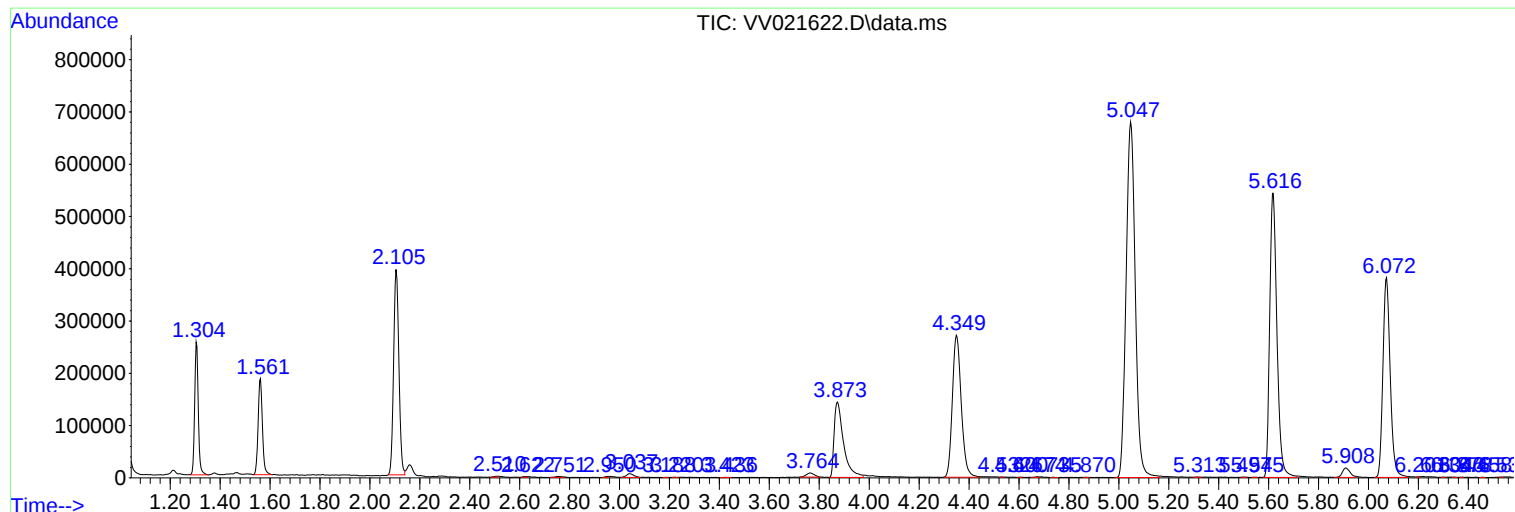

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071221\
Data File : VV021622.D
Acq On : 12 Jul 2021 13:37
Operator : SY/MD
Sample : M2978-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7H5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071221\
Data File : VV021622.D
Acq On : 12 Jul 2021 13:37
Operator : SY/MD
Sample : M2978-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7H5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
