

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071221\
 Data File : VV021623.D
 Acq On : 12 Jul 2021 14:01
 Operator : SY/MD
 Sample : M2978-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7J1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
 Title : VOC Analysis

Signal : TIC: VV021623.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	94	rBV	251763	249589	14.56%	1.850%
2	1.561	154	162	177	rVB	173293	208462	12.16%	1.545%
3	2.105	321	331	342	rBV	381841	555901	32.44%	4.120%
4	2.281	377	386	400	rVB3	4762	10596	0.62%	0.079%
5	2.507	449	456	464	rBV4	1591	2819	0.16%	0.021%
6	2.622	485	492	500	rVV4	1531	2637	0.15%	0.020%
7	2.761	527	535	542	rBV6	1324	2449	0.14%	0.018%
8	2.957	586	596	611	rBV6	1822	5002	0.29%	0.037%
9	3.037	611	621	637	rVV4	4789	10987	0.64%	0.081%
10	3.098	637	640	644	rVB3	665	503	0.03%	0.004%
11	3.140	650	653	657	rVB3	416	334	0.02%	0.002%
12	3.593	791	794	798	rBV	642	380	0.02%	0.003%
13	3.664	808	816	818	rBV2	480	452	0.03%	0.003%
14	3.687	818	823	828	rBV5	706	736	0.04%	0.005%
15	3.760	835	846	860	rBV3	5547	12328	0.72%	0.091%
16	3.873	870	881	921	rBV	146632	389363	22.72%	2.886%
17	4.278	1004	1007	1012	rVB4	540	471	0.03%	0.003%
18	4.349	1012	1029	1059	rBV	268227	666797	38.91%	4.942%
19	4.593	1102	1105	1110	rBV5	462	319	0.02%	0.002%
20	4.693	1135	1136	1140	rVB3	799	397	0.02%	0.003%
21	4.764	1155	1158	1162	rBV3	655	502	0.03%	0.004%
22	4.786	1162	1165	1168	rVV	435	380	0.02%	0.003%
23	4.854	1183	1186	1191	rBV2	452	354	0.02%	0.003%
24	4.918	1202	1206	1211	rVB3	510	355	0.02%	0.003%
25	4.960	1215	1219	1221	rBV3	402	336	0.02%	0.002%
26	5.047	1228	1246	1274	rBV2	671577	1713658	100.00%	12.701%
27	5.330	1330	1334	1336	rBV2	388	322	0.02%	0.002%
28	5.490	1378	1384	1389	rBV4	729	929	0.05%	0.007%
29	5.545	1399	1401	1406	rVB3	496	359	0.02%	0.003%
30	5.619	1411	1424	1457	rBV	548694	1118782	65.29%	8.292%
31	5.908	1503	1514	1536	rVB2	20880	44495	2.60%	0.330%
32	6.072	1550	1565	1593	rBV	373112	766535	44.73%	5.681%
33	6.214	1603	1609	1614	rBV7	1254	1620	0.09%	0.012%
34	6.304	1633	1637	1640	rBV2	494	471	0.03%	0.003%
35	6.497	1694	1697	1698	rBV	636	386	0.02%	0.003%
36	6.529	1703	1707	1708	rBV3	563	403	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071221\
 Data File : VV021623.D
 Acq On : 12 Jul 2021 14:01
 Operator : SY/MD
 Sample : M2978-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7J1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
 Title : VOC Analysis

37	6.542	1708	1711	1715	rVB4	631	438	0.03%	0.003%
38	6.571	1716	1720	1721	rBV3	472	341	0.02%	0.003%
39	6.754	1773	1777	1780	rBV2	520	430	0.03%	0.003%
40	6.931	1826	1832	1838	rBV3	590	944	0.06%	0.007%
41	6.989	1838	1850	1874	rBV	230650	419836	24.50%	3.112%
42	7.185	1907	1911	1913	rBV2	508	334	0.02%	0.002%
43	7.275	1935	1939	1940	rBV3	530	333	0.02%	0.002%
44	7.317	1940	1952	1971	rBV	821509	1429500	83.42%	10.595%
45	7.622	2037	2047	2074	rBV	153836	273461	15.96%	2.027%
46	7.940	2137	2146	2158	rBV4	2779	4750	0.28%	0.035%
47	7.982	2158	2159	2164	rVB3	537	384	0.02%	0.003%
48	8.053	2175	2181	2182	rBV4	664	623	0.04%	0.005%
49	8.088	2182	2192	2230	rBV2	440879	844763	49.30%	6.261%
50	8.439	2298	2301	2304	rVB4	749	508	0.03%	0.004%
51	8.571	2337	2342	2344	rBV4	354	317	0.02%	0.002%
52	8.619	2354	2357	2361	rBV3	479	425	0.02%	0.003%
53	8.638	2361	2363	2367	rVB2	551	401	0.02%	0.003%
54	8.683	2367	2377	2382	rVB3	732	727	0.04%	0.005%
55	8.709	2382	2385	2388	rBV2	509	475	0.03%	0.004%
56	8.786	2404	2409	2411	rBV2	443	400	0.02%	0.003%
57	8.854	2418	2430	2465	rBV	796960	1321892	77.14%	9.797%
58	9.114	2507	2511	2512	rBV3	468	319	0.02%	0.002%
59	9.156	2518	2524	2526	rBV3	890	940	0.05%	0.007%
60	9.564	2646	2651	2655	rVV4	669	539	0.03%	0.004%
61	9.818	2727	2730	2734	rBV2	744	794	0.05%	0.006%
62	9.876	2744	2748	2751	rBV3	386	367	0.02%	0.003%
63	10.130	2817	2827	2842	rVB3	5135	8712	0.51%	0.065%
64	10.217	2842	2854	2875	rBV	510397	806406	47.06%	5.977%
65	10.384	2900	2906	2915	rVB3	6894	10670	0.62%	0.079%
66	10.583	2960	2968	2974	rBV6	1599	2660	0.16%	0.020%
67	10.661	2986	2992	2994	rBV2	805	731	0.04%	0.005%
68	10.831	3040	3045	3046	rBV2	662	480	0.03%	0.004%
69	10.882	3056	3061	3063	rBV3	555	584	0.03%	0.004%
70	10.924	3066	3074	3077	rBV5	5547	7637	0.45%	0.057%
71	11.040	3105	3110	3115	rBV5	1120	1171	0.07%	0.009%
72	11.104	3128	3130	3134	rBV3	566	440	0.03%	0.003%
73	11.149	3134	3144	3153	rBV7	3575	6689	0.39%	0.050%
74	11.249	3164	3175	3196	rBV	831643	1295542	75.60%	9.602%
75	11.387	3214	3218	3223	rBV5	1308	1372	0.08%	0.010%
76	11.429	3227	3231	3245	rVB6	3953	6006	0.35%	0.045%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071221\
 Data File : VV021623.D
 Acq On : 12 Jul 2021 14:01
 Operator : SY/MD
 Sample : M2978-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7J1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
 Title : VOC Analysis

77	11.535	3257	3264	3265	rBV3	1175	962	0.06%	0.007%
78	11.554	3266	3270	3280	rVB7	1557	1859	0.11%	0.014%
79	11.625	3280	3292	3317	rBV	781063	1241540	72.45%	9.202%
80	11.792	3334	3344	3352	rVB	1526	2845	0.17%	0.021%
81	11.831	3353	3356	3358	rBV3	573	381	0.02%	0.003%
82	11.905	3374	3379	3381	rBV3	563	418	0.02%	0.003%
83	11.985	3401	3404	3406	rBV2	682	483	0.03%	0.004%
84	12.091	3433	3437	3438	rBV2	598	406	0.02%	0.003%
85	12.226	3472	3479	3481	rBV3	553	547	0.03%	0.004%
86	12.252	3481	3487	3494	rVV6	2336	3540	0.21%	0.026%
87	12.355	3509	3519	3531	rBV5	4430	7724	0.45%	0.057%
88	12.416	3535	3538	3541	rBV	643	358	0.02%	0.003%
89	12.500	3560	3564	3569	rVB5	458	467	0.03%	0.003%
90	12.593	3587	3593	3595	rBV4	820	846	0.05%	0.006%
91	12.686	3618	3622	3627	rVB3	511	480	0.03%	0.004%
92	12.799	3650	3657	3660	rBV4	1558	1880	0.11%	0.014%
93	13.004	3717	3721	3723	rBV2	618	482	0.03%	0.004%
94	13.165	3766	3771	3772	rBV3	473	451	0.03%	0.003%
95	13.268	3801	3803	3807	rVB2	539	318	0.02%	0.002%
96	13.287	3807	3809	3814	rBV	473	367	0.02%	0.003%
97	13.397	3840	3843	3847	rVB3	480	356	0.02%	0.003%
98	13.435	3849	3855	3858	rBV3	843	858	0.05%	0.006%
99	13.847	3978	3983	3986	rBV3	546	620	0.04%	0.005%
100	14.329	4131	4133	4136	rVB2	640	354	0.02%	0.003%




Sum of corrected areas: 13492292

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071221\
Data File : VV021623.D
Acq On : 12 Jul 2021 14:01
Operator : SY/MD
Sample : M2978-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7J1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

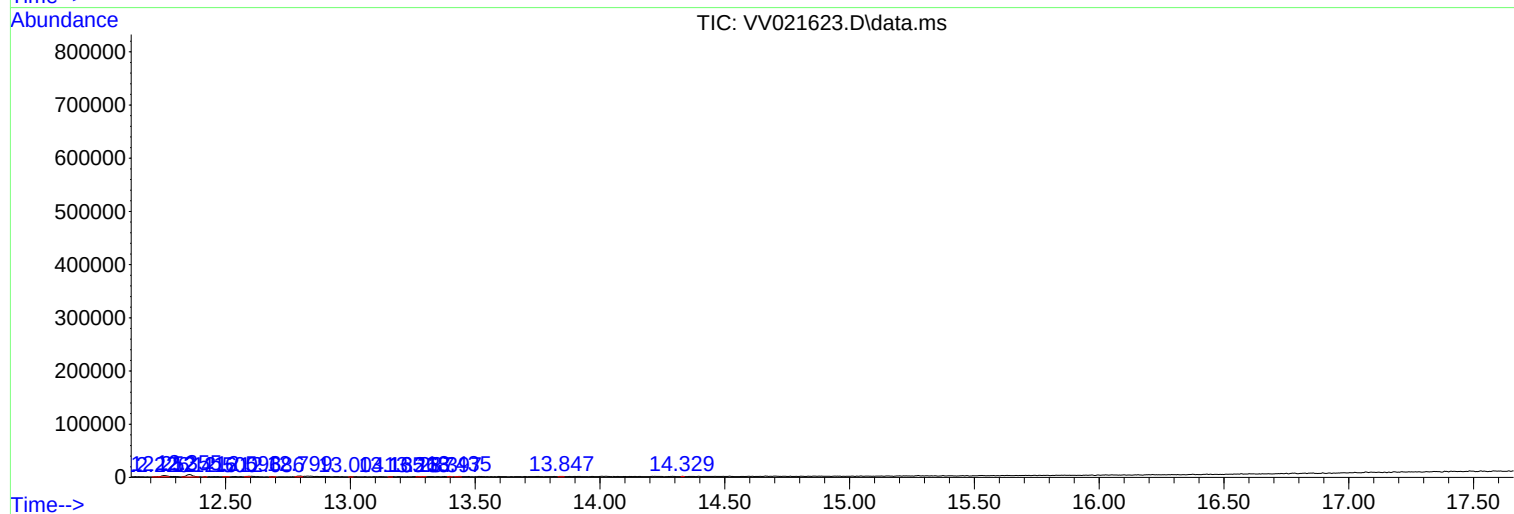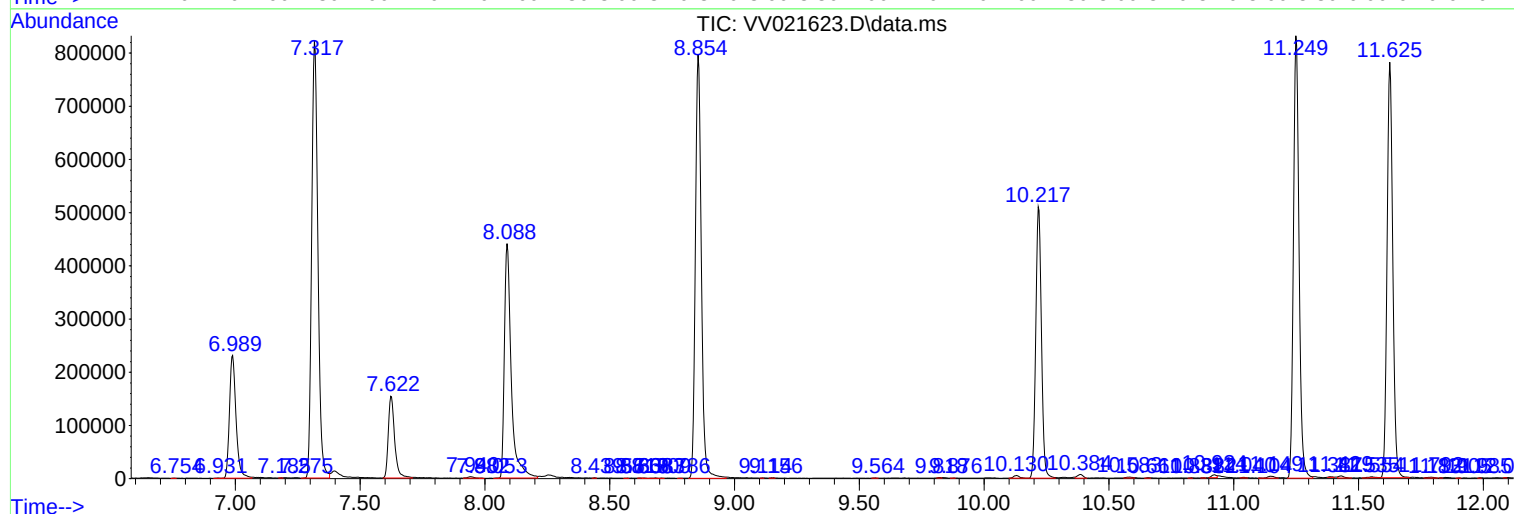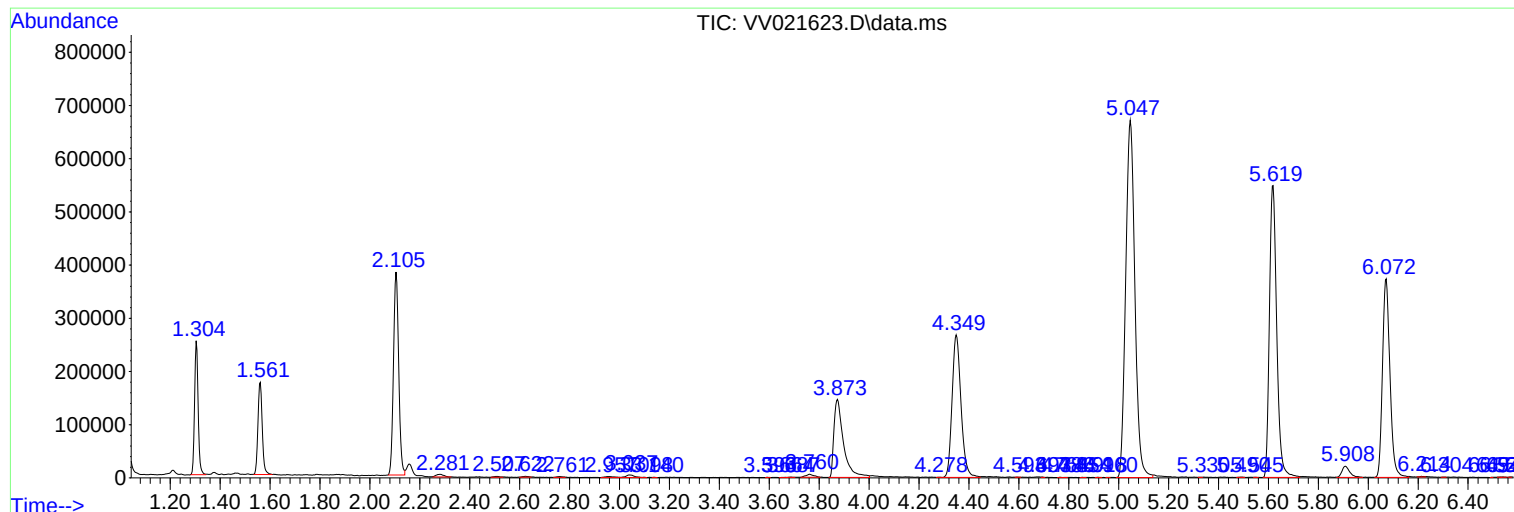

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071221\
Data File : VV021623.D
Acq On : 12 Jul 2021 14:01
Operator : SY/MD
Sample : M2978-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7J1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071221\
Data File : VV021623.D
Acq On : 12 Jul 2021 14:01
Operator : SY/MD
Sample : M2978-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7J1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
