

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071221\
 Data File : VV021624.D
 Acq On : 12 Jul 2021 14:25
 Operator : SY/MD
 Sample : M3008-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGE65

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M

Title : VOC Analysis

Signal : TIC: VV021624.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	97	rVB	268547	261598	14.67%	1.861%
2	1.561	154	162	179	rVB	187072	220758	12.38%	1.571%
3	2.105	322	331	344	rBV	395582	571220	32.03%	4.064%
4	2.587	479	481	483	rBV	487	246	0.01%	0.002%
5	2.870	567	569	571	rBV2	159	93	0.01%	0.001%
6	3.079	632	634	637	rVB2	660	347	0.02%	0.002%
7	3.230	679	681	684	rBV2	283	117	0.01%	0.001%
8	3.320	707	709	711	rVB	223	75	0.00%	0.001%
9	3.343	711	716	719	rBV2	278	264	0.01%	0.002%
10	3.404	733	735	736	rBV	199	96	0.01%	0.001%
11	3.449	746	749	751	rBV2	323	162	0.01%	0.001%
12	3.471	755	756	759	rVV	292	136	0.01%	0.001%
13	3.497	763	764	765	rBV	280	85	0.00%	0.001%
14	3.523	769	772	774	rBV4	249	120	0.01%	0.001%
15	3.616	798	801	802	rBV	209	127	0.01%	0.001%
16	3.699	822	827	831	rBV4	390	523	0.03%	0.004%
17	3.738	837	839	842	rBV2	292	193	0.01%	0.001%
18	3.777	848	851	853	rVB2	206	88	0.00%	0.001%
19	3.796	853	857	859	rBV2	354	289	0.02%	0.002%
20	3.825	863	866	869	rBV2	279	188	0.01%	0.001%
21	3.873	871	881	929	rBV	151970	417094	23.39%	2.967%
22	4.278	1004	1007	1009	rBV2	434	281	0.02%	0.002%
23	4.355	1013	1031	1068	rVV3	331387	1106109	62.02%	7.869%
24	4.635	1116	1118	1120	rBV2	327	128	0.01%	0.001%
25	4.671	1125	1129	1131	rBV2	437	322	0.02%	0.002%
26	4.754	1151	1155	1157	rVB2	395	245	0.01%	0.002%
27	4.783	1157	1164	1165	rBV3	361	285	0.02%	0.002%
28	4.841	1180	1182	1186	rVB	318	224	0.01%	0.002%
29	4.860	1186	1188	1190	rBV2	580	309	0.02%	0.002%
30	4.886	1194	1196	1200	rVV3	253	139	0.01%	0.001%
31	4.934	1205	1211	1216	rBV5	444	478	0.03%	0.003%
32	4.960	1216	1219	1223	rBV2	377	322	0.02%	0.002%
33	5.047	1229	1246	1277	rBV2	702319	1783481	100.00%	12.689%
34	5.285	1318	1320	1322	rBV2	518	221	0.01%	0.002%
35	5.371	1344	1347	1351	rBV2	560	469	0.03%	0.003%
36	5.407	1355	1358	1359	rBV	680	348	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW071221\
 Data File : VW021624.D
 Acq On : 12 Jul 2021 14:25
 Operator : SY/MD
 Sample : M3008-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGE65

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
 Title : VOC Analysis

37	5.478	1377	1380	1382	rBV3	211	87	0.00%	0.001%
38	5.497	1382	1386	1387	rBV3	592	386	0.02%	0.003%
39	5.619	1411	1424	1454	rBV	507683	1035316	58.05%	7.366%
40	5.815	1483	1485	1491	rVB2	714	503	0.03%	0.004%
41	5.841	1491	1493	1496	rBV3	692	318	0.02%	0.002%
42	5.912	1504	1515	1530	rBV3	11895	25524	1.43%	0.182%
43	5.995	1539	1541	1542	rBV3	187	55	0.00%	0.000%
44	6.018	1546	1548	1549	rBV	302	148	0.01%	0.001%
45	6.072	1550	1565	1597	rBV	389513	801887	44.96%	5.705%
46	6.391	1662	1664	1669	rVB4	660	477	0.03%	0.003%
47	6.429	1674	1676	1677	rBV2	318	152	0.01%	0.001%
48	6.465	1686	1687	1689	rVB2	156	55	0.00%	0.000%
49	6.516	1689	1703	1721	rBV	44047	86975	4.88%	0.619%
50	6.635	1736	1740	1742	rBV3	769	711	0.04%	0.005%
51	6.722	1766	1767	1771	rBV2	346	184	0.01%	0.001%
52	6.754	1775	1777	1780	rBV2	245	115	0.01%	0.001%
53	6.773	1781	1783	1785	rBV2	181	72	0.00%	0.001%
54	6.802	1790	1792	1798	rBV2	313	190	0.01%	0.001%
55	6.841	1802	1804	1807	rVB3	188	114	0.01%	0.001%
56	6.860	1807	1810	1812	rVB2	195	104	0.01%	0.001%
57	6.924	1828	1830	1833	rBV2	150	50	0.00%	0.000%
58	6.944	1833	1836	1839	rVB2	409	258	0.01%	0.002%
59	6.989	1839	1850	1887	rBV	243550	445181	24.96%	3.167%
60	7.317	1940	1952	1970	rBV	871331	1490230	83.56%	10.602%
61	7.622	2037	2047	2076	rBV	164846	287711	16.13%	2.047%
62	7.850	2116	2118	2123	rVB3	746	584	0.03%	0.004%
63	7.879	2123	2127	2130	rVB2	274	141	0.01%	0.001%
64	7.895	2130	2132	2136	rBV	334	190	0.01%	0.001%
65	7.937	2140	2145	2148	rBV4	2127	2281	0.13%	0.016%
66	8.002	2163	2165	2168	rBV2	363	209	0.01%	0.001%
67	8.031	2168	2174	2178	rBV4	610	797	0.04%	0.006%
68	8.088	2182	2192	2230	rBV	483104	881285	49.41%	6.270%
69	8.551	2332	2336	2338	rBV3	366	247	0.01%	0.002%
70	8.606	2350	2353	2354	rBV2	340	166	0.01%	0.001%
71	8.667	2370	2372	2376	rVB3	323	193	0.01%	0.001%
72	8.728	2389	2391	2393	rBV3	282	183	0.01%	0.001%
73	8.741	2393	2395	2398	rVV2	364	201	0.01%	0.001%
74	8.773	2403	2405	2407	rBV	410	200	0.01%	0.001%
75	8.854	2419	2430	2465	rBV	741368	1227808	68.84%	8.735%
76	9.265	2553	2558	2559	rBV2	326	258	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071221\
 Data File : VV021624.D
 Acq On : 12 Jul 2021 14:25
 Operator : SY/MD
 Sample : M3008-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGE65

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
 Title : VOC Analysis

77	9.326	2575	2577	2582	rVB3	540	285	0.02%	0.002%
78	9.346	2582	2583	2584	rVB3	321	62	0.00%	0.000%
79	9.448	2613	2615	2616	rBV3	230	76	0.00%	0.001%
80	9.741	2699	2706	2713	rVB6	1241	1794	0.10%	0.013%
81	9.776	2713	2717	2721	rBV2	509	508	0.03%	0.004%
82	9.892	2749	2753	2758	rBV3	664	663	0.04%	0.005%
83	9.995	2783	2785	2788	rBV2	377	287	0.02%	0.002%
84	10.127	2820	2826	2836	rVB3	5704	9052	0.51%	0.064%
85	10.217	2842	2854	2879	rBV	552536	864913	48.50%	6.153%
86	10.432	2916	2921	2923	rBV3	514	502	0.03%	0.004%
87	10.548	2952	2957	2959	rBV4	768	676	0.04%	0.005%
88	11.037	3102	3109	3110	rBV	1287	1170	0.07%	0.008%
89	11.249	3164	3175	3194	rBV	778371	1213055	68.02%	8.630%
90	11.625	3281	3292	3318	rVB	817403	1302632	73.04%	9.268%
91	12.468	3553	3554	3558	rBV2	610	350	0.02%	0.002%
92	12.590	3590	3592	3593	rBV2	812	407	0.02%	0.003%
93	13.169	3770	3772	3774	rBV2	506	218	0.01%	0.002%
94	13.252	3796	3798	3802	rBV2	599	389	0.02%	0.003%


Sum of corrected areas: 14055765

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071221\
Data File : VV021624.D
Acq On : 12 Jul 2021 14:25
Operator : SY/MD
Sample : M3008-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGE65

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

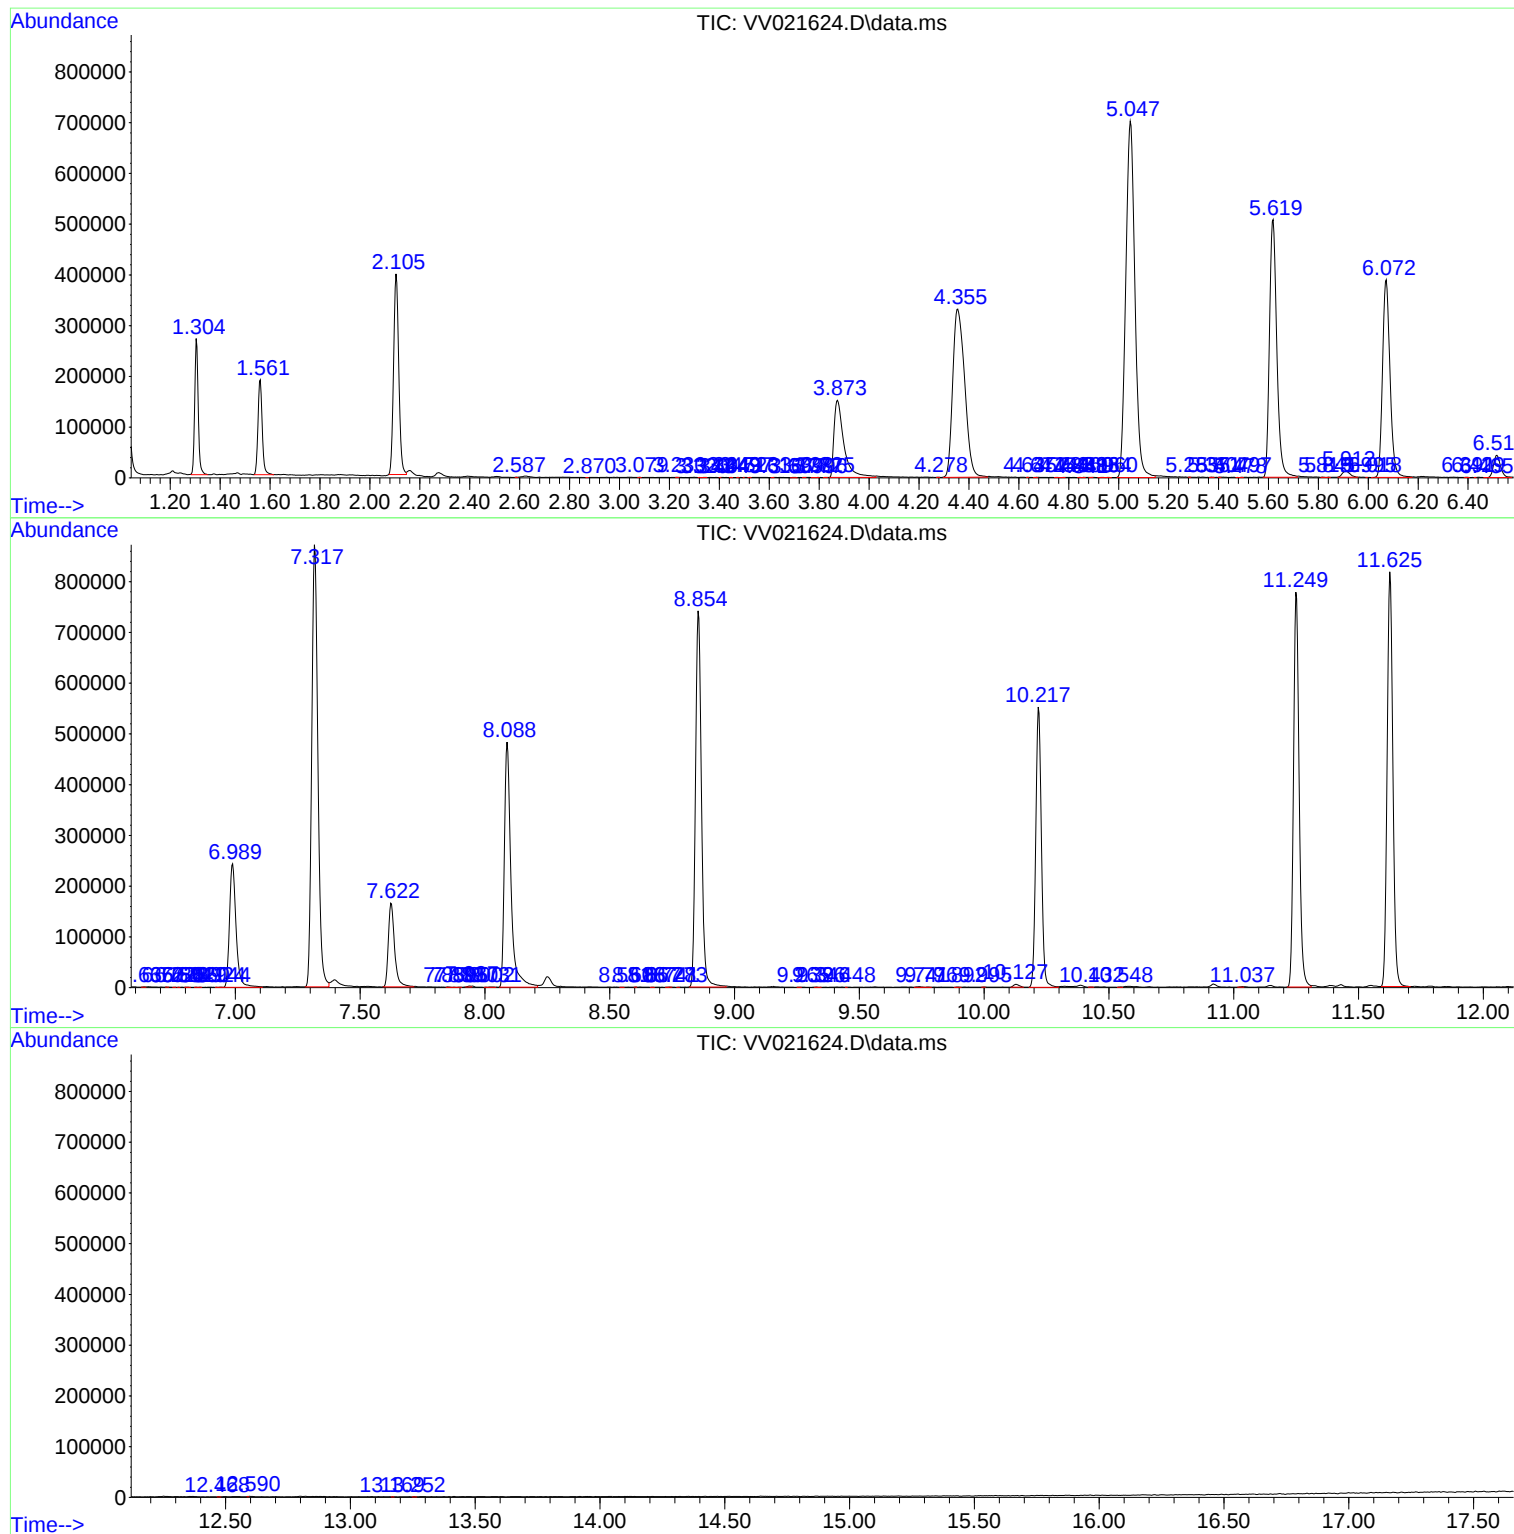

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071221\
Data File : VV021624.D
Acq On : 12 Jul 2021 14:25
Operator : SY/MD
Sample : M3008-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGE65

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071221\
Data File : VV021624.D
Acq On : 12 Jul 2021 14:25
Operator : SY/MD
Sample : M3008-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGE65

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
