

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071221\
 Data File : VV021626.D
 Acq On : 12 Jul 2021 15:13
 Operator : SY/MD
 Sample : M3008-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGE69

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M

Title : VOC Analysis

Signal : TIC: VV021626.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	98	rVB	254081	248953	14.50%	1.840%
2	1.561	154	162	175	rBV	177370	210153	12.24%	1.553%
3	2.104	321	331	344	rBV	377885	551112	32.10%	4.073%
4	2.503	450	455	465	rVB5	2039	3500	0.20%	0.026%
5	2.612	486	489	498	rBV3	932	1279	0.07%	0.009%
6	2.658	501	503	505	rVB2	387	129	0.01%	0.001%
7	2.828	553	556	557	rBV2	410	194	0.01%	0.001%
8	2.844	557	561	566	rVV3	727	615	0.04%	0.005%
9	2.895	575	577	579	rBV	593	306	0.02%	0.002%
10	2.995	605	608	610	rBV2	276	199	0.01%	0.001%
11	3.005	610	611	615	rVV	345	165	0.01%	0.001%
12	3.095	636	639	643	rVB2	502	403	0.02%	0.003%
13	3.133	646	651	652	rBV2	504	301	0.02%	0.002%
14	3.185	665	667	669	rBV	344	149	0.01%	0.001%
15	3.198	669	671	675	rVV2	431	201	0.01%	0.001%
16	3.368	722	724	725	rBV	502	248	0.01%	0.002%
17	3.403	732	735	737	rBV3	261	158	0.01%	0.001%
18	3.503	763	766	769	rBV	393	220	0.01%	0.002%
19	3.522	769	772	777	rBV3	378	325	0.02%	0.002%
20	3.622	798	803	805	rBV2	531	401	0.02%	0.003%
21	3.683	819	822	829	rBV3	410	337	0.02%	0.002%
22	3.747	840	842	845	rBV2	505	254	0.01%	0.002%
23	3.873	871	881	922	rBV	148014	393763	22.94%	2.910%
24	4.349	1014	1029	1059	rBV	263629	653420	38.06%	4.829%
25	4.616	1109	1112	1114	rBV3	500	297	0.02%	0.002%
26	4.699	1135	1138	1146	rBV5	552	576	0.03%	0.004%
27	4.735	1146	1149	1151	rBV3	298	192	0.01%	0.001%
28	4.960	1217	1219	1222	rVB2	369	165	0.01%	0.001%
29	5.046	1228	1246	1283	rBV2	669819	1716692	100.00%	12.687%
30	5.619	1411	1424	1453	rBV	542484	1092705	63.65%	8.075%
31	5.799	1478	1480	1485	rVB2	553	400	0.02%	0.003%
32	5.915	1504	1516	1528	rBV3	10845	22943	1.34%	0.170%
33	6.011	1543	1546	1549	rBV3	323	237	0.01%	0.002%
34	6.072	1550	1565	1593	rVV	372540	764407	44.53%	5.649%
35	6.384	1660	1662	1667	rBV3	795	439	0.03%	0.003%
36	6.403	1667	1668	1671	rVB2	425	162	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071221\
 Data File : VV021626.D
 Acq On : 12 Jul 2021 15:13
 Operator : SY/MD
 Sample : M3008-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGE69

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
 Title : VOC Analysis

37	6.423	1671	1674	1676	rBV	587	375	0.02%	0.003%
38	6.506	1698	1700	1702	rBV	435	202	0.01%	0.001%
39	6.522	1703	1705	1706	rVV	339	131	0.01%	0.001%
40	6.538	1707	1710	1713	rVB2	650	398	0.02%	0.003%
41	6.641	1734	1742	1743	rBV5	779	868	0.05%	0.006%
42	6.715	1763	1765	1768	rVB2	332	181	0.01%	0.001%
43	6.731	1768	1770	1775	rVB3	417	248	0.01%	0.002%
44	6.760	1775	1779	1780	rBV2	429	259	0.02%	0.002%
45	6.805	1791	1793	1796	rBV2	248	143	0.01%	0.001%
46	6.818	1796	1797	1802	rVB3	693	407	0.02%	0.003%
47	6.850	1802	1807	1811	rBV3	377	322	0.02%	0.002%
48	6.908	1822	1825	1826	rBV	405	179	0.01%	0.001%
49	6.931	1829	1832	1833	rBV	217	132	0.01%	0.001%
50	6.989	1838	1850	1875	rBV	234049	423109	24.65%	3.127%
51	7.316	1940	1952	1969	rBV	813568	1424542	82.98%	10.528%
52	7.625	2037	2048	2073	rBV	155893	275975	16.08%	2.040%
53	7.786	2096	2098	2100	rVB2	756	295	0.02%	0.002%
54	7.853	2117	2119	2123	rVB2	525	372	0.02%	0.003%
55	7.947	2139	2148	2154	rVV3	1922	3358	0.20%	0.025%
56	8.088	2174	2192	2237	rBV	483224	867093	50.51%	6.408%
57	8.500	2318	2320	2323	rBV2	286	153	0.01%	0.001%
58	8.535	2329	2331	2334	rBV3	542	377	0.02%	0.003%
59	8.625	2356	2359	2362	rBV2	451	336	0.02%	0.002%
60	8.660	2366	2370	2375	rBV3	480	559	0.03%	0.004%
61	8.709	2382	2385	2386	rBV2	288	135	0.01%	0.001%
62	8.770	2400	2404	2406	rBV2	309	254	0.01%	0.002%
63	8.799	2411	2413	2416	rBV	403	264	0.02%	0.002%
64	8.853	2417	2430	2460	rBV	802188	1306187	76.09%	9.653%
65	9.143	2511	2520	2533	rBV2	21711	37498	2.18%	0.277%
66	9.236	2546	2549	2555	rVB3	553	432	0.03%	0.003%
67	9.271	2558	2560	2561	rBV	495	250	0.01%	0.002%
68	9.326	2575	2577	2580	rVB2	326	156	0.01%	0.001%
69	9.377	2591	2593	2595	rBV	535	275	0.02%	0.002%
70	9.423	2605	2607	2613	rVB3	368	264	0.02%	0.002%
71	9.480	2620	2625	2627	rBV	451	411	0.02%	0.003%
72	9.551	2638	2647	2659	rBV2	14006	22115	1.29%	0.163%
73	9.622	2665	2669	2673	rBV2	472	461	0.03%	0.003%
74	9.734	2699	2704	2705	rBV2	277	158	0.01%	0.001%
75	9.747	2706	2708	2711	rVB2	481	256	0.01%	0.002%
76	9.767	2711	2714	2718	rBV2	454	345	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071221\
 Data File : VV021626.D
 Acq On : 12 Jul 2021 15:13
 Operator : SY/MD
 Sample : M3008-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGE69

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
 Title : VOC Analysis

77	9.879	2747	2749	2751	rVB	423	190	0.01%	0.001%
78	9.924	2760	2763	2764	rBV	428	225	0.01%	0.002%
79	10.056	2801	2804	2810	rBV	341	358	0.02%	0.003%
80	10.130	2816	2827	2838	rVB3	5506	9068	0.53%	0.067%
81	10.217	2840	2854	2878	rBV	526498	838219	48.83%	6.195%
82	10.451	2914	2927	2944	rBV	11852	26982	1.57%	0.199%
83	10.545	2950	2956	2966	rBV2	4945	7441	0.43%	0.055%
84	10.744	3009	3018	3029	rBV2	6404	10585	0.62%	0.078%
85	10.812	3037	3039	3041	rBV2	341	199	0.01%	0.001%
86	10.853	3049	3052	3054	rBV3	630	458	0.03%	0.003%
87	10.918	3064	3072	3087	rVB2	31741	50035	2.91%	0.370%
88	11.004	3097	3099	3102	rBV3	495	289	0.02%	0.002%
89	11.146	3134	3143	3151	rBV5	3204	5359	0.31%	0.040%
90	11.249	3164	3175	3194	rBV	808754	1275797	74.32%	9.429%
91	11.532	3257	3263	3273	rBV2	6187	9486	0.55%	0.070%
92	11.625	3281	3292	3317	rVB	780823	1244929	72.52%	9.200%
93	12.075	3430	3432	3434	rBV	552	202	0.01%	0.001%
94	12.091	3434	3437	3440	rBV4	1017	919	0.05%	0.007%
95	12.419	3535	3539	3544	rVB2	1854	1683	0.10%	0.012%
96	12.467	3551	3554	3569	rVB6	2641	3700	0.22%	0.027%
97	12.885	3680	3684	3697	rVB5	4039	4981	0.29%	0.037%
98	13.149	3763	3766	3767	rBV	412	248	0.01%	0.002%
99	13.393	3840	3842	3844	rBV	504	243	0.01%	0.002%
100	13.522	3874	3882	3887	rBV5	2925	4122	0.24%	0.030%




Sum of corrected areas: 13531193

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071221\
Data File : VV021626.D
Acq On : 12 Jul 2021 15:13
Operator : SY/MD
Sample : M3008-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGE69

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

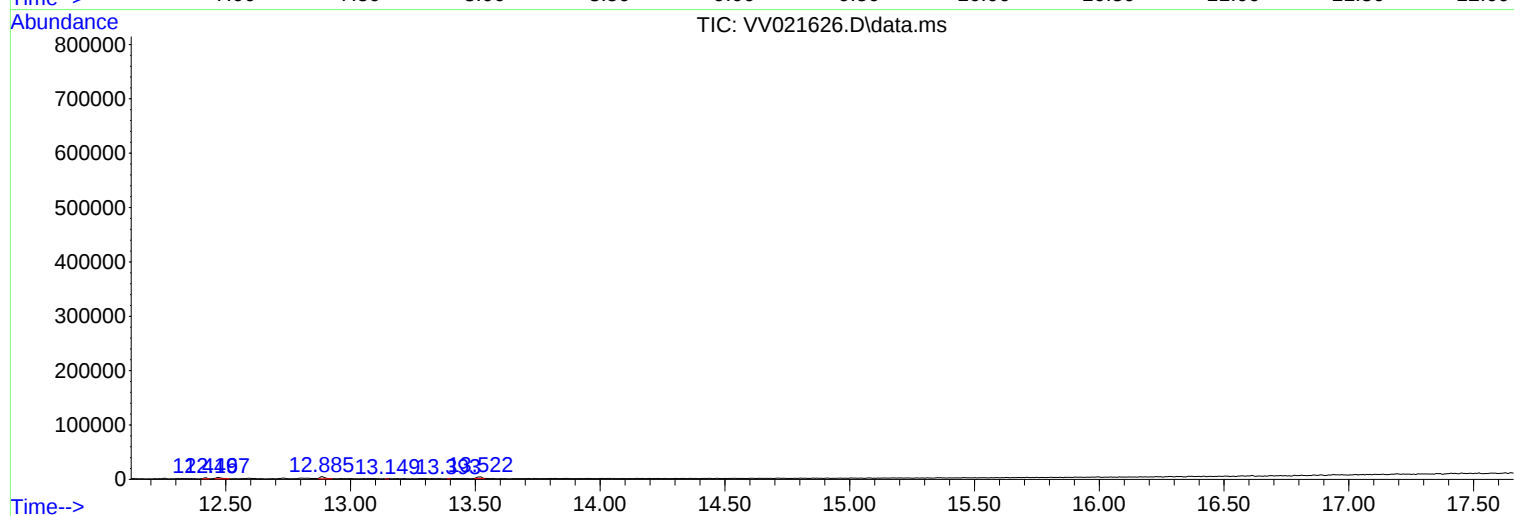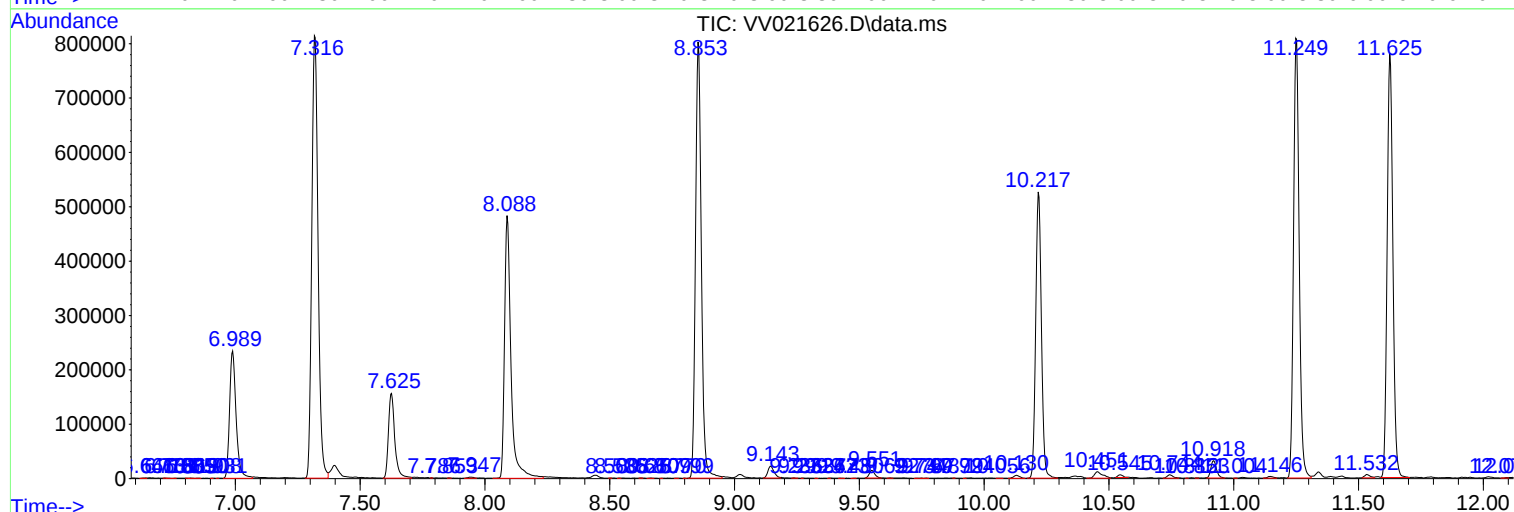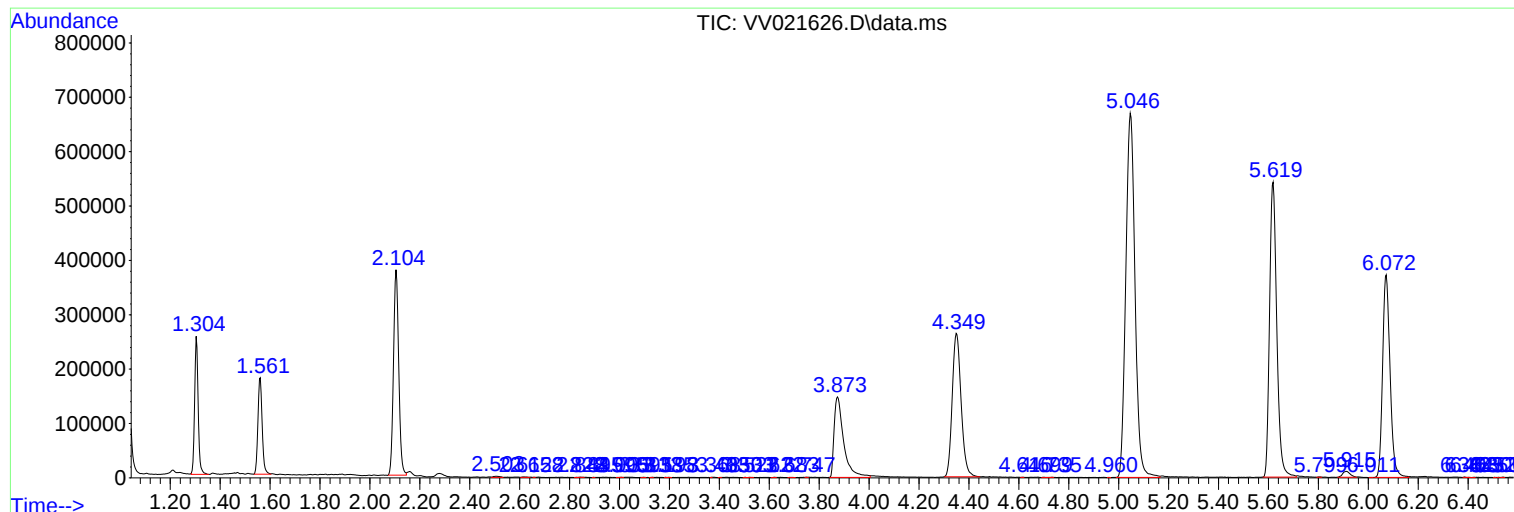

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071221\
Data File : VV021626.D
Acq On : 12 Jul 2021 15:13
Operator : SY/MD
Sample : M3008-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGE69

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071221\
Data File : VV021626.D
Acq On : 12 Jul 2021 15:13
Operator : SY/MD
Sample : M3008-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGE69

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
