

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071221\
 Data File : VV021627.D
 Acq On : 12 Jul 2021 15:37
 Operator : SY/MD
 Sample : M3008-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGE70

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M

Title : VOC Analysis

Signal : TIC: VV021627.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	97	rVB	250754	250718	14.33%	1.842%
2	1.561	155	162	176	rVB	184301	208601	11.93%	1.533%
3	2.105	321	331	344	rBV	389131	567729	32.46%	4.171%
4	2.503	447	455	464	rBV6	2389	3932	0.22%	0.029%
5	2.693	510	514	518	rBV3	539	419	0.02%	0.003%
6	2.780	539	541	545	rVB2	390	263	0.02%	0.002%
7	2.812	545	551	552	rBV2	475	408	0.02%	0.003%
8	2.886	572	574	578	rBV2	319	249	0.01%	0.002%
9	2.944	590	592	595	rBV3	575	355	0.02%	0.003%
10	3.040	620	622	626	rVB3	494	264	0.02%	0.002%
11	3.085	633	636	641	rBV2	524	423	0.02%	0.003%
12	3.188	663	668	671	rVV3	435	408	0.02%	0.003%
13	3.266	690	692	697	rVB3	220	134	0.01%	0.001%
14	3.439	743	746	749	rBV2	391	232	0.01%	0.002%
15	3.577	785	789	794	rBV3	515	324	0.02%	0.002%
16	3.603	794	797	798	rBV	437	213	0.01%	0.002%
17	3.655	809	813	816	rBV2	423	225	0.01%	0.002%
18	3.693	820	825	834	rVB3	463	579	0.03%	0.004%
19	3.748	838	842	844	rBV2	427	383	0.02%	0.003%
20	3.783	851	853	855	rBV2	263	147	0.01%	0.001%
21	3.873	871	881	912	rBV	153884	395683	22.62%	2.907%
22	4.349	1011	1029	1058	rBV	271564	677009	38.70%	4.974%
23	4.722	1141	1145	1149	rBV2	329	249	0.01%	0.002%
24	4.745	1149	1152	1156	rVB2	371	270	0.02%	0.002%
25	4.818	1172	1175	1181	rVB3	392	383	0.02%	0.003%
26	4.854	1181	1186	1192	rBB4	310	396	0.02%	0.003%
27	4.912	1197	1204	1207	rBV3	403	460	0.03%	0.003%
28	4.928	1207	1209	1212	rVB3	562	332	0.02%	0.002%
29	4.947	1212	1215	1217	rBV	245	137	0.01%	0.001%
30	5.047	1227	1246	1278	rBV2	683912	1749230	100.00%	12.852%
31	5.394	1352	1354	1356	rBV	428	177	0.01%	0.001%
32	5.462	1373	1375	1376	rBV	404	147	0.01%	0.001%
33	5.616	1411	1423	1456	rBV	531556	1073042	61.34%	7.884%
34	5.912	1505	1515	1532	rVB4	9132	19683	1.13%	0.145%
35	6.072	1550	1565	1591	rBV	385255	781860	44.70%	5.745%
36	6.326	1642	1644	1647	rVB4	414	225	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071221\
 Data File : VV021627.D
 Acq On : 12 Jul 2021 15:37
 Operator : SY/MD
 Sample : M3008-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGE70

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
 Title : VOC Analysis

37	6.378	1654	1660	1665	rBV4	474	465	0.03%	0.003%
38	6.404	1665	1668	1671	rBV2	321	247	0.01%	0.002%
39	6.420	1671	1673	1676	rVV3	507	308	0.02%	0.002%
40	6.433	1676	1677	1680	rVB2	369	130	0.01%	0.001%
41	6.455	1683	1684	1687	rBV	223	123	0.01%	0.001%
42	6.629	1733	1738	1739	rBV2	699	482	0.03%	0.004%
43	6.645	1741	1743	1746	rVV3	732	458	0.03%	0.003%
44	6.741	1771	1773	1776	rVB3	443	221	0.01%	0.002%
45	6.757	1776	1778	1781	rBV2	352	214	0.01%	0.002%
46	6.815	1792	1796	1800	rVV2	302	246	0.01%	0.002%
47	6.876	1810	1815	1817	rBV	367	254	0.01%	0.002%
48	6.989	1837	1850	1878	rBV	235645	431779	24.68%	3.172%
49	7.317	1939	1952	1969	rBV	835929	1452957	83.06%	10.676%
50	7.622	2035	2047	2073	rBV	159200	280032	16.01%	2.058%
51	7.941	2139	2146	2147	rBV2	2067	1958	0.11%	0.014%
52	7.992	2159	2162	2163	rBV	471	233	0.01%	0.002%
53	8.047	2177	2179	2181	rVB	389	171	0.01%	0.001%
54	8.088	2181	2192	2226	rBV	490673	879402	50.27%	6.461%
55	8.420	2294	2295	2296	rBV	680	255	0.01%	0.002%
56	8.442	2299	2302	2309	rVB	11106	8953	0.51%	0.066%
57	8.561	2337	2339	2341	rVB2	299	127	0.01%	0.001%
58	8.574	2341	2343	2348	rBV2	330	287	0.02%	0.002%
59	8.632	2359	2361	2367	rBV2	411	382	0.02%	0.003%
60	8.760	2399	2401	2405	rVB4	524	369	0.02%	0.003%
61	8.780	2405	2407	2408	rBV	331	127	0.01%	0.001%
62	8.854	2418	2430	2453	rBV	787444	1276026	72.95%	9.376%
63	9.146	2509	2521	2531	rBV2	11598	20978	1.20%	0.154%
64	9.240	2548	2550	2553	rVB2	396	178	0.01%	0.001%
65	9.275	2553	2561	2563	rBV3	425	457	0.03%	0.003%
66	9.323	2574	2576	2580	rVB	294	187	0.01%	0.001%
67	9.346	2580	2583	2587	rBV2	387	269	0.02%	0.002%
68	9.378	2591	2593	2594	rBV	326	168	0.01%	0.001%
69	9.503	2628	2632	2635	rVB3	484	306	0.02%	0.002%
70	9.551	2635	2647	2656	rBV3	7749	12540	0.72%	0.092%
71	9.619	2664	2668	2669	rBV	477	282	0.02%	0.002%
72	9.645	2674	2676	2678	rBV	374	157	0.01%	0.001%
73	9.661	2678	2681	2685	rBV2	446	369	0.02%	0.003%
74	9.680	2685	2687	2689	rBV3	426	218	0.01%	0.002%
75	9.712	2694	2697	2699	rBV	341	174	0.01%	0.001%
76	9.738	2699	2705	2710	rVB4	421	411	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071221\
 Data File : VV021627.D
 Acq On : 12 Jul 2021 15:37
 Operator : SY/MD
 Sample : M3008-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGE70

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
 Title : VOC Analysis

77	9.818	2724	2730	2732	rBV2	305	305	0.02%	0.002%
78	9.870	2744	2746	2747	rBV2	294	140	0.01%	0.001%
79	9.905	2755	2757	2760	rVB2	336	155	0.01%	0.001%
80	9.921	2760	2762	2763	rBV2	325	137	0.01%	0.001%
81	10.127	2818	2826	2838	rVB5	4817	7910	0.45%	0.058%
82	10.217	2841	2854	2876	rBV	550205	862696	49.32%	6.339%
83	10.452	2919	2927	2942	rBV2	8247	17935	1.03%	0.132%
84	10.744	3009	3018	3027	rBV3	4242	7382	0.42%	0.054%
85	10.828	3039	3044	3046	rBV3	768	684	0.04%	0.005%
86	10.918	3063	3072	3090	rVB2	26067	42379	2.42%	0.311%
87	11.114	3131	3133	3136	rBV3	366	183	0.01%	0.001%
88	11.149	3136	3144	3152	rVV6	3270	5165	0.30%	0.038%
89	11.249	3163	3175	3196	rBV	800637	1252022	71.58%	9.199%
90	11.474	3244	3245	3248	rVB	486	187	0.01%	0.001%
91	11.535	3258	3264	3273	rBV5	3726	5715	0.33%	0.042%
92	11.625	3280	3292	3314	rVB	829698	1283572	73.38%	9.431%
93	11.908	3377	3380	3381	rBV	922	449	0.03%	0.003%
94	12.021	3410	3415	3422	rVB6	2323	2953	0.17%	0.022%
95	12.185	3463	3466	3470	rBV3	554	441	0.03%	0.003%
96	12.413	3530	3537	3546	rBV6	2288	3723	0.21%	0.027%
97	12.780	3649	3651	3652	rBV	682	350	0.02%	0.003%
98	12.889	3679	3685	3694	rVB6	4519	6593	0.38%	0.048%
99	12.982	3712	3714	3717	rBV2	356	222	0.01%	0.002%
100	13.307	3811	3815	3818	rBV3	731	681	0.04%	0.005%




Sum of corrected areas: 13610168

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071221\
Data File : VV021627.D
Acq On : 12 Jul 2021 15:37
Operator : SY/MD
Sample : M3008-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGE70

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

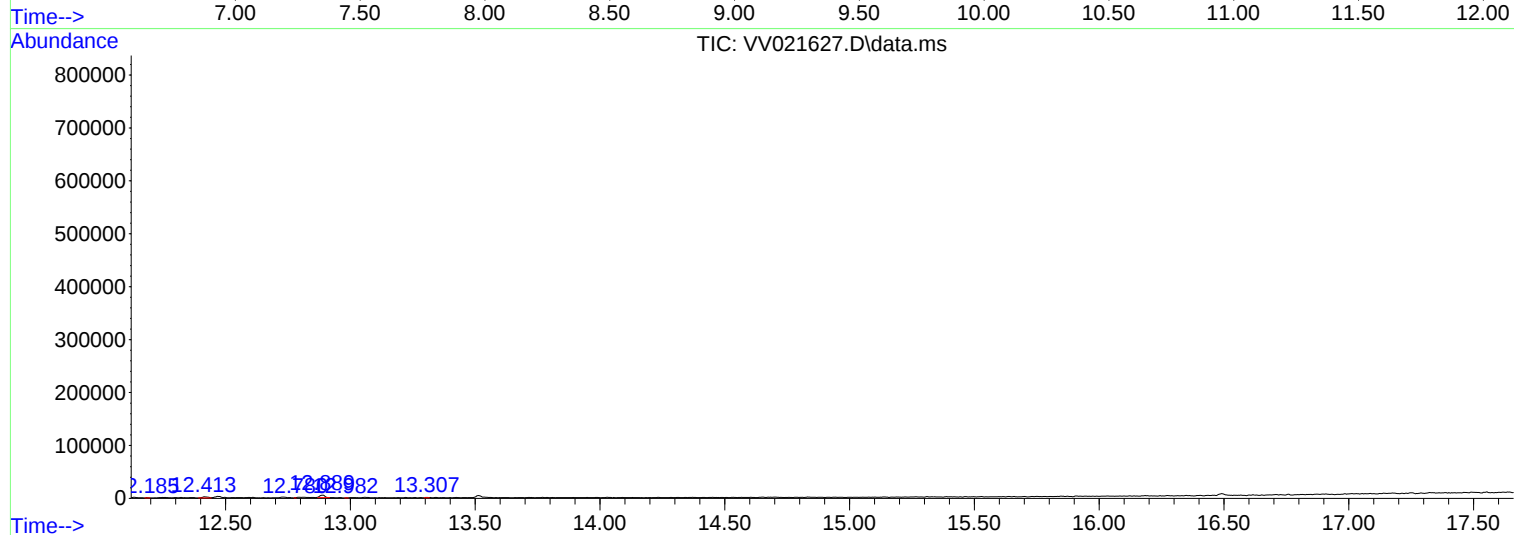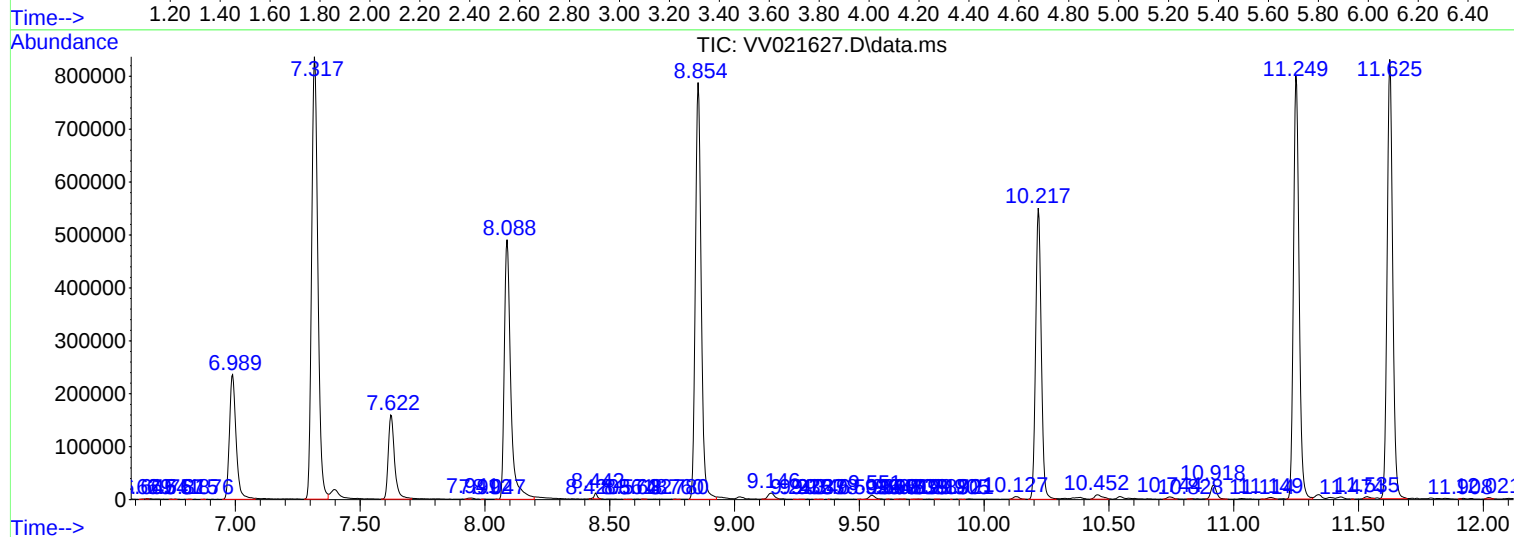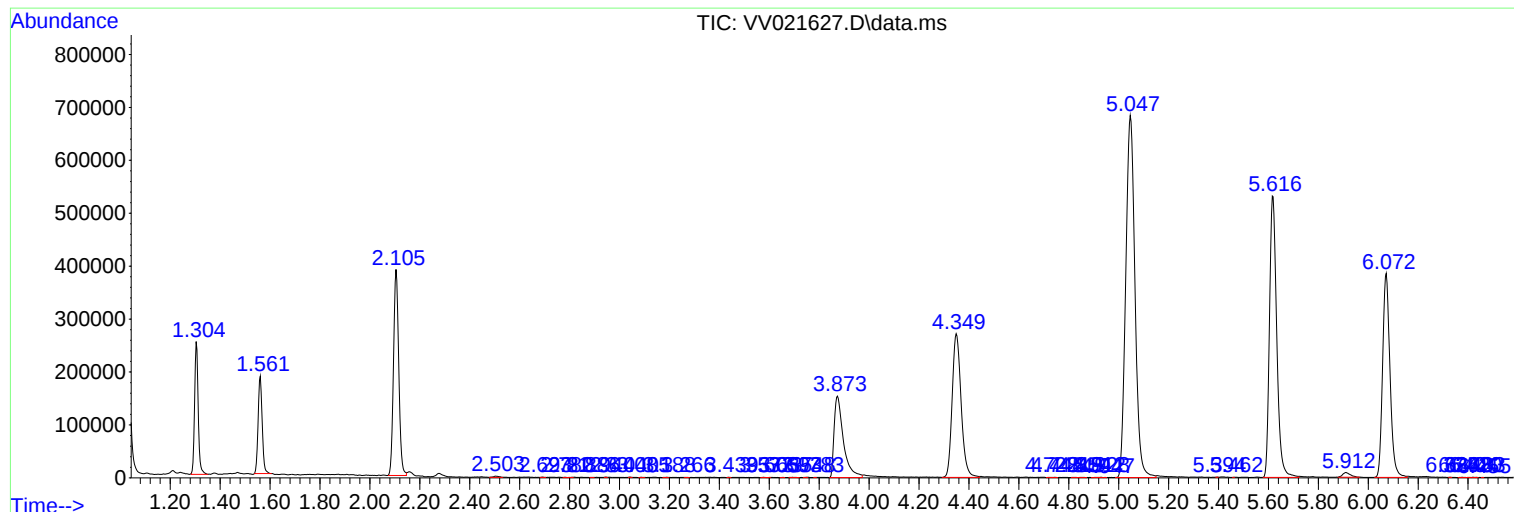

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071221\
Data File : VV021627.D
Acq On : 12 Jul 2021 15:37
Operator : SY/MD
Sample : M3008-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGE70

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071221\
Data File : VV021627.D
Acq On : 12 Jul 2021 15:37
Operator : SY/MD
Sample : M3008-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGE70

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
