

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071221\
 Data File : VV021628.D
 Acq On : 12 Jul 2021 16:01
 Operator : SY/MD
 Sample : M3008-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGE71

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M

Title : VOC Analysis

Signal : TIC: VV021628.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	97	rBV	246610	244985	14.44%	1.849%
2	1.558	154	161	182	rVB	181016	213298	12.57%	1.610%
3	2.105	321	331	344	rBV	372930	543551	32.03%	4.102%
4	2.497	450	453	454	rBV2	1267	676	0.04%	0.005%
5	2.754	530	533	537	rBV4	631	458	0.03%	0.003%
6	2.796	543	546	549	rBV4	547	294	0.02%	0.002%
7	2.857	562	565	566	rBV	369	222	0.01%	0.002%
8	2.915	581	583	587	rBV2	388	251	0.01%	0.002%
9	2.953	590	595	600	rVB4	621	618	0.04%	0.005%
10	2.976	600	602	606	rBV2	596	458	0.03%	0.003%
11	2.992	606	607	612	rBV2	294	240	0.01%	0.002%
12	3.095	635	639	643	rBV2	471	416	0.02%	0.003%
13	3.121	643	647	648	rBV2	274	159	0.01%	0.001%
14	3.256	685	689	692	rBV3	438	414	0.02%	0.003%
15	3.384	722	729	731	rBV2	384	381	0.02%	0.003%
16	3.461	750	753	755	rBV	250	111	0.01%	0.001%
17	3.474	755	757	760	rBV	277	147	0.01%	0.001%
18	3.494	760	763	766	rVB2	309	185	0.01%	0.001%
19	3.519	767	771	772	rBV	360	182	0.01%	0.001%
20	3.613	798	800	801	rBV	258	85	0.01%	0.001%
21	3.629	803	805	808	rVB	362	182	0.01%	0.001%
22	3.648	808	811	813	rBV	184	151	0.01%	0.001%
23	3.674	817	819	824	rVB	251	179	0.01%	0.001%
24	3.706	825	829	831	rBV2	195	147	0.01%	0.001%
25	3.767	846	848	849	rVB2	280	80	0.00%	0.001%
26	3.780	849	852	854	rVV2	238	102	0.01%	0.001%
27	3.806	857	860	863	rBV2	445	289	0.02%	0.002%
28	3.873	871	881	917	rBV	143104	377712	22.26%	2.850%
29	4.349	1013	1029	1054	rBV	262435	652495	38.45%	4.924%
30	4.735	1147	1149	1152	rBV2	239	150	0.01%	0.001%
31	4.757	1154	1156	1158	rBV2	253	132	0.01%	0.001%
32	4.809	1170	1172	1175	rBV2	103	61	0.00%	0.000%
33	4.822	1175	1176	1177	rBV	311	80	0.00%	0.001%
34	4.847	1183	1184	1186	rBV	261	121	0.01%	0.001%
35	5.047	1228	1246	1282	rBV2	663758	1697125	100.00%	12.806%
36	5.474	1376	1379	1381	rBV	371	232	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071221\
 Data File : VV021628.D
 Acq On : 12 Jul 2021 16:01
 Operator : SY/MD
 Sample : M3008-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGE71

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
 Title : VOC Analysis

37	5.497	1384	1386	1388	rBV2	238	126	0.01%	0.001%
38	5.548	1397	1402	1405	rBV4	714	683	0.04%	0.005%
39	5.616	1411	1423	1449	rBV	535307	1079611	63.61%	8.147%
40	5.908	1506	1514	1538	rVB5	9121	20376	1.20%	0.154%
41	5.989	1538	1539	1542	rBV3	449	181	0.01%	0.001%
42	6.072	1550	1565	1588	rBV	369413	760514	44.81%	5.739%
43	6.346	1649	1650	1654	rVB3	294	185	0.01%	0.001%
44	6.394	1663	1665	1669	rVB	211	94	0.01%	0.001%
45	6.442	1678	1680	1683	rVB	594	300	0.02%	0.002%
46	6.458	1683	1685	1686	rBV	259	97	0.01%	0.001%
47	6.477	1689	1691	1695	rVB2	330	126	0.01%	0.001%
48	6.497	1695	1697	1698	rBV2	344	191	0.01%	0.001%
49	6.748	1773	1775	1776	rBV	237	91	0.01%	0.001%
50	6.812	1791	1795	1798	rBV4	330	277	0.02%	0.002%
51	6.834	1800	1802	1805	rVB	450	154	0.01%	0.001%
52	6.857	1805	1809	1810	rBV2	248	149	0.01%	0.001%
53	6.873	1810	1814	1816	rBV3	307	185	0.01%	0.001%
54	6.940	1831	1835	1836	rBV3	391	244	0.01%	0.002%
55	6.989	1838	1850	1878	rVV	225471	413471	24.36%	3.120%
56	7.317	1940	1952	1969	rBV	810765	1409120	83.03%	10.633%
57	7.622	2037	2047	2080	rBV	153562	269766	15.90%	2.036%
58	7.828	2109	2111	2112	rBV2	399	151	0.01%	0.001%
59	7.879	2125	2127	2128	rBV	408	234	0.01%	0.002%
60	7.947	2140	2148	2154	rVB5	2294	3491	0.21%	0.026%
61	8.027	2166	2173	2175	rVB	432	467	0.03%	0.004%
62	8.046	2175	2179	2180	rBV	622	370	0.02%	0.003%
63	8.088	2182	2192	2226	rBV	460307	827244	48.74%	6.242%
64	8.500	2318	2320	2322	rVB2	512	239	0.01%	0.002%
65	8.532	2327	2330	2334	rBV4	663	530	0.03%	0.004%
66	8.635	2358	2362	2363	rBV	173	119	0.01%	0.001%
67	8.648	2363	2366	2370	rVB2	377	260	0.02%	0.002%
68	8.670	2371	2373	2377	rVV2	289	240	0.01%	0.002%
69	8.702	2381	2383	2386	rBV2	263	165	0.01%	0.001%
70	8.731	2390	2392	2394	rBV	446	193	0.01%	0.001%
71	8.796	2409	2412	2413	rBV	316	168	0.01%	0.001%
72	8.854	2418	2430	2463	rVV	785190	1290073	76.02%	9.735%
73	9.146	2511	2521	2534	rBV3	13443	23202	1.37%	0.175%
74	9.339	2577	2581	2582	rBV	242	139	0.01%	0.001%
75	9.394	2596	2598	2602	rBV2	445	269	0.02%	0.002%
76	9.471	2620	2622	2624	rBV	282	150	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071221\
 Data File : VV021628.D
 Acq On : 12 Jul 2021 16:01
 Operator : SY/MD
 Sample : M3008-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGE71

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
 Title : VOC Analysis

77	9.551	2638	2647	2657	rBV2	9866	16436	0.97%	0.124%
78	9.632	2669	2672	2676	rBV4	379	337	0.02%	0.003%
79	9.754	2708	2710	2713	rBV2	205	91	0.01%	0.001%
80	9.770	2713	2715	2716	rBV2	189	66	0.00%	0.000%
81	9.882	2747	2750	2753	rBV3	383	259	0.02%	0.002%
82	9.985	2781	2782	2783	rBV3	319	108	0.01%	0.001%
83	10.127	2818	2826	2837	rVB5	4693	7915	0.47%	0.060%
84	10.169	2837	2839	2841	rVB	274	110	0.01%	0.001%
85	10.217	2841	2854	2877	rBV	519256	819426	48.28%	6.183%
86	10.455	2919	2928	2948	rBV	8451	17297	1.02%	0.131%
87	10.545	2951	2956	2962	rBV6	3091	4106	0.24%	0.031%
88	10.718	3008	3010	3011	rBV2	508	230	0.01%	0.002%
89	10.744	3011	3018	3033	rVB5	4299	7096	0.42%	0.054%
90	10.918	3064	3072	3091	rVB2	21174	34286	2.02%	0.259%
91	10.995	3091	3096	3102	rBV5	488	454	0.03%	0.003%
92	11.149	3135	3144	3150	rBV6	2888	4278	0.25%	0.032%
93	11.249	3164	3175	3196	rBV	790300	1258954	74.18%	9.500%
94	11.538	3256	3265	3274	rBV3	5400	10773	0.63%	0.081%
95	11.625	3280	3292	3315	rBV	782523	1227358	72.32%	9.261%
96	12.021	3409	3415	3421	rBV4	1678	2302	0.14%	0.017%
97	12.236	3478	3482	3483	rBV	648	368	0.02%	0.003%




Sum of corrected areas: 13252264

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071221\
Data File : VV021628.D
Acq On : 12 Jul 2021 16:01
Operator : SY/MD
Sample : M3008-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGE71

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

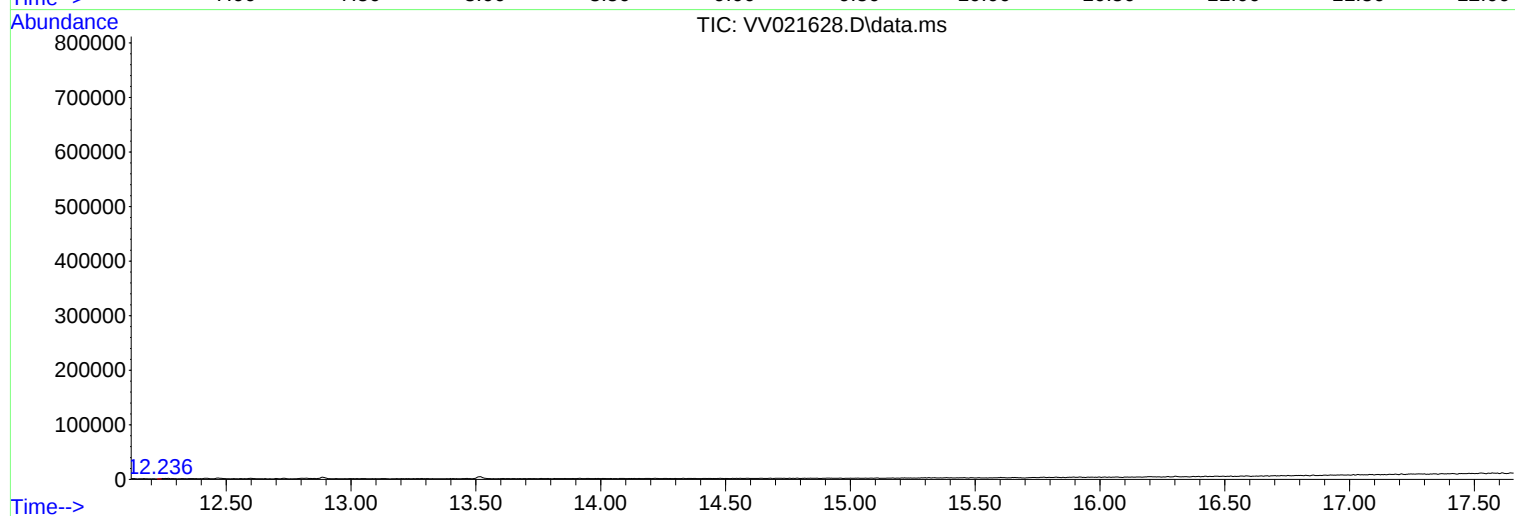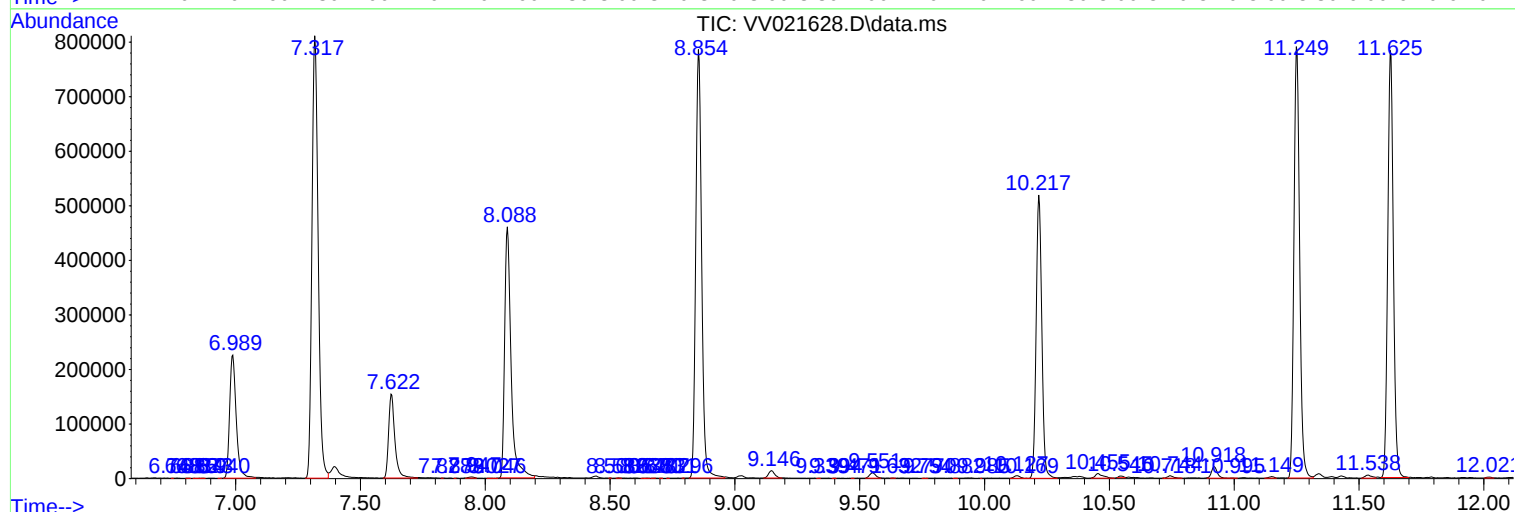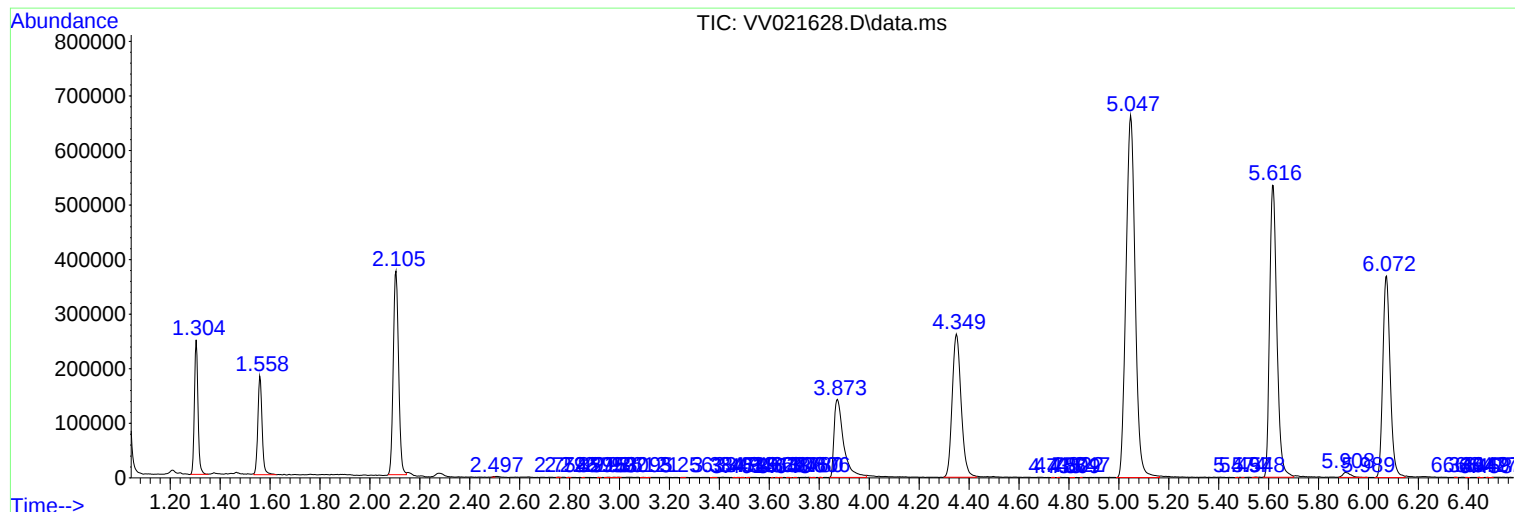

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071221\
Data File : VV021628.D
Acq On : 12 Jul 2021 16:01
Operator : SY/MD
Sample : M3008-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGE71

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071221\
Data File : VV021628.D
Acq On : 12 Jul 2021 16:01
Operator : SY/MD
Sample : M3008-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGE71

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
