

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071221\
 Data File : VV021629.D
 Acq On : 12 Jul 2021 16:25
 Operator : SY/MD
 Sample : M2959-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7H4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
 Title : VOC Analysis

Signal : TIC: VV021629.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	96	rVB	249469	242138	14.73%	1.911%
2	1.558	154	161	175	rVB	177178	202207	12.30%	1.595%
3	2.105	321	331	342	rBV	367189	530983	32.29%	4.190%
4	2.780	539	541	544	rBV2	330	205	0.01%	0.002%
5	2.815	549	552	557	rVB2	486	403	0.02%	0.003%
6	2.841	557	560	562	rBV2	237	107	0.01%	0.001%
7	2.857	563	565	569	rVV3	494	281	0.02%	0.002%
8	2.892	573	576	577	rBV	282	118	0.01%	0.001%
9	3.098	638	640	642	rBV3	280	121	0.01%	0.001%
10	3.111	642	644	646	rBV2	222	105	0.01%	0.001%
11	3.172	659	663	665	rBV3	534	318	0.02%	0.003%
12	3.220	674	678	680	rBV3	867	633	0.04%	0.005%
13	3.356	718	720	723	rVB2	414	141	0.01%	0.001%
14	3.410	735	737	740	rBV	211	136	0.01%	0.001%
15	3.426	740	742	744	rVV2	462	169	0.01%	0.001%
16	3.455	748	751	754	rBV2	401	209	0.01%	0.002%
17	3.468	754	755	758	rVB	236	87	0.01%	0.001%
18	3.494	758	763	764	rBV	423	249	0.02%	0.002%
19	3.529	772	774	777	rBV2	246	134	0.01%	0.001%
20	3.561	782	784	785	rBV	189	82	0.00%	0.001%
21	3.587	791	792	793	rBV	158	43	0.00%	0.000%
22	3.735	834	838	843	rVB3	503	420	0.03%	0.003%
23	3.761	843	846	847	rBV2	391	251	0.02%	0.002%
24	3.815	860	863	865	rBV2	326	212	0.01%	0.002%
25	3.873	871	881	920	rBV	138428	366491	22.29%	2.892%
26	4.278	1005	1007	1008	rBV	434	206	0.01%	0.002%
27	4.349	1012	1029	1054	rBV	254999	637398	38.76%	5.029%
28	4.738	1146	1150	1152	rBV2	244	162	0.01%	0.001%
29	4.754	1153	1155	1156	rBV2	213	63	0.00%	0.000%
30	4.764	1156	1158	1159	rBV2	329	148	0.01%	0.001%
31	4.799	1167	1169	1174	rVB2	393	298	0.02%	0.002%
32	4.828	1177	1178	1179	rBV2	210	48	0.00%	0.000%
33	4.841	1180	1182	1185	rBV2	284	187	0.01%	0.001%
34	4.876	1190	1193	1198	rVV4	367	253	0.02%	0.002%
35	4.908	1201	1203	1207	rVB2	687	470	0.03%	0.004%
36	4.931	1207	1210	1216	rBV2	384	455	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071221\
 Data File : VV021629.D
 Acq On : 12 Jul 2021 16:25
 Operator : SY/MD
 Sample : M2959-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7H4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
 Title : VOC Analysis

37	4.986	1225	1227	1228	rBV	307	163	0.01%	0.001%
38	5.047	1228	1246	1275	rVV2	642496	1644288	100.00%	12.974%
39	5.343	1333	1338	1339	rBV2	556	449	0.03%	0.004%
40	5.404	1354	1357	1358	rBV	629	392	0.02%	0.003%
41	5.481	1380	1381	1382	rBV	444	114	0.01%	0.001%
42	5.542	1398	1400	1403	rBV4	591	276	0.02%	0.002%
43	5.616	1410	1423	1448	rBV	509659	1022202	62.17%	8.065%
44	5.908	1503	1514	1529	rBV2	15512	32275	1.96%	0.255%
45	6.069	1551	1564	1590	rBV	358708	736792	44.81%	5.813%
46	6.343	1647	1649	1652	rVB3	575	216	0.01%	0.002%
47	6.429	1669	1676	1679	rBV3	385	421	0.03%	0.003%
48	6.458	1684	1685	1686	rBV	142	33	0.00%	0.000%
49	6.471	1687	1689	1692	rBV	330	192	0.01%	0.002%
50	6.510	1697	1701	1703	rBV2	494	299	0.02%	0.002%
51	6.629	1735	1738	1739	rBV	446	235	0.01%	0.002%
52	6.706	1760	1762	1765	rVB2	434	249	0.02%	0.002%
53	6.773	1779	1783	1788	rVB2	400	304	0.02%	0.002%
54	6.806	1788	1793	1795	rBV2	326	326	0.02%	0.003%
55	6.844	1802	1805	1807	rBV2	408	236	0.01%	0.002%
56	6.896	1819	1821	1822	rVB	233	63	0.00%	0.000%
57	6.905	1822	1824	1827	rVB2	298	111	0.01%	0.001%
58	6.924	1827	1830	1832	rBV2	321	222	0.01%	0.002%
59	6.941	1833	1835	1838	rBV2	338	183	0.01%	0.001%
60	6.989	1838	1850	1871	rBV	218921	399756	24.31%	3.154%
61	7.317	1940	1952	1971	rBV	794211	1373408	83.53%	10.837%
62	7.622	2038	2047	2071	rBV	149043	257999	15.69%	2.036%
63	7.870	2121	2124	2130	rBV5	637	624	0.04%	0.005%
64	7.921	2134	2140	2141	rBV3	429	377	0.02%	0.003%
65	8.043	2175	2178	2180	rBV2	306	202	0.01%	0.002%
66	8.088	2182	2192	2236	rVV	436213	809215	49.21%	6.385%
67	8.436	2299	2300	2301	rBV	261	87	0.01%	0.001%
68	8.468	2308	2310	2315	rVB4	490	319	0.02%	0.003%
69	8.622	2354	2358	2361	rBV3	676	607	0.04%	0.005%
70	8.764	2399	2402	2408	rBV2	258	231	0.01%	0.002%
71	8.854	2417	2430	2456	rBV	746771	1214111	73.84%	9.580%
72	9.043	2487	2489	2495	rVB5	874	855	0.05%	0.007%
73	9.420	2605	2606	2608	rBV2	259	119	0.01%	0.001%
74	9.477	2622	2624	2626	rBV	298	196	0.01%	0.002%
75	9.510	2631	2634	2635	rBV	334	182	0.01%	0.001%
76	9.645	2674	2676	2677	rBV	255	122	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071221\
 Data File : VV021629.D
 Acq On : 12 Jul 2021 16:25
 Operator : SY/MD
 Sample : M2959-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7H4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M

Title : VOC Analysis

77	9.731	2699	2703	2704	rBV2	496	276	0.02%	0.002%
78	9.751	2707	2709	2713	rBV2	404	254	0.02%	0.002%
79	9.789	2717	2721	2725	rBV2	574	515	0.03%	0.004%
80	9.809	2725	2727	2728	rBV	427	190	0.01%	0.001%
81	9.857	2740	2742	2746	rVB3	405	250	0.02%	0.002%
82	10.127	2819	2826	2842	rVB4	4874	7840	0.48%	0.062%
83	10.217	2842	2854	2875	rBV	491918	775745	47.18%	6.121%
84	10.918	3067	3072	3077	rBV5	4496	5989	0.36%	0.047%
85	11.153	3135	3145	3159	rBV7	3562	6993	0.43%	0.055%
86	11.249	3164	3175	3204	rBV	760039	1193181	72.57%	9.415%
87	11.542	3261	3266	3268	rBV3	781	612	0.04%	0.005%
88	11.625	3281	3292	3313	rBV	762022	1192993	72.55%	9.413%
89	11.973	3396	3400	3402	rBV3	574	466	0.03%	0.004%
90	12.355	3513	3519	3526	rBV5	3045	4147	0.25%	0.033%




Sum of corrected areas: 12673833

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071221\
Data File : VV021629.D
Acq On : 12 Jul 2021 16:25
Operator : SY/MD
Sample : M2959-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7H4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

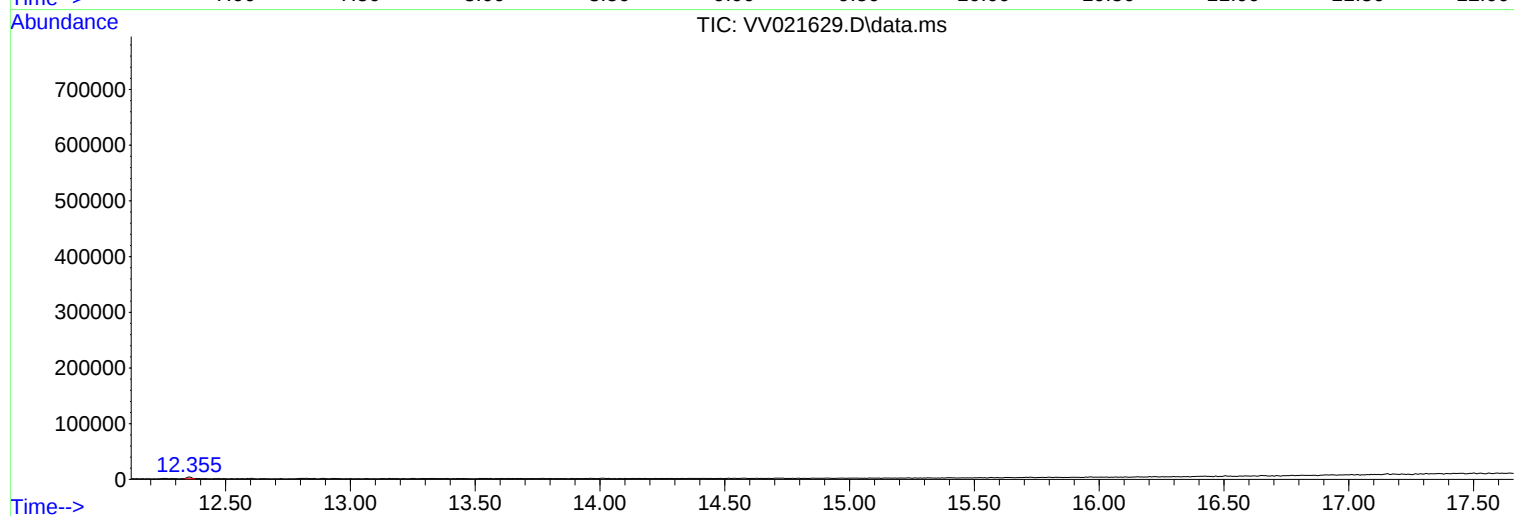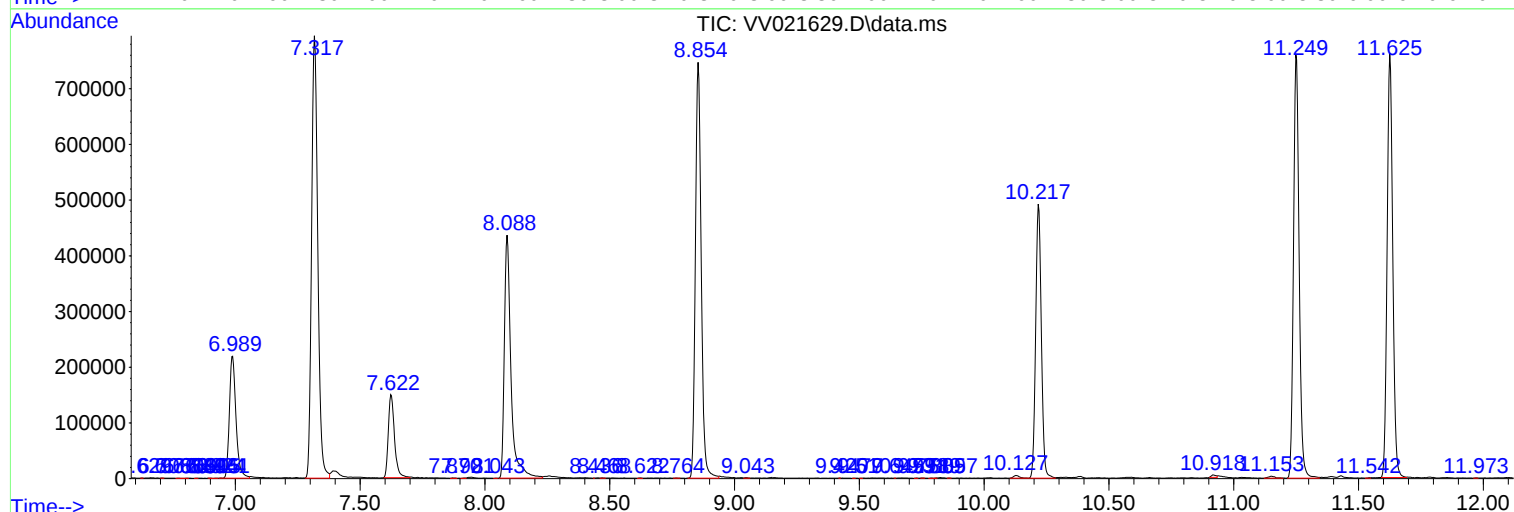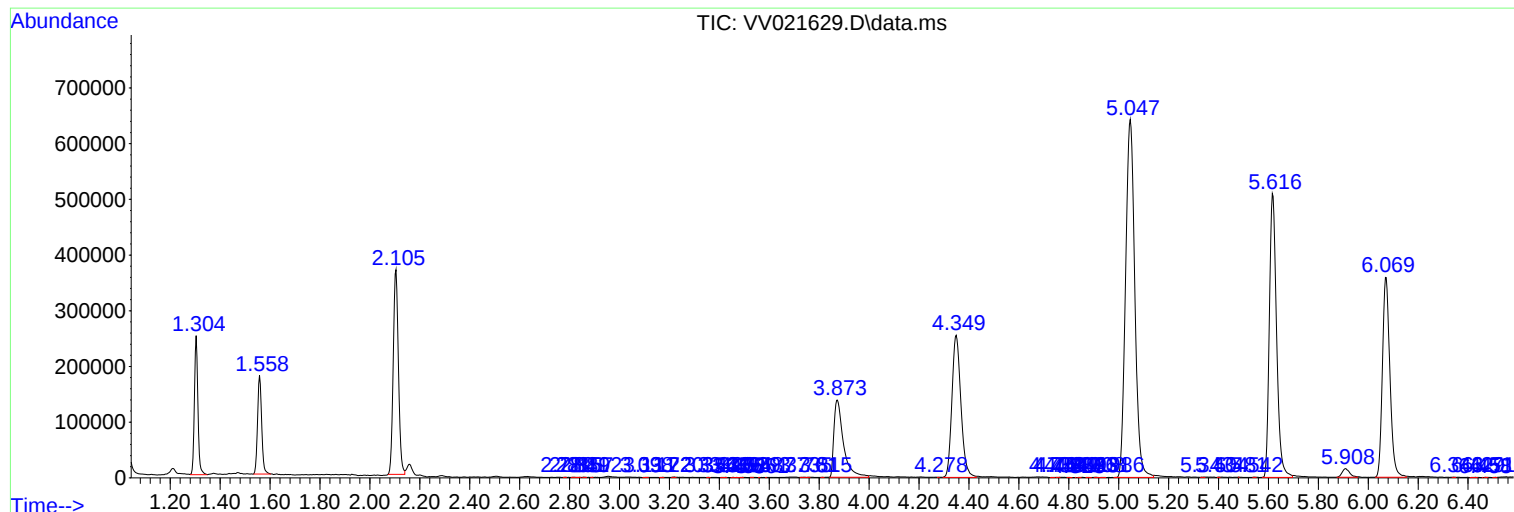

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071221\
Data File : VV021629.D
Acq On : 12 Jul 2021 16:25
Operator : SY/MD
Sample : M2959-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7H4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071221\
Data File : VV021629.D
Acq On : 12 Jul 2021 16:25
Operator : SY/MD
Sample : M2959-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7H4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
