
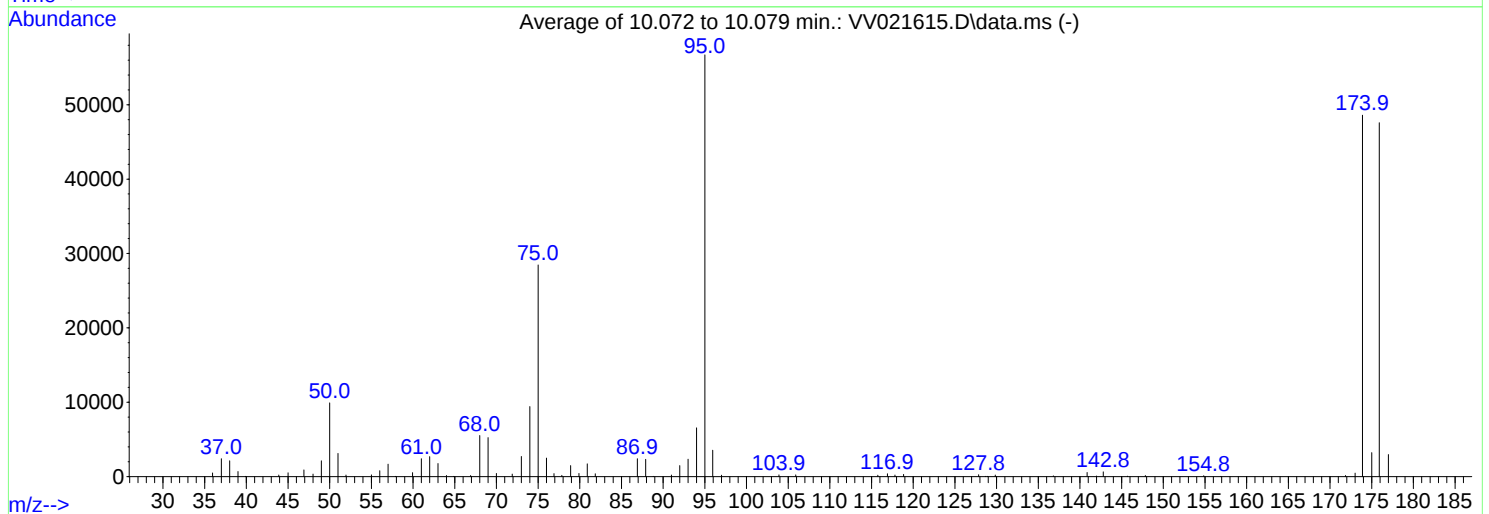


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071221\
 Data File : VV021615.D
 Acq On : 12 Jul 2021 08:57
 Operator : SY/MD
 Sample : BFB203
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB203

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
 Title : VOC Analysis
 Last Update : Tue Jul 13 01:14:23 2021

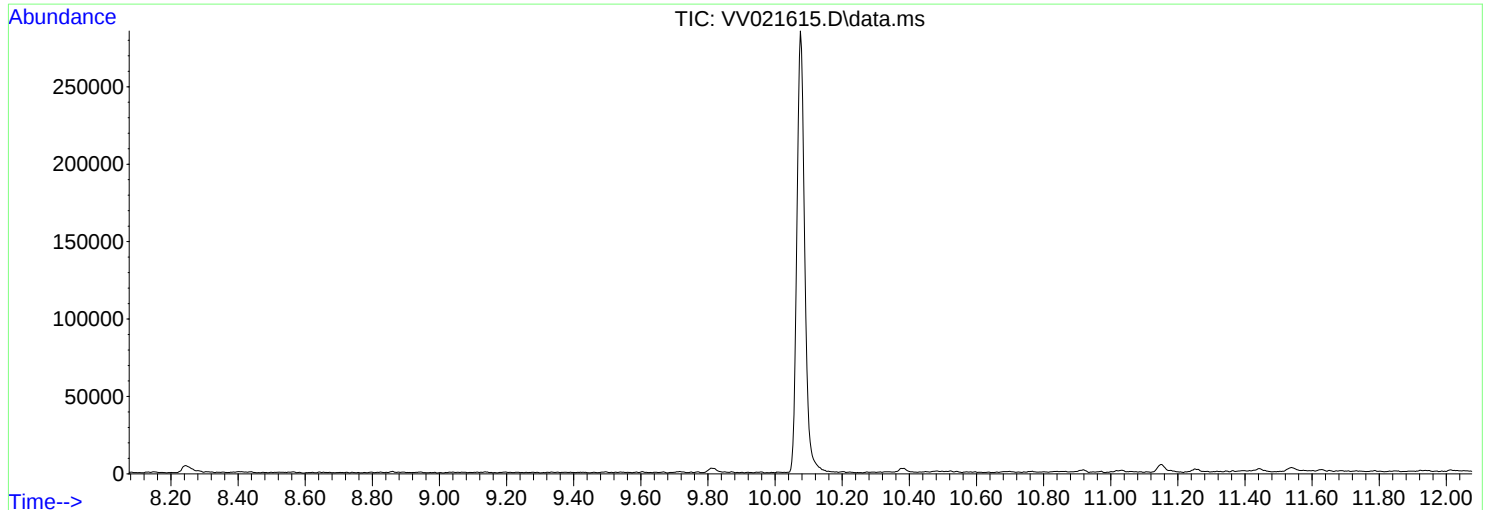

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2798

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	9913	PASS
75	95	30	80	50.2	28461	PASS
95	95	100	100	100.0	56707	PASS
96	95	5	9	6.3	3547	PASS
173	174	0.00	2	1.0	481	PASS
174	95	50	120	85.7	48597	PASS
175	174	5	9	6.7	3234	PASS
176	174	95	105	97.9	47576	PASS
177	176	5	10	6.3	2976	PASS

m/z	Abundance
36.00	509.0
37.00	2500.0
38.00	2239.0
39.00	848.0
39.90	208.0
40.90	103.0
44.00	705.0
45.00	523.0
46.90	957.0
48.00	353.0
49.00	2185.0
50.00	10280.0
51.00	3200.0
52.00	227.0
55.00	219.0
56.00	819.0
57.00	1759.0
60.00	576.0
61.00	2467.0
62.00	2790.0
63.00	1808.0
64.00	148.0
64.90	106.0
66.90	163.0
68.00	5749.0
69.00	5466.0
70.00	419.0
71.90	359.0
73.00	2845.0
74.00	9749.0
75.00	29288.0
76.00	2534.0
76.90	429.0
77.90	161.0
78.90	1536.0
79.90	427.0
80.90	1791.0
81.80	410.0
86.90	2514.0
87.90	2414.0
91.00	223.0
92.00	1523.0
93.00	2448.0
94.00	6819.0
95.00	58464.0
96.00	3705.0
97.00	191.0
103.90	253.0
105.90	242.0
115.80	203.0
116.90	399.0
117.80	226.0
118.90	324.0
127.80	284.0
128.90	119.0
129.90	210.0
136.80	106.0
140.80	585.0
142.00	123.0
142.80	684.0
145.70	118.0
147.90	164.0
154.80	127.0
171.80	153.0
173.00	502.0
173.90	50304.0
175.00	3306.0
175.90	49352.0
177.00	3075.0

Instrument :
MSVOA_V
ClientSampleId :
BFB203

m/z	Abundance
36.00	487.0
37.00	2392.0
38.00	2070.0
39.00	801.0
40.00	245.0
44.00	654.0
45.00	441.0
46.90	818.0
48.00	297.0
49.00	2210.0
50.00	9677.0
51.00	3004.0
51.90	226.0
55.00	228.0
56.00	734.0
57.00	1606.0
59.90	515.0
61.00	2319.0
62.00	2627.0
63.00	1755.0
64.10	162.0
67.00	138.0
68.00	5549.0
69.00	5139.0
70.00	376.0
71.90	337.0
73.00	2699.0
74.00	9346.0
75.00	27784.0
76.00	2474.0
76.90	400.0
77.80	153.0
78.90	1481.0
79.90	430.0
80.90	1570.0
81.90	372.0
86.90	2429.0
87.90	2149.0
91.00	196.0
92.00	1375.0
93.00	2321.0
94.00	6300.0
95.00	56736.0
96.00	3515.0
97.00	155.0
103.90	266.0
105.90	252.0
115.80	220.0
116.90	370.0
117.80	231.0
118.90	282.0
127.90	260.0
129.70	190.0
136.80	112.0
140.80	584.0
142.80	652.0
147.80	156.0
154.90	117.0
171.90	163.0
173.00	561.0
173.90	49136.0
175.00	3170.0
175.90	48152.0
177.00	2901.0

Instrument :
MSVOA_V
ClientSampleId :
BFB203

m/z	Abundance
39.00	113.0
39.90	186.0
41.10	146.0
43.90	452.0
95.90	100.0

Instrument :
MSVOA_V
ClientSampleId :
BFB203

m/z	Abundance
35.90	496.0
37.00	2338.0
38.00	2093.0
39.00	774.0
39.80	228.0
40.90	122.0
43.90	662.0
45.00	564.0
46.90	906.0
48.00	409.0
49.00	2000.0
50.00	9783.0
51.00	3127.0
52.00	222.0
55.00	246.0
56.00	805.0
57.00	1685.0
57.90	103.0
60.00	547.0
61.00	2444.0
62.00	2632.0
63.00	1712.0
63.90	175.0
66.80	169.0
68.00	5287.0
69.00	5131.0
70.00	473.0
71.90	361.0
73.00	2583.0
74.00	9194.0
75.00	28312.0
76.00	2472.0
76.90	398.0
77.80	185.0
78.90	1450.0
79.90	454.0
80.90	1795.0
81.80	385.0
86.90	2259.0
87.90	2420.0
88.80	155.0
91.00	261.0
92.00	1550.0
93.00	2240.0
94.00	6548.0
95.00	54920.0
96.00	3721.0
97.00	206.0
103.90	199.0
105.90	214.0
115.70	188.0
116.90	399.0
117.80	222.0
118.80	329.0
127.80	259.0
128.70	101.0
129.90	250.0
136.80	104.0
140.90	519.0
142.00	141.0
142.80	629.0
145.70	105.0
147.90	168.0
154.80	141.0
156.90	102.0
171.80	119.0
173.00	379.0
173.90	46352.0
175.00	3226.0
175.90	45224.0
177.00	2953.0

Instrument :
MSVOA_V
ClientSampleId :
BFB203