


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071223\
Data File : VV031684.D
Acq On : 12 Jul 2023 10:23
Operator : SY/MD
Sample : BFB397
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB397

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM071123WMA.M
Title : VOC Analysis
Last Update : Thu Jul 13 04:58:07 2023

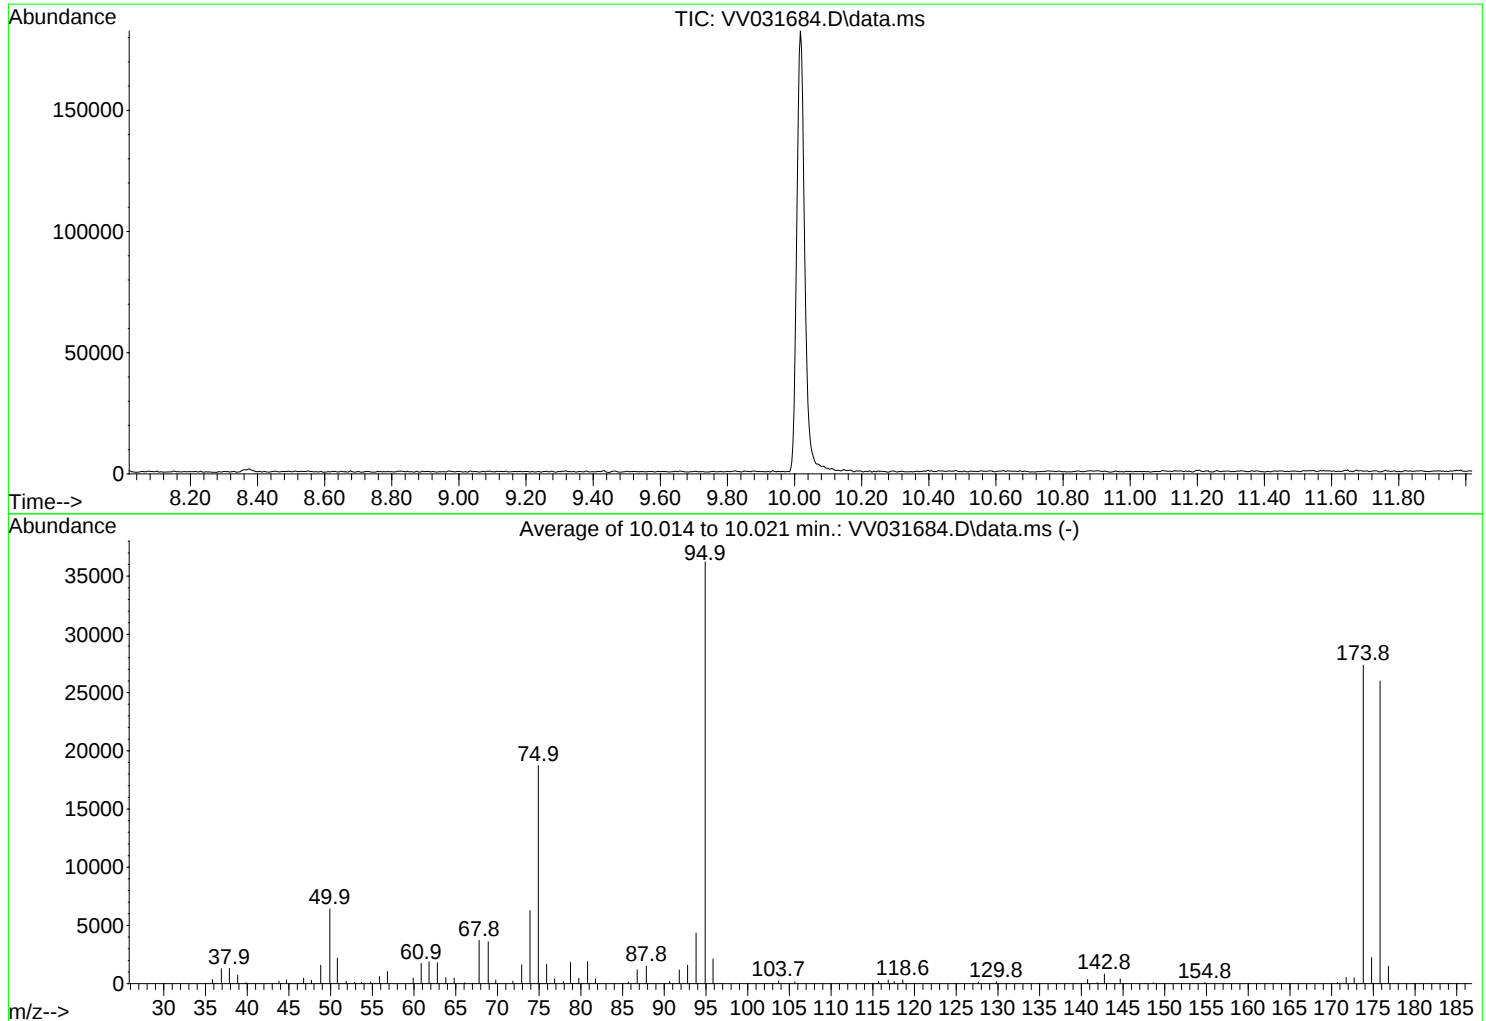

AutoFind: Scans 2791, 2792, 2793; Background Corrected with Scan 2781

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	6414	PASS
75	95	30	80	51.7	18720	PASS
95	95	100	100	100.0	36229	PASS
96	95	5	9	5.8	2116	PASS
173	174	0.00	2	1.8	494	PASS
174	95	50	120	75.5	27360	PASS
175	174	5	9	8.2	2236	PASS
176	174	95	105	95.0	25995	PASS
177	176	5	10	5.8	1504	PASS

m/z	Abundance
37.10	104.0
39.80	252.0
43.80	629.0

Instrument :
MSVOA_V
ClientSampleId :
BFB397

m/z	Abundance
35.80	357.0
36.90	1463.0
37.90	1324.0
38.90	819.0
39.90	313.0
43.80	865.0
44.70	391.0
46.70	441.0
47.70	252.0
48.80	1656.0
49.90	6304.0
50.80	2134.0
51.80	226.0
52.80	105.0
53.70	109.0
54.70	168.0
55.80	596.0
56.80	1099.0
59.90	472.0
60.90	1685.0
61.80	1871.0
62.80	1698.0
63.80	525.0
64.80	427.0
67.80	3622.0
68.90	3691.0
69.80	282.0
71.80	271.0
72.90	1611.0
73.90	6382.0
74.90	18232.0
75.90	1716.0
76.90	440.0
77.90	160.0
78.70	1807.0
79.70	448.0
80.80	1828.0
81.70	396.0
85.70	135.0
86.70	1076.0
87.80	1577.0
90.70	195.0
91.80	1182.0
92.80	1587.0
93.80	4375.0
94.90	35328.0
95.80	2225.0
96.70	105.0
103.70	201.0
105.60	167.0
115.70	151.0
116.80	301.0
117.60	182.0
118.60	320.0
127.60	136.0
129.80	155.0
140.80	379.0
141.90	145.0
142.80	858.0
144.70	390.0
148.60	100.0
154.80	183.0
171.70	469.0
172.70	468.0
173.80	25984.0
174.80	2211.0
175.80	24936.0
176.80	1502.0

Instrument :
MSVOA_V
ClientSampleId :
BFB397

m/z	Abundance
35.90	338.0
36.90	1402.0
37.80	1353.0
38.80	760.0
39.90	354.0
43.80	856.0
44.70	310.0
46.80	453.0
47.70	283.0
48.80	1641.0
49.90	6622.0
50.80	2265.0
51.80	207.0
52.90	116.0
53.70	127.0
54.80	162.0
55.90	646.0
56.80	1088.0
59.90	499.0
60.90	1771.0
61.80	1964.0
62.80	1874.0
63.80	551.0
64.80	479.0
66.10	113.0
67.80	3870.0
68.90	3734.0
69.80	306.0
71.80	221.0
72.90	1656.0
73.90	6468.0
74.90	19192.0
75.90	1718.0
76.80	427.0
77.90	177.0
78.70	1849.0
79.70	487.0
80.80	1988.0
81.80	431.0
85.70	150.0
86.70	1209.0
87.80	1549.0
90.70	194.0
91.80	1227.0
92.80	1589.0
93.80	4446.0
94.90	37352.0
95.80	2149.0
103.70	251.0
105.70	159.0
115.70	191.0
116.80	320.0
117.50	200.0
118.60	350.0
127.60	147.0
129.80	209.0
140.80	366.0
141.90	116.0
142.80	862.0
144.70	423.0
148.60	112.0
154.80	144.0
170.70	135.0
171.80	557.0
172.70	521.0
173.80	28384.0
174.80	2282.0
175.80	26832.0
176.80	1523.0

Instrument :
MSVOA_V
ClientSampleId :
BFB397

m/z	Abundance
35.90	328.0
36.90	1294.0
37.80	1238.0
38.80	647.0
39.90	342.0
43.80	836.0
44.80	232.0
46.80	514.0
47.70	333.0
48.80	1446.0
49.90	6315.0
50.80	2214.0
51.90	217.0
52.90	121.0
53.70	106.0
54.90	137.0
55.90	611.0
56.80	950.0
59.90	474.0
60.80	1726.0
61.80	1821.0
62.80	1819.0
63.80	485.0
64.80	524.0
66.00	112.0
67.80	3628.0
68.90	3369.0
69.80	313.0
71.90	176.0
72.90	1540.0
73.90	6003.0
74.90	18736.0
75.90	1524.0
76.80	385.0
77.90	156.0
78.80	1774.0
79.80	452.0
80.80	1884.0
81.80	407.0
85.70	136.0
86.80	1323.0
87.90	1430.0
90.60	200.0
91.80	1146.0
92.80	1551.0
93.80	4226.0
94.90	36008.0
95.90	1975.0
103.70	258.0
105.70	193.0
115.70	221.0
116.90	325.0
117.50	173.0
118.60	293.0
127.70	144.0
129.80	172.0
140.70	336.0
142.70	757.0
144.60	372.0
147.70	115.0
170.70	158.0
171.80	585.0
172.70	493.0
173.80	27712.0
174.80	2214.0
175.80	26216.0
176.80	1488.0

Instrument :
MSVOA_V
ClientSampleId :
BFB397